

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007605.D
 Acq On : 23 Oct 2021 00:18
 Operator : CG/JU
 Sample : M4281-11
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY67

Quant Time: Oct 23 00:46:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	217497	20.000	ng/u1	0.00
20) Naphthalene-d8	10.751	136	886254	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.580	164	581096	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.333	188	1246484	20.000	ng/u1	0.00
79) Chrysene-d12	21.421	240	1292398	20.000	ng/u1	0.00
88) Perylene-d12	23.862	264	1332585	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	22156	4.023	ng/uL	0.00
4) Pyridine-d5	3.810	84	21445	1.423	ng/u1	0.02
7) Phenol-d5	7.104	99	104922	6.177	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	237925	23.486	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.475	132	262575	19.651	ng/u1	0.00
15) 4-Methylphenol-d8	8.651	113	187257	14.313	ng/u1	0.00
21) Nitrobenzene-d5	9.098	128	162031	28.890	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.828	143	159637	30.472	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	313441	24.530	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	34428	1.992	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	1164370	28.963	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1281089	25.356	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	41697	6.464	ng/u1	0.00
60) Fluorene-d10	15.575	176	976399	29.022	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	76844	15.385	ng/u1	0.00
73) Anthracene-d10	17.433	188	1604570	30.311	ng/u1	0.00
81) Pyrene-d10	19.663	212	1942177	30.060	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.704	264	1948933	29.393	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.410	88	70870	11.831	ng/uL	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007605.D
Acq On : 23 Oct 2021 00:18
Operator : CG/JU
Sample : M4281-11
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY67

Quant Time: Oct 23 00:46:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

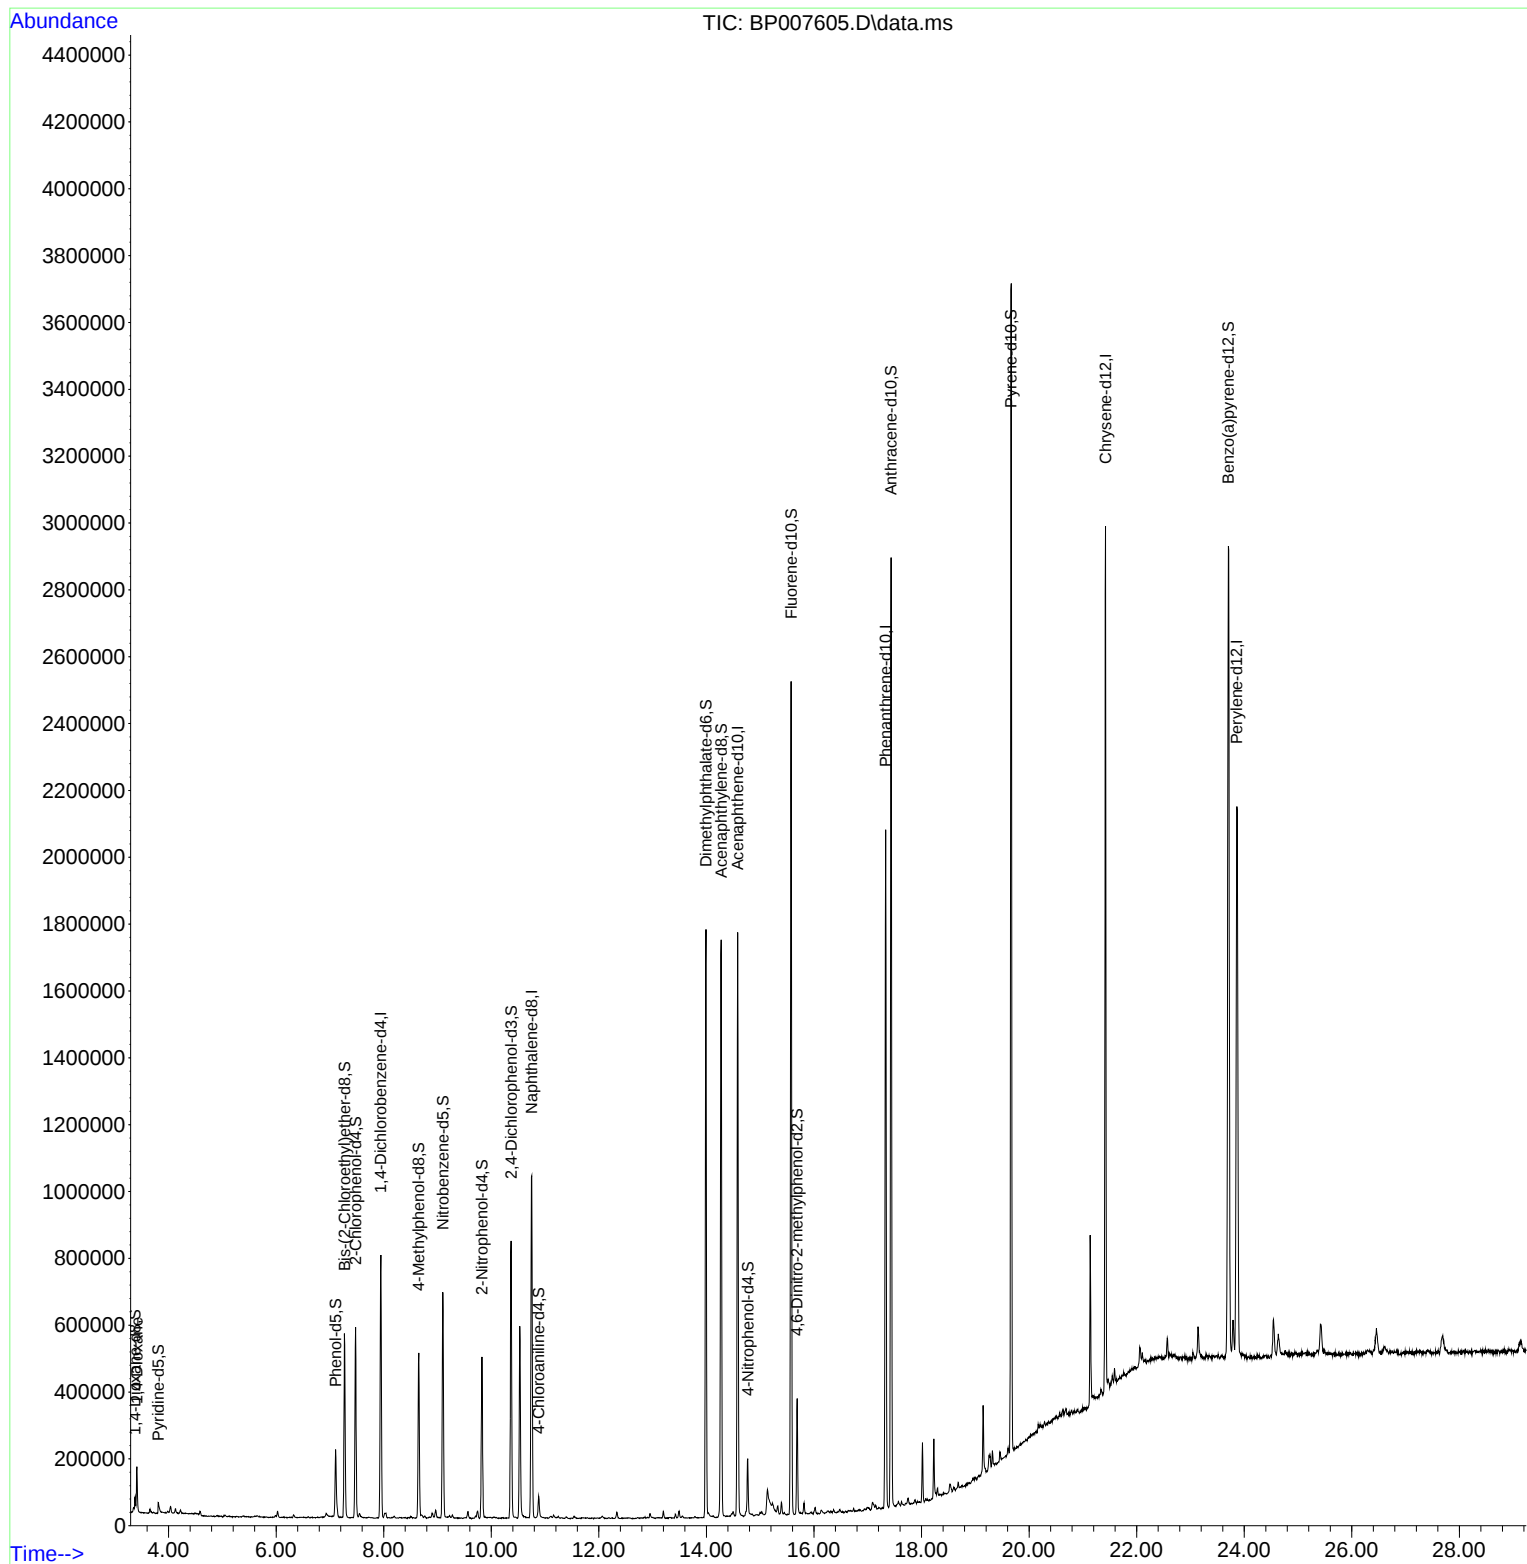

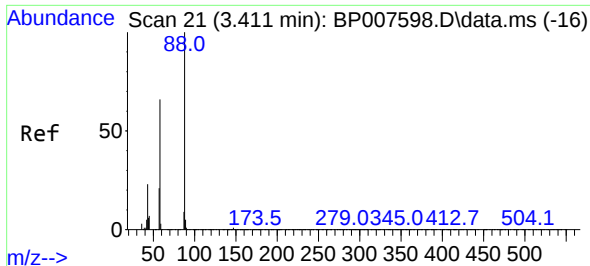

#2
1,4-Dioxane
Concen: 11.831 ng/uL
RT: 3.410 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP007605.D
Acq: 23 Oct 2021 00:18

Instrument :
BNA_P
ClientSampleId :
BFY67

Tgt Ion: 88 Resp: 70870
Ion Ratio Lower Upper
88 100
43 26.8 24.2 36.2
58 72.9 62.5 93.7

