

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007606.D
 Acq On : 23 Oct 2021 00:52
 Operator : CG/JU
 Sample : M4281-02
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY58

Quant Time: Oct 23 01:47:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	220516	20.000	ng/u1	0.00
20) Naphthalene-d8	10.752	136	914760	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	599034	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.334	188	1280027	20.000	ng/u1	0.00
79) Chrysene-d12	21.422	240	1344781	20.000	ng/u1	0.00
88) Perylene-d12	23.863	264	1376159	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	22994	4.118	ng/uL	0.00
4) Pyridine-d5	3.793	84	114458	7.489	ng/u1	0.00
7) Phenol-d5	7.105	99	130938	7.603	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	314898	30.658	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.475	132	354602	26.174	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	241395	18.198	ng/u1	0.00
21) Nitrobenzene-d5	9.099	128	219683	37.948	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.828	143	226260	41.843	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	412903	31.307	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	525760	29.479	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	1412736	34.088	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1670643	32.076	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	47410	7.129	ng/u1	0.00
60) Fluorene-d10	15.575	176	1228134	35.411	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	88716	17.297	ng/u1	0.00
73) Anthracene-d10	17.433	188	2107150	38.762	ng/u1	0.00
81) Pyrene-d10	19.663	212	2524969	37.558	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	2534368	37.012	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.411	88	1383730	227.836	ng/uL 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007606.D
Acq On : 23 Oct 2021 00:52
Operator : CG/JU
Sample : M4281-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY58

Quant Time: Oct 23 01:47:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

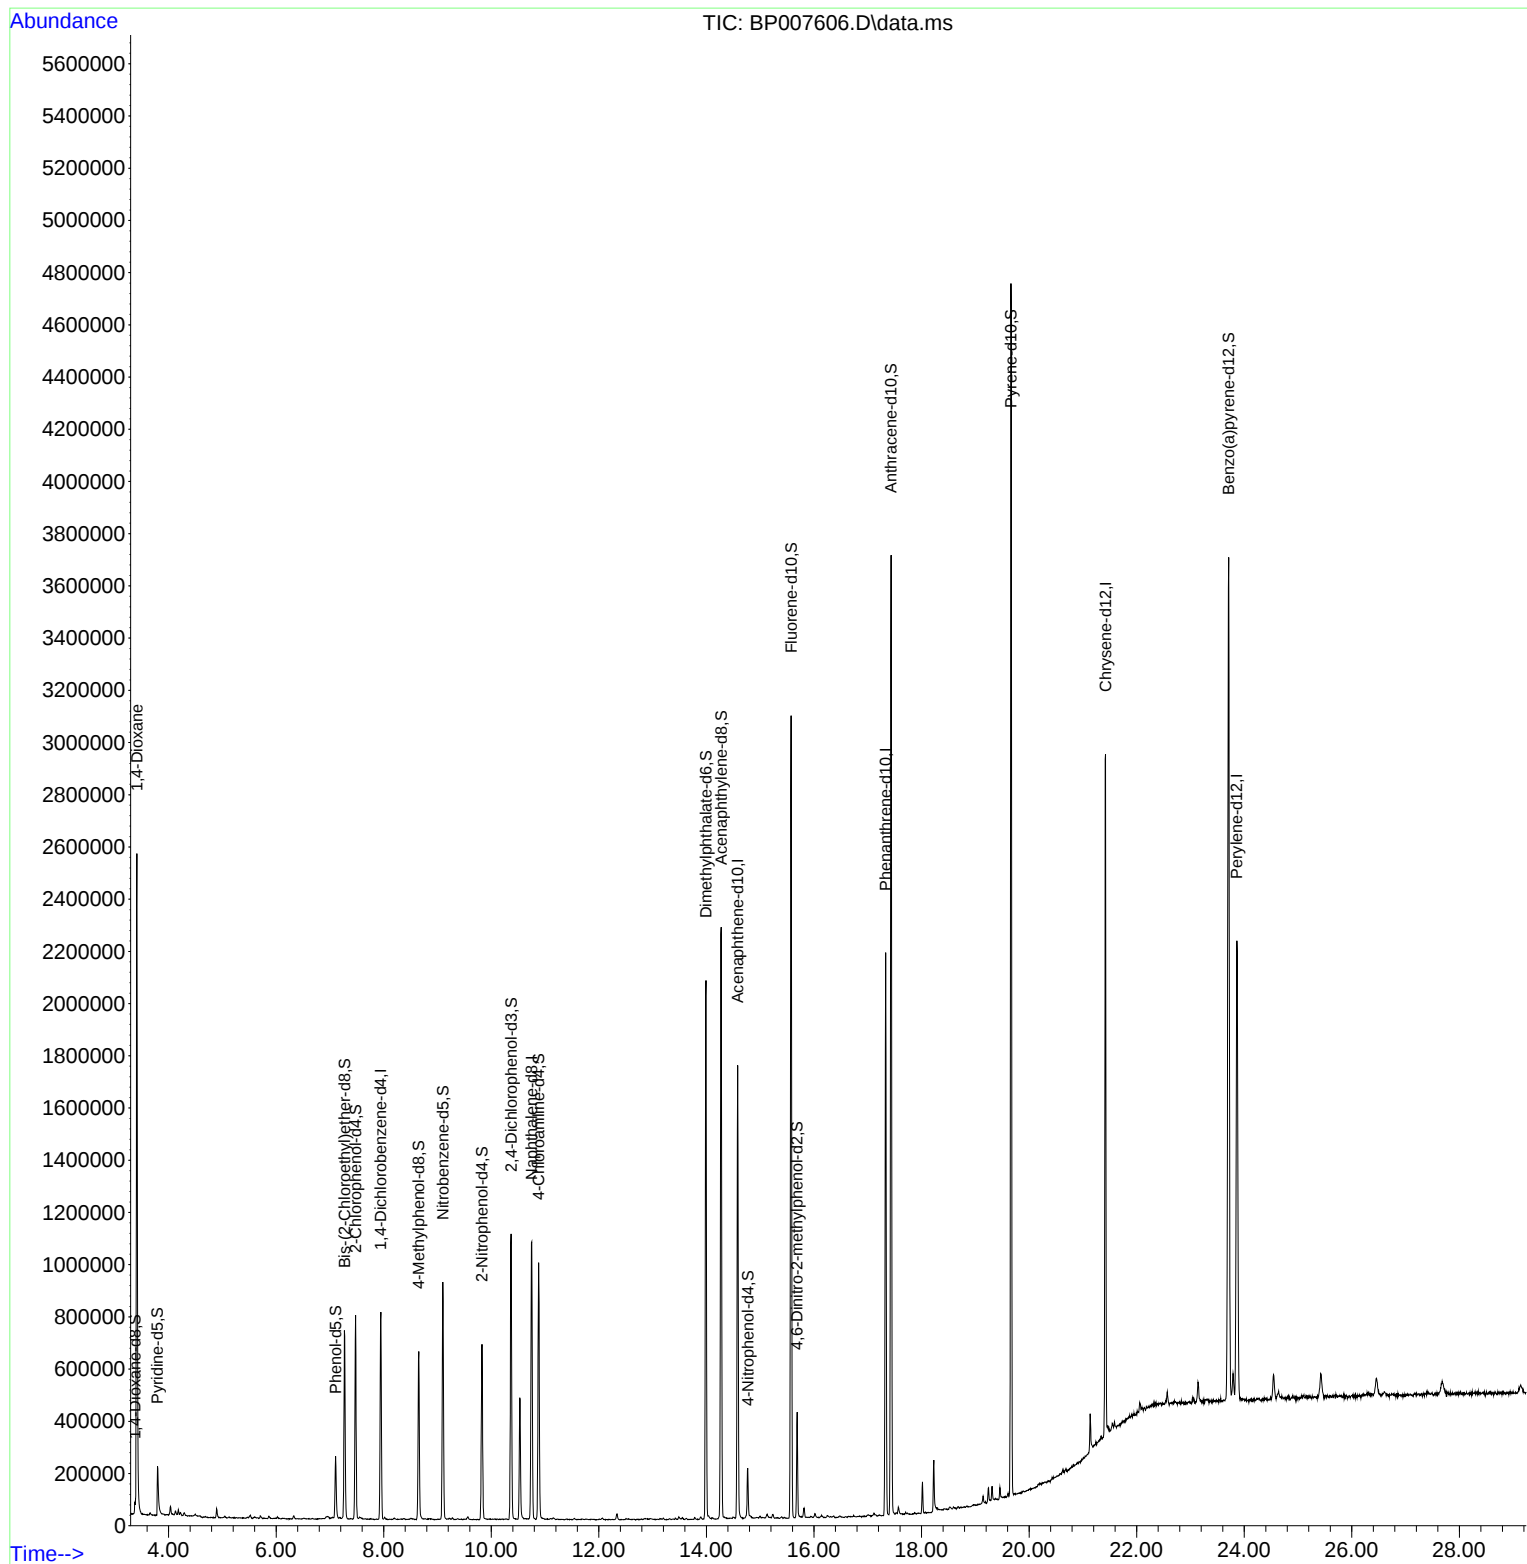

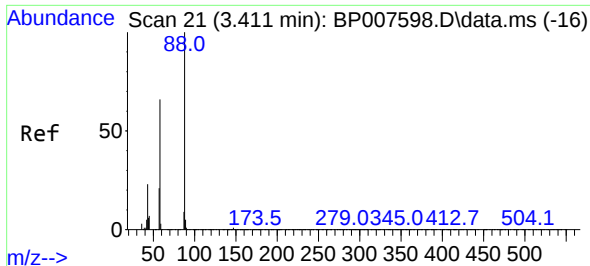

#2
 1,4-Dioxane
 Concen: 227.836 ng/uL
 RT: 3.411 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP007606.D
 Acq: 23 Oct 2021 00:52

Instrument :
 BNA_P
 ClientSampleId :
 BFY58

Tgt Ion: 88 Resp: 1383730

Ion	Ratio	Lower	Upper
88	100		
43	25.4	24.2	36.2
58	67.1	62.5	93.7

