

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007626.D
 Acq On : 23 Oct 2021 12:43
 Operator : CG/JU
 Sample : M4262-13
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFYA4

Quant Time: Oct 25 01:02:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	201402	20.000	ng/u1	0.00
20) Naphthalene-d8	10.752	136	825512	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	551428	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.334	188	1189803	20.000	ng/u1	0.00
79) Chrysene-d12	21.422	240	1274827	20.000	ng/u1	0.00
88) Perylene-d12	23.869	264	1320640	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	23615	4.631	ng/uL	0.00
4) Pyridine-d5	3.799	84	126357	9.052	ng/u1	0.00
7) Phenol-d5	7.111	99	139872	8.893	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	330566	35.238	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.475	132	386906	31.269	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	265513	21.916	ng/u1	0.00
21) Nitrobenzene-d5	9.099	128	243514	46.613	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.828	143	269305	55.188	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	480014	40.330	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	524405	32.582	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	1544814	40.493	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1870957	39.023	ng/u1	0.00
54) 4-Nitrophenol-d4	14.775	143	59351	9.696	ng/u1	0.00
60) Fluorene-d10	15.575	176	1344897	42.125	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	172996	36.287	ng/u1	0.00
73) Anthracene-d10	17.434	188	2291386	45.348	ng/u1	0.00
81) Pyrene-d10	19.669	212	2805526	44.022	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	2924770	44.509	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.411	88	91723	16.536	ng/uL	92
18) 4-Methylphenol	8.711	108	18711	1.450	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007626.D
Acq On : 23 Oct 2021 12:43
Operator : CG/JU
Sample : M4262-13
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFYA4

Quant Time: Oct 25 01:02:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration




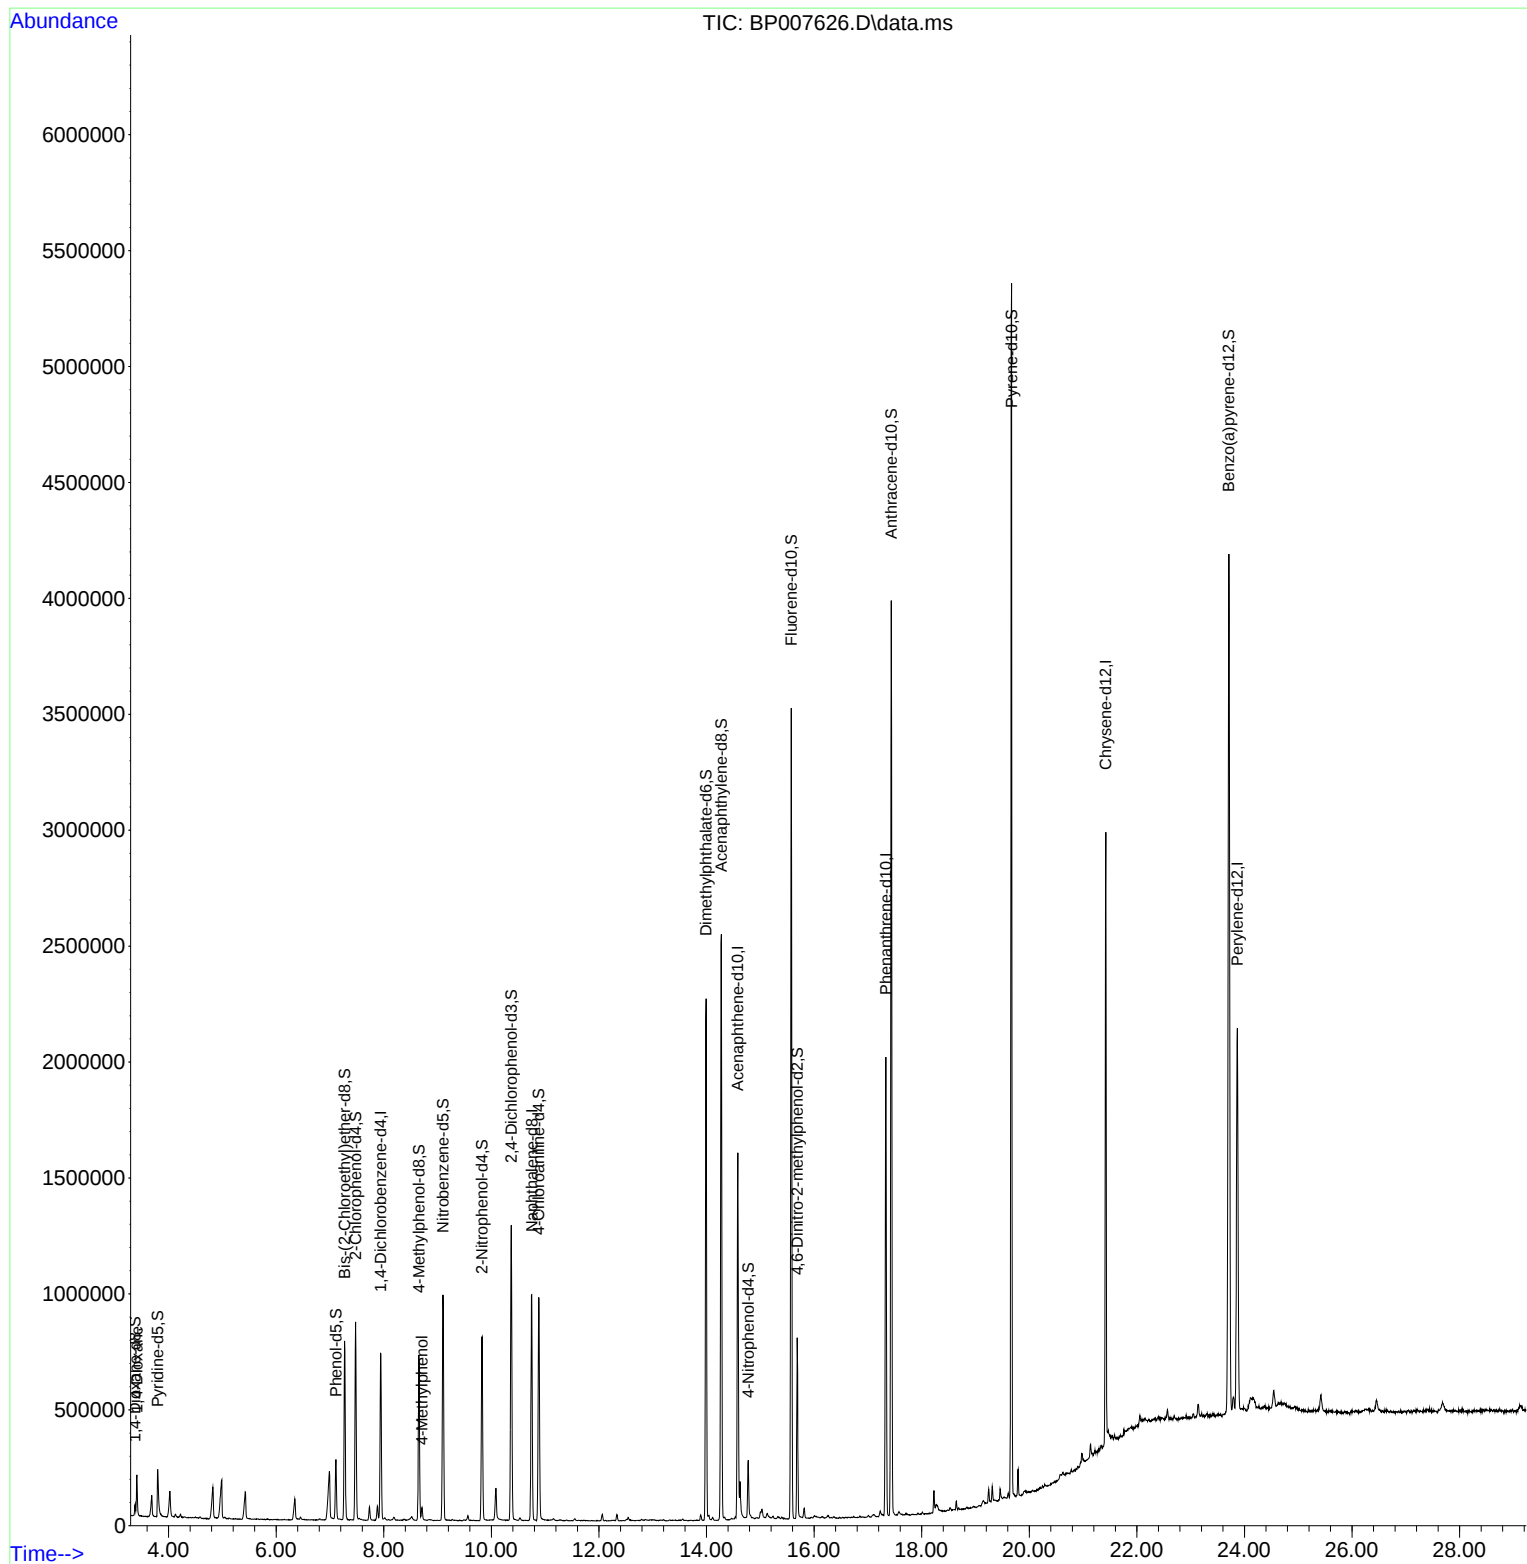


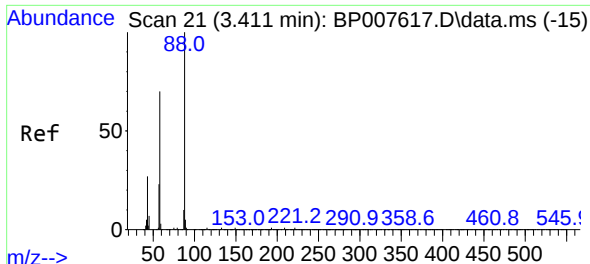

#2
1,4-Dioxane
Concen: 16.536 ng/uL
RT: 3.411 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP007626.D
Acq: 23 Oct 2021 12:43

Instrument :
BNA_P
ClientSampleId :
BFYA4

Tgt Ion:	88	Resp:	91723
Ion	Ratio	Lower	Upper
88	100		
43	26.2	24.2	36.2
58	71.1	62.5	93.7

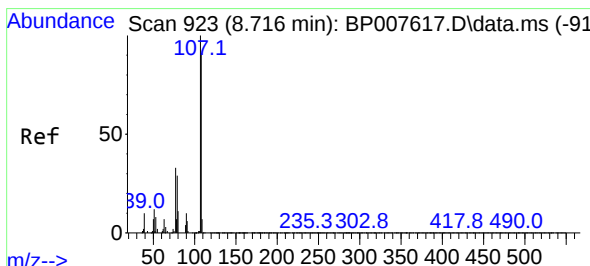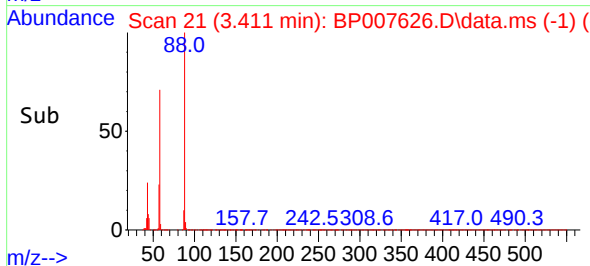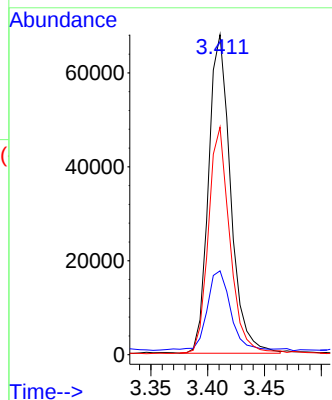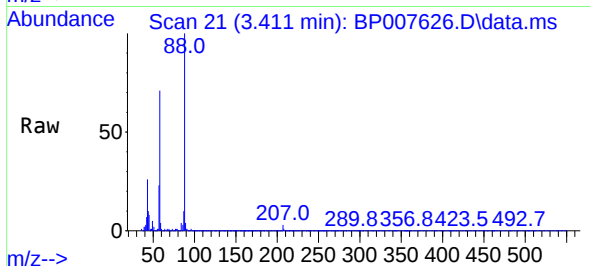

#18
4-Methylphenol
Concen: 1.450 ng/uL
RT: 8.711 min Scan# 922
Delta R.T. -0.011 min
Lab File: BP007626.D
Acq: 23 Oct 2021 12:43

Tgt Ion:	108	Resp:	18711
Ion	Ratio	Lower	Upper
108	100		
107	120.2	90.9	136.3

