

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007545.D
 Acq On : 21 Oct 2021 09:21
 Operator : CG/JU
 Sample : PB140022BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.376	11	15	24	rVB	52848	73408	1.50%	0.144%
2	3.793	83	86	109	rBV	736480	1112934	22.76%	2.190%
3	4.128	139	143	152	rVB	14065	26368	0.54%	0.052%
4	7.111	644	650	660	rVB	833430	1280929	26.19%	2.520%
5	7.281	672	679	691	rVB	639546	1006045	20.57%	1.980%
6	7.481	704	713	723	rBV	836672	1303492	26.65%	2.565%
7	7.952	786	793	803	rBV	730402	1142643	23.36%	2.248%
8	8.658	906	913	924	rBV	1040331	1610682	32.93%	3.169%
9	9.111	982	990	1000	rBV	738700	1201589	24.57%	2.364%
10	9.834	1105	1113	1127	rBV	557540	921517	18.84%	1.813%
11	10.375	1196	1205	1217	rBV	1000889	1635342	33.44%	3.218%
12	10.758	1263	1270	1280	rVB	963432	1642296	33.58%	3.232%
13	10.887	1284	1292	1303	rBV	976327	1656553	33.87%	3.260%
14	11.557	1400	1406	1411	rBV10	2877	6386	0.13%	0.013%
15	12.346	1534	1540	1547	rBV	19719	33886	0.69%	0.067%
16	13.328	1704	1707	1713	rVB8	3901	5527	0.11%	0.011%
17	13.557	1743	1746	1753	rVB8	4277	8564	0.18%	0.017%
18	13.999	1814	1821	1827	rBV	1737521	2386497	48.79%	4.696%
19	14.281	1862	1869	1880	rBV	1966026	2873334	58.75%	5.654%
20	14.587	1914	1921	1929	rBV	1468357	2244471	45.89%	4.416%
21	14.775	1944	1953	1966	rBV	779275	1151006	23.53%	2.265%
22	15.240	2029	2032	2037	rVB6	3599	5231	0.11%	0.010%
23	15.581	2084	2090	2101	rVB	2511685	3635353	74.33%	7.153%
24	15.693	2103	2109	2124	rVV	528152	739246	15.11%	1.455%
25	15.822	2126	2131	2138	rVB2	34156	52604	1.08%	0.104%
26	16.263	2200	2206	2209	rBV8	5226	7818	0.16%	0.015%
27	16.375	2219	2225	2226	rBV6	4298	5115	0.10%	0.010%
28	17.128	2349	2353	2361	rVB	10281	16366	0.33%	0.032%
29	17.340	2382	2389	2396	rBV	1863562	2732372	55.87%	5.376%
30	17.440	2400	2406	2419	rVB	2849513	4073569	83.29%	8.016%
31	17.575	2427	2429	2434	rVB6	6649	9018	0.18%	0.018%
32	17.710	2449	2452	2457	rBV4	4387	7829	0.16%	0.015%
33	18.016	2501	2504	2508	rBV5	6323	7650	0.16%	0.015%
34	18.234	2537	2541	2547	rBV8	7366	15357	0.31%	0.030%
35	19.251	2710	2714	2720	rBV3	40395	52316	1.07%	0.103%
36	19.316	2721	2725	2731	rBV	39579	57813	1.18%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007545.D
Acq On : 21 Oct 2021 09:21
Operator : CG/JU
Sample : PB140022BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK022

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	19.675	2780	2786	2798	rBV	3591702	4853277	99.23%	9.550%
38	21.428	3079	3084	3091	rBV	2377986	3092474	63.23%	6.085%
39	23.716	3466	3473	3485	rBV2	2324898	4890885	100.00%	9.624%
40	23.880	3494	3501	3511	rVB2	1495309	3243354	66.31%	6.382%




Sum of corrected areas: 50821116

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007545.D
Acq On : 21 Oct 2021 09:21
Operator : CG/JU
Sample : PB140022BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK022

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

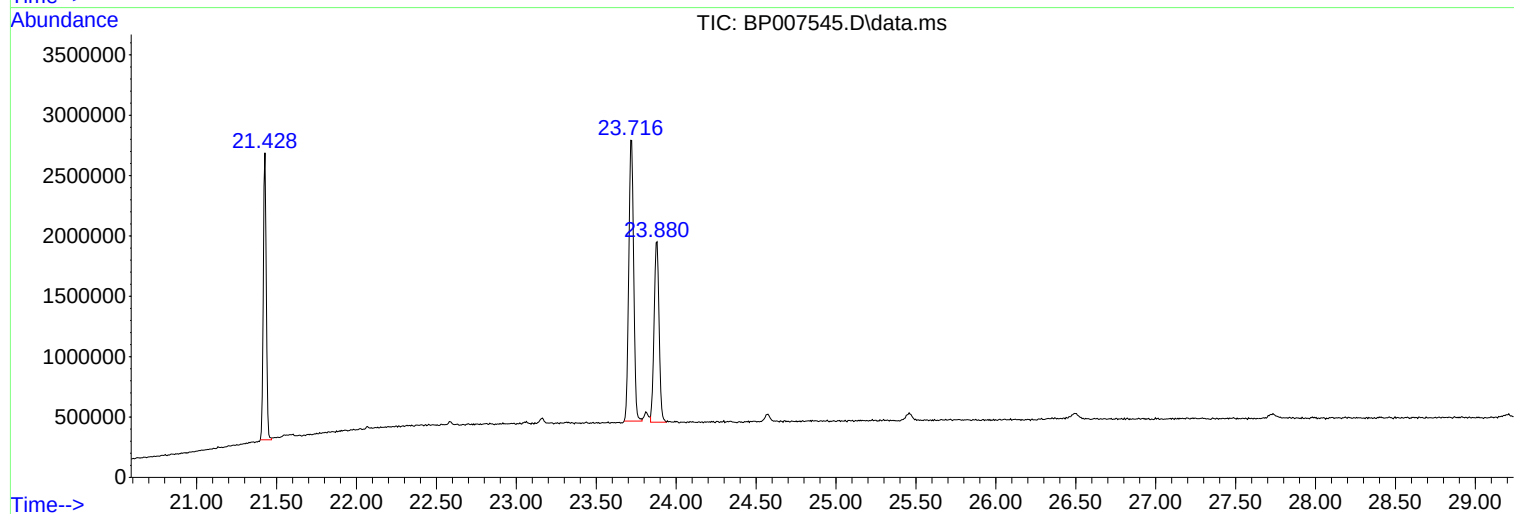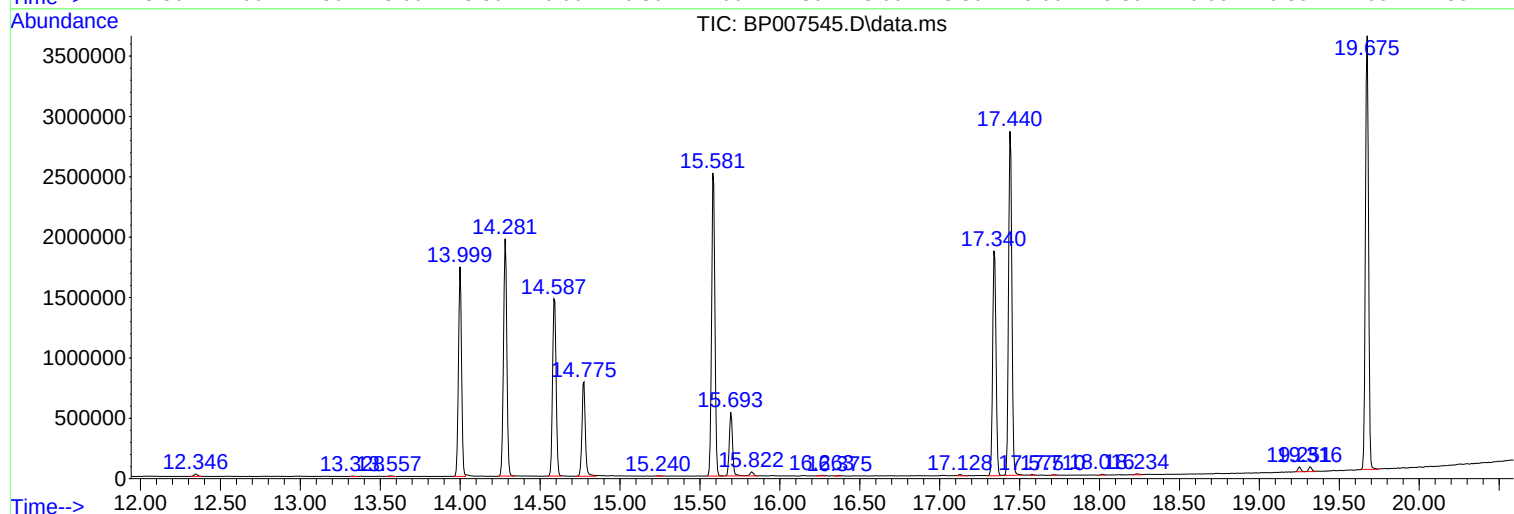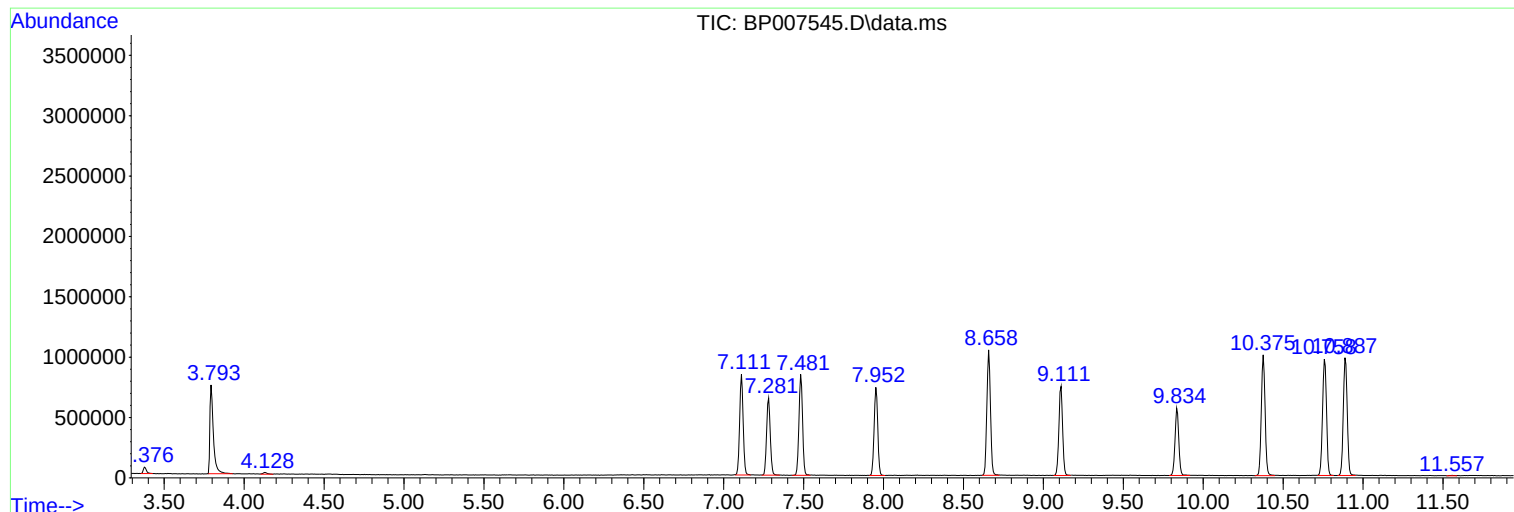

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007545.D
Acq On : 21 Oct 2021 09:21
Operator : CG/JU
Sample : PB140022BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK022

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007545.D
Acq On : 21 Oct 2021 09:21
Operator : CG/JU
Sample : PB140022BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK022

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
