

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007560.D
 Acq On : 21 Oct 2021 18:06
 Operator : CG/JU
 Sample : M4262-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	19	rBV	42682	50448	0.85%	0.093%
2	3.411	19	21	29	rVB	32321	41934	0.70%	0.077%
3	3.658	59	63	69	rBV	8772	16311	0.27%	0.030%
4	3.799	84	87	100	rBV	203956	314836	5.29%	0.582%
5	4.040	123	128	132	rVB	31048	45066	0.76%	0.083%
6	4.128	140	143	147	rVB	12252	16994	0.29%	0.031%
7	4.222	154	159	165	rBV7	14604	22053	0.37%	0.041%
8	4.581	219	220	225	rVB4	5077	6779	0.11%	0.013%
9	5.052	295	300	306	rVB4	10386	19487	0.33%	0.036%
10	5.652	400	402	410	rVB9	3220	7269	0.12%	0.013%
11	6.034	461	467	475	rBV7	5294	9134	0.15%	0.017%
12	6.328	509	517	522	rBV3	11137	19061	0.32%	0.035%
13	6.963	620	625	627	rVB4	4829	6726	0.11%	0.012%
14	7.111	643	650	660	rVB	322730	523636	8.80%	0.967%
15	7.275	670	678	688	rBV	661223	1051711	17.67%	1.943%
16	7.481	706	713	722	rBV	773084	1245138	20.92%	2.300%
17	7.952	785	793	800	rBV	701843	1118662	18.79%	2.066%
18	8.016	800	804	808	rVB5	7612	12550	0.21%	0.023%
19	8.199	828	835	840	rBV6	10657	22378	0.38%	0.041%
20	8.510	883	888	892	rBV3	7489	12111	0.20%	0.022%
21	8.652	905	912	926	rBV	789028	1289846	21.67%	2.383%
22	9.105	982	989	1005	rBV	792370	1287595	21.63%	2.378%
23	9.228	1005	1010	1013	rVV7	5914	11286	0.19%	0.021%
24	9.281	1016	1019	1024	rVB7	6995	10413	0.17%	0.019%
25	9.569	1063	1068	1073	rBV4	8512	13160	0.22%	0.024%
26	9.834	1104	1113	1123	rBV	591305	993563	16.69%	1.835%
27	10.369	1195	1204	1216	rBV	1018883	1691552	28.42%	3.125%
28	10.534	1226	1232	1246	rBV	465463	763799	12.83%	1.411%
29	10.752	1261	1269	1278	rVB	921642	1577355	26.50%	2.914%
30	10.887	1283	1292	1301	rBV	865463	1494442	25.11%	2.760%
31	11.546	1399	1404	1408	rBV8	6271	11664	0.20%	0.022%
32	12.010	1477	1483	1487	rBV8	3737	7623	0.13%	0.014%
33	12.063	1487	1492	1496	rBV8	6663	12212	0.21%	0.023%
34	12.204	1510	1516	1519	rBV7	7100	12043	0.20%	0.022%
35	12.246	1519	1523	1527	rVV7	7466	10602	0.18%	0.020%
36	12.340	1532	1539	1548	rVB2	20679	34676	0.58%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007560.D
 Acq On : 21 Oct 2021 18:06
 Operator : CG/JU
 Sample : M4262-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	12.957	1640	1644	1648	rBV6	8826	13075	0.22%	0.024%
38	13.204	1681	1686	1692	rBV5	10931	15973	0.27%	0.030%
39	13.498	1731	1736	1740	rVB4	21557	33002	0.55%	0.061%
40	13.563	1742	1747	1750	rVB4	5242	8840	0.15%	0.016%
41	13.993	1813	1820	1835	rBV	1855100	2695656	45.29%	4.979%
42	14.275	1856	1868	1879	rBV	2080771	3114246	52.32%	5.752%
43	14.587	1911	1921	1928	rBV	1405718	2136293	35.89%	3.946%
44	14.769	1943	1952	1959	rBV	190599	292144	4.91%	0.540%
45	15.004	1987	1992	1999	rVV10	14384	21430	0.36%	0.040%
46	15.122	2009	2012	2018	rVB2	5053	8573	0.14%	0.016%
47	15.334	2044	2048	2054	rVB2	7854	10737	0.18%	0.020%
48	15.398	2054	2059	2064	rVV	33282	49792	0.84%	0.092%
49	15.451	2064	2068	2074	rVB8	7100	11403	0.19%	0.021%
50	15.581	2080	2090	2101	rBV	2826199	4137265	69.51%	7.642%
51	15.692	2102	2109	2115	rBV	662340	933863	15.69%	1.725%
52	15.816	2126	2130	2137	rVB2	33842	51690	0.87%	0.095%
53	15.945	2147	2152	2155	rBV5	6098	10059	0.17%	0.019%
54	16.022	2162	2165	2171	rVB4	16156	22153	0.37%	0.041%
55	16.134	2180	2184	2196	rBV4	9544	26765	0.45%	0.049%
56	16.251	2198	2204	2206	rBV6	7362	14327	0.24%	0.026%
57	16.369	2221	2224	2229	rVB7	7687	13422	0.23%	0.025%
58	16.486	2240	2244	2251	rVB10	9085	14465	0.24%	0.027%
59	16.592	2259	2262	2267	rBV7	6263	9222	0.15%	0.017%
60	16.745	2284	2288	2292	rVB7	9181	13355	0.22%	0.025%
61	16.981	2324	2328	2332	rBV6	12020	17347	0.29%	0.032%
62	17.010	2332	2333	2339	rVB5	4804	6400	0.11%	0.012%
63	17.116	2348	2351	2355	rBV3	11475	13438	0.23%	0.025%
64	17.339	2382	2389	2398	rVB	1877948	2633484	44.25%	4.864%
65	17.439	2399	2406	2416	rBV	3320730	4780914	80.33%	8.831%
66	17.528	2418	2421	2425	rVB6	9462	13520	0.23%	0.025%
67	17.634	2437	2439	2443	rVB	8148	8855	0.15%	0.016%
68	17.751	2455	2459	2464	rVB7	11176	18924	0.32%	0.035%
69	18.022	2500	2505	2510	rBV	112431	134304	2.26%	0.248%
70	18.081	2512	2515	2518	rBV4	5770	8205	0.14%	0.015%
71	18.228	2536	2540	2549	rBV	110393	164979	2.77%	0.305%
72	18.298	2549	2552	2557	rVB	15226	22167	0.37%	0.041%
73	18.533	2588	2592	2600	rVB	9774	18935	0.32%	0.035%
74	19.122	2689	2692	2693	rBV3	18515	16851	0.28%	0.031%
75	19.151	2693	2697	2705	rVB	207891	241513	4.06%	0.446%
76	19.245	2710	2713	2716	rBV2	49992	64417	1.08%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007560.D
 Acq On : 21 Oct 2021 18:06
 Operator : CG/JU
 Sample : M4262-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY94

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

77	19.280	2716	2719	2721	rVV2	36708	33818	0.57%	0.062%
78	19.316	2721	2725	2729	rVB	48704	59280	1.00%	0.109%
79	19.463	2747	2750	2755	rBV4	31344	37236	0.63%	0.069%
80	19.669	2779	2785	2792	rBV	4398452	5836532	98.06%	10.781%
81	21.145	3032	3036	3042	rBV2	145908	224137	3.77%	0.414%
82	21.422	3078	3083	3089	rBV	2361701	3148862	52.90%	5.816%
83	23.716	3466	3473	3482	rVB2	2935631	5951923	100.00%	10.994%
84	23.874	3493	3500	3509	rVB2	1537680	3240189	54.44%	5.985%




Sum of corrected areas: 54138095

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007560.D
Acq On : 21 Oct 2021 18:06
Operator : CG/JU
Sample : M4262-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY94

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

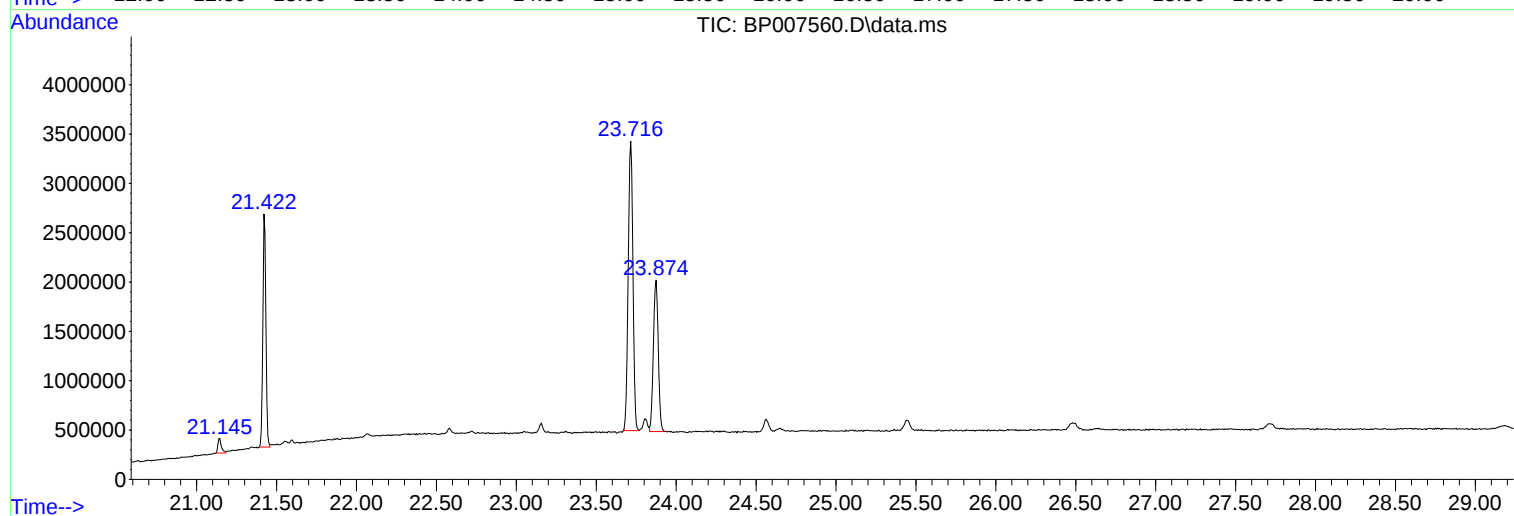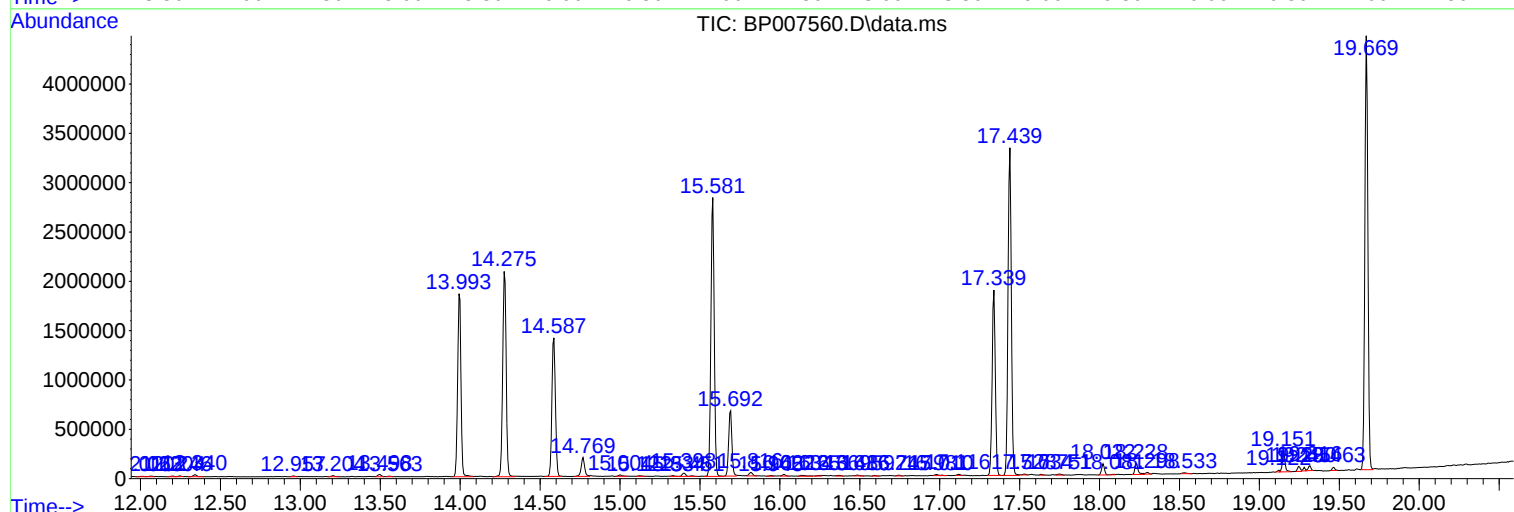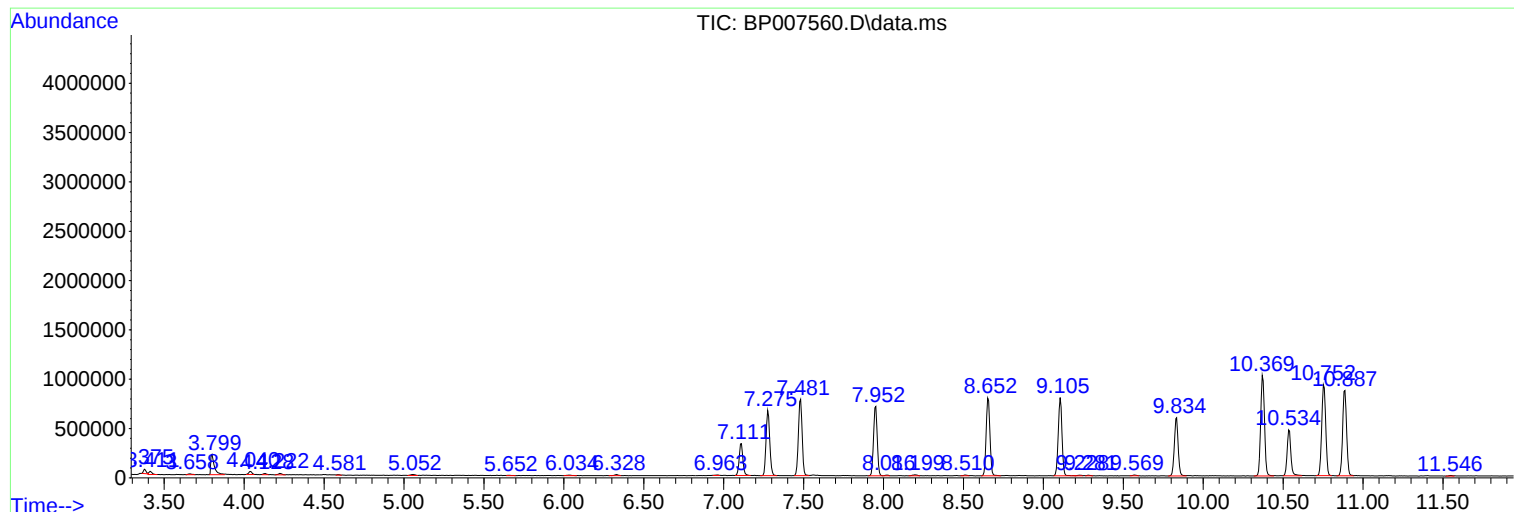

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007560.D
Acq On : 21 Oct 2021 18:06
Operator : CG/JU
Sample : M4262-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY94










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.534	9.68 ng/ul	763799	Naphthalene-d8	10.752

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83

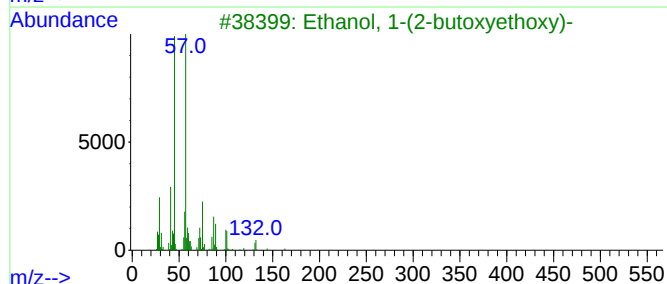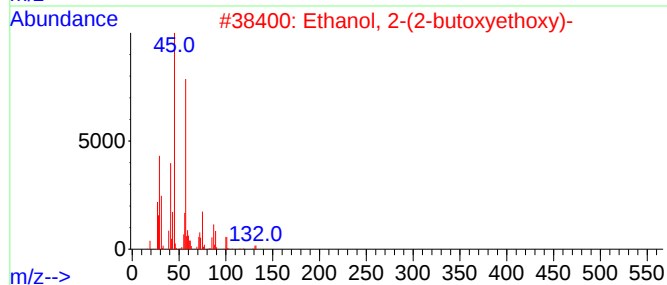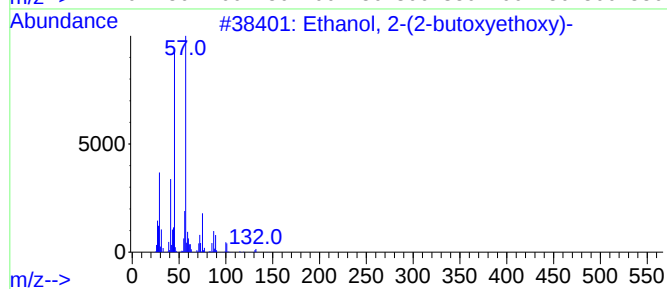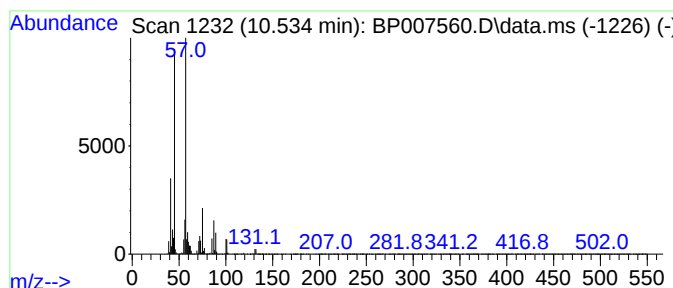

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007560.D
Acq On : 21 Oct 2021 18:06
Operator : CG/JU
Sample : M4262-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY94

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.534	9.7	ng/ul	763799	2	10.752	1577360	20.0