

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007562.D
 Acq On : 21 Oct 2021 19:48
 Operator : CG/JU
 Sample : PB140023BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK023

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	26	rVB	60689	79059	1.45%	0.141%
2	3.793	82	86	103	rBV	772424	1200046	21.98%	2.134%
3	4.128	140	143	148	rVB	14705	18295	0.34%	0.033%
4	5.128	308	313	316	rBV7	4390	6334	0.12%	0.011%
5	7.111	641	650	658	rBV	914403	1466049	26.85%	2.606%
6	7.275	671	678	692	rVB	730441	1151393	21.09%	2.047%
7	7.481	706	713	722	rBV	923834	1482586	27.15%	2.636%
8	7.946	784	792	801	rBV	739299	1189978	21.79%	2.116%
9	8.652	904	912	926	rBV	1150403	1852272	33.92%	3.293%
10	9.105	979	989	999	rBV	854175	1400830	25.66%	2.491%
11	9.828	1105	1112	1122	rBV	651981	1093513	20.03%	1.944%
12	10.369	1197	1204	1216	rBV	1139201	1885682	34.54%	3.353%
13	10.752	1262	1269	1281	rVB	1036002	1721392	31.53%	3.060%
14	10.881	1281	1291	1301	rBV	1100165	1892145	34.65%	3.364%
15	12.340	1532	1539	1545	rVB	23963	40319	0.74%	0.072%
16	13.551	1742	1745	1750	rVB4	4946	8359	0.15%	0.015%
17	13.993	1813	1820	1834	rBV	1972530	2724273	49.90%	4.843%
18	14.275	1859	1868	1878	rBV	2175625	3268885	59.87%	5.812%
19	14.581	1913	1920	1932	rBV	1526078	2326290	42.61%	4.136%
20	14.769	1943	1952	1965	rBV	939671	1349429	24.71%	2.399%
21	15.240	2027	2032	2037	rBV9	4695	9654	0.18%	0.017%
22	15.581	2081	2090	2099	rBV	2720376	4108460	75.25%	7.304%
23	15.692	2103	2109	2121	rBV	592624	866247	15.87%	1.540%
24	15.816	2126	2130	2137	rVV	35772	61761	1.13%	0.110%
25	15.875	2137	2140	2146	rVB8	2903	6256	0.11%	0.011%
26	15.945	2146	2152	2154	rBV6	4405	7382	0.14%	0.013%
27	16.145	2181	2186	2191	rVB9	4103	7158	0.13%	0.013%
28	16.257	2200	2205	2210	rBV9	7207	14021	0.26%	0.025%
29	17.016	2330	2334	2337	rBV5	5806	7892	0.14%	0.014%
30	17.116	2347	2351	2356	rBV2	9188	14877	0.27%	0.026%
31	17.334	2382	2388	2396	rBV	1902592	2818457	51.62%	5.011%
32	17.439	2399	2406	2417	rVV	3081184	4572387	83.74%	8.129%
33	17.575	2424	2429	2434	rVB7	8270	14212	0.26%	0.025%
34	18.004	2500	2502	2507	rBV5	6748	10113	0.19%	0.018%
35	19.245	2709	2713	2720	rBV	45335	58788	1.08%	0.105%
36	19.316	2720	2725	2731	rBV	46259	67008	1.23%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007562.D
Acq On : 21 Oct 2021 19:48
Operator : CG/JU
Sample : PB140023BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK023

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	19.669	2779	2785	2792	rBV	4154473	5429692	99.45%	9.653%
38	21.422	3078	3083	3089	rBV	2480781	3217465	58.93%	5.720%
39	23.716	3466	3473	3482	rVB2	2693589	5459984	100.00%	9.707%
40	23.874	3493	3500	3510	rVB	1590333	3337344	61.12%	5.933%




Sum of corrected areas: 56246287

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007562.D
Acq On : 21 Oct 2021 19:48
Operator : CG/JU
Sample : PB140023BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK023

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

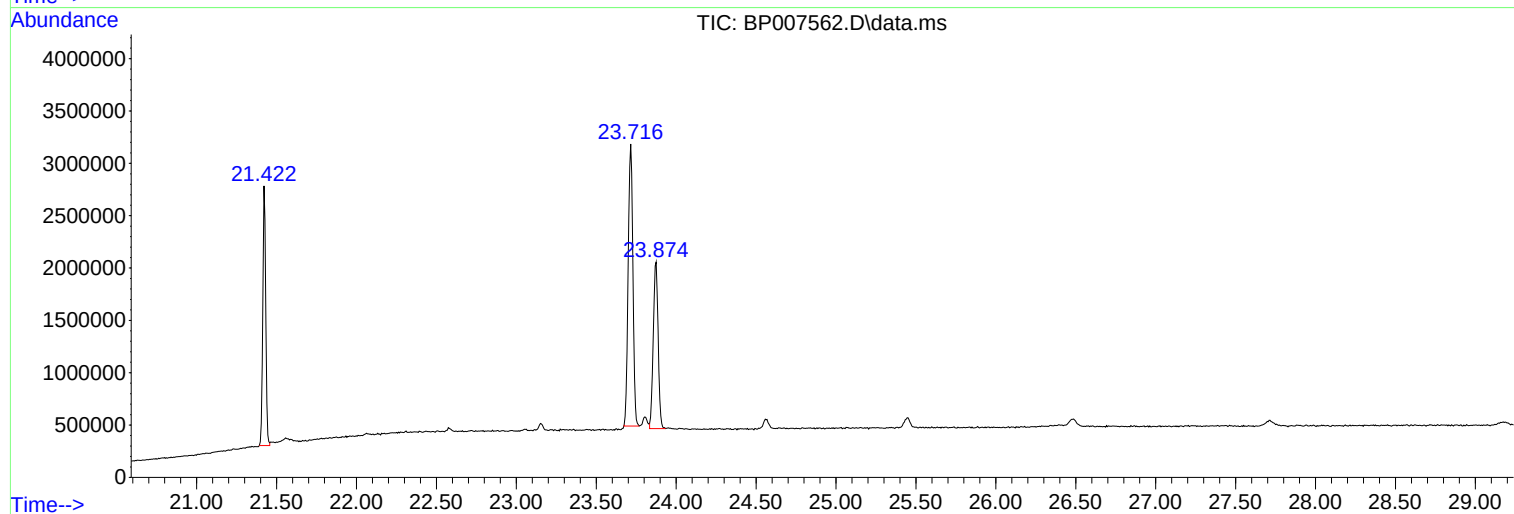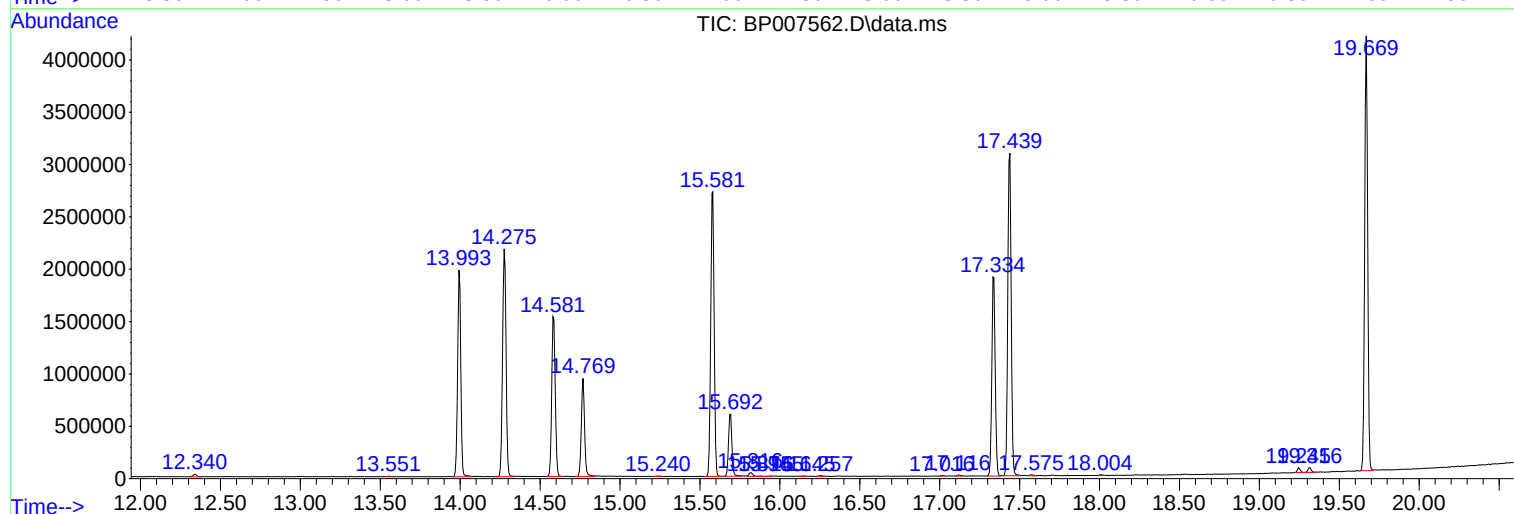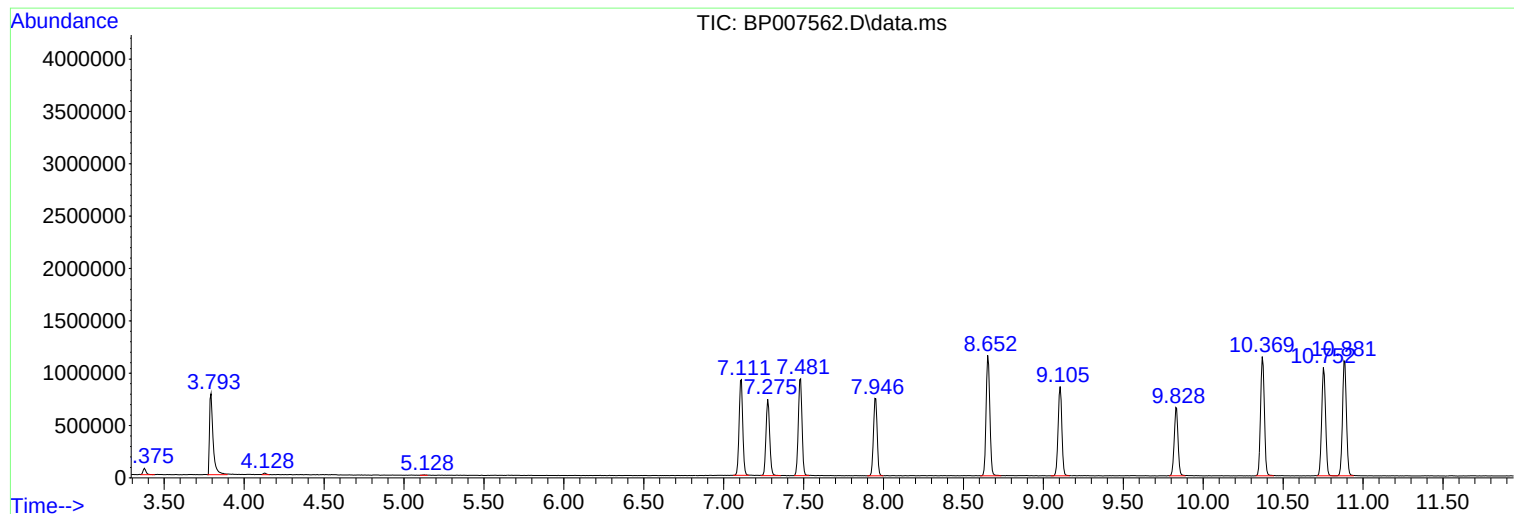

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007562.D
Acq On : 21 Oct 2021 19:48
Operator : CG/JU
Sample : PB140023BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK023

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007562.D
Acq On : 21 Oct 2021 19:48
Operator : CG/JU
Sample : PB140023BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK023

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
