

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007566.D
 Acq On : 21 Oct 2021 22:03
 Operator : CG/JU
 Sample : M4262-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	7	10	12	rBV4	10824	14311	0.22%	0.025%
2	3.376	12	15	21	rVB	60746	77962	1.22%	0.134%
3	3.658	60	63	68	rBV	8854	11833	0.19%	0.020%
4	3.793	84	86	103	rBV	208192	347105	5.43%	0.594%
5	4.034	122	127	134	rVB	31661	49788	0.78%	0.085%
6	4.128	139	143	148	rVB	17224	21386	0.33%	0.037%
7	4.223	155	159	163	rBV6	12253	17422	0.27%	0.030%
8	4.581	218	220	226	rVB5	5271	9080	0.14%	0.016%
9	5.052	297	300	304	rVB4	7019	8926	0.14%	0.015%
10	6.334	511	518	526	rVB4	13181	25448	0.40%	0.044%
11	6.958	620	624	629	rVB6	5483	8859	0.14%	0.015%
12	7.105	643	649	660	rVB	233722	368739	5.77%	0.632%
13	7.275	670	678	688	rBV	754109	1179967	18.47%	2.021%
14	7.475	704	712	723	rBV	768413	1215659	19.03%	2.082%
15	7.552	723	725	728	rBV4	5388	6975	0.11%	0.012%
16	7.946	784	792	800	rBV	797894	1250851	19.58%	2.142%
17	8.022	800	805	808	rVB2	12593	18486	0.29%	0.032%
18	8.099	814	818	822	rVB6	4233	7331	0.11%	0.013%
19	8.199	829	835	842	rVB6	11101	22093	0.35%	0.038%
20	8.511	883	888	897	rBV6	9706	19067	0.30%	0.033%
21	8.652	905	912	926	rBV	647604	1050332	16.44%	1.799%
22	9.105	981	989	1001	rBV	870348	1452422	22.74%	2.488%
23	9.287	1015	1020	1025	rVB9	6811	11742	0.18%	0.020%
24	9.575	1062	1069	1075	rVB2	11236	20596	0.32%	0.035%
25	9.828	1100	1112	1127	rBV	666344	1113723	17.44%	1.907%
26	10.058	1146	1151	1156	rBV9	3408	7934	0.12%	0.014%
27	10.369	1196	1204	1214	rBV	1076389	1791366	28.04%	3.068%
28	10.534	1225	1232	1245	rBV	485017	794430	12.44%	1.361%
29	10.752	1261	1269	1280	rVB	1045167	1802053	28.21%	3.086%
30	10.881	1283	1291	1303	rBV	903196	1553037	24.31%	2.660%
31	11.404	1375	1380	1385	rBV2	6920	12226	0.19%	0.021%
32	11.463	1385	1390	1398	rVB2	3700	7056	0.11%	0.012%
33	12.069	1488	1493	1500	rVB3	12368	21589	0.34%	0.037%
34	12.340	1532	1539	1546	rVB	26273	43325	0.68%	0.074%
35	12.957	1639	1644	1648	rBV6	5909	10531	0.16%	0.018%
36	13.093	1661	1667	1672	rBV6	6424	12368	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007566.D
 Acq On : 21 Oct 2021 22:03
 Operator : CG/JU
 Sample : M4262-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	13.204	1681	1686	1691	rVB6	7209	12476	0.20%	0.021%
38	13.428	1719	1724	1729	rBV3	14775	21562	0.34%	0.037%
39	13.493	1729	1735	1739	rVV4	10356	17148	0.27%	0.029%
40	13.557	1742	1746	1751	rVV3	5556	9312	0.15%	0.016%

41	13.898	1798	1804	1807	rBV4	7452	12391	0.19%	0.021%
42	13.993	1812	1820	1826	rBV	2200873	2973263	46.55%	5.092%
43	14.116	1837	1841	1846	rVB8	6327	10864	0.17%	0.019%
44	14.275	1857	1868	1876	rBV	2331659	3393724	53.13%	5.812%
45	14.581	1913	1920	1932	rBV	1651689	2502842	39.18%	4.287%

46	14.763	1942	1951	1957	rBV	201051	326401	5.11%	0.559%
47	14.998	1987	1991	1995	rBV6	13453	18168	0.28%	0.031%
48	15.128	2009	2013	2020	rVB4	9941	17241	0.27%	0.030%
49	15.228	2027	2030	2036	rVB8	3322	6440	0.10%	0.011%
50	15.328	2044	2047	2055	rBV4	6266	11773	0.18%	0.020%

51	15.398	2055	2059	2063	rVV5	8090	11408	0.18%	0.020%
52	15.575	2082	2089	2098	rBV	3110184	4518136	70.73%	7.738%
53	15.687	2101	2108	2117	rBV	793862	1108219	17.35%	1.898%
54	15.816	2125	2130	2135	rVV	35982	55699	0.87%	0.095%
55	15.857	2135	2137	2141	rVB5	9757	11787	0.18%	0.020%

56	16.022	2162	2165	2168	rBV3	12198	13909	0.22%	0.024%
57	16.145	2182	2186	2193	rBV9	9531	20570	0.32%	0.035%
58	16.198	2193	2195	2197	rVV3	5970	6511	0.10%	0.011%
59	16.257	2199	2205	2210	rVV9	10750	27266	0.43%	0.047%
60	16.322	2212	2216	2217	rVV4	8422	11974	0.19%	0.021%

61	16.340	2217	2219	2228	rVB5	15303	34477	0.54%	0.059%
62	16.487	2240	2244	2249	rBV8	7270	12947	0.20%	0.022%
63	16.592	2258	2262	2265	rBV6	5587	8891	0.14%	0.015%
64	16.745	2283	2288	2291	rVB7	9492	13463	0.21%	0.023%
65	17.010	2328	2333	2336	rBV7	6255	10624	0.17%	0.018%

66	17.122	2349	2352	2355	rVB2	9663	11018	0.17%	0.019%
67	17.334	2382	2388	2395	rBV	2032005	2954492	46.25%	5.060%
68	17.434	2398	2405	2417	rBV	3582726	5250642	82.20%	8.993%
69	18.022	2500	2505	2510	rBV	97057	125867	1.97%	0.216%
70	18.228	2536	2540	2549	rBV2	144853	188509	2.95%	0.323%

71	18.522	2586	2590	2599	rBV2	41588	75776	1.19%	0.130%
72	19.151	2693	2697	2704	rVB	107547	133020	2.08%	0.228%
73	19.245	2709	2713	2716	rBV2	53597	66914	1.05%	0.115%
74	19.310	2721	2724	2729	rVV	53296	63277	0.99%	0.108%
75	19.463	2746	2750	2755	rBV3	43014	54660	0.86%	0.094%

76	19.669	2779	2785	2792	rBV	4797652	6368411	99.70%	10.907%
----	--------	------	------	------	-----	---------	---------	--------	---------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007566.D
Acq On : 21 Oct 2021 22:03
Operator : CG/JU
Sample : M4262-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY92

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

77	21.139	3032	3035	3043	rBV2	173472	232925	3.65%	0.399%
78	21.422	3078	3083	3089	rBV	2502930	3367903	52.73%	5.768%
79	23.716	3465	3473	3482	rVB2	3095774	6387529	100.00%	10.940%
80	23.869	3492	3499	3515	rVB2	1669476	3521099	55.12%	6.031%




Sum of corrected areas: 58387546

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007566.D
Acq On : 21 Oct 2021 22:03
Operator : CG/JU
Sample : M4262-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY92

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

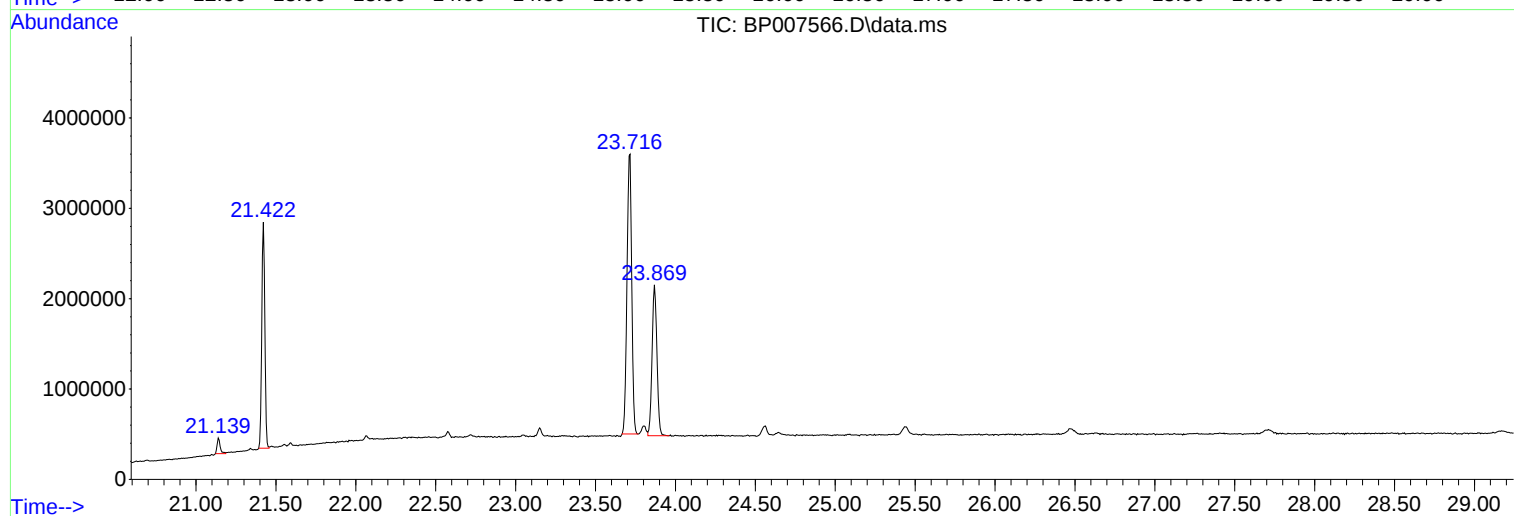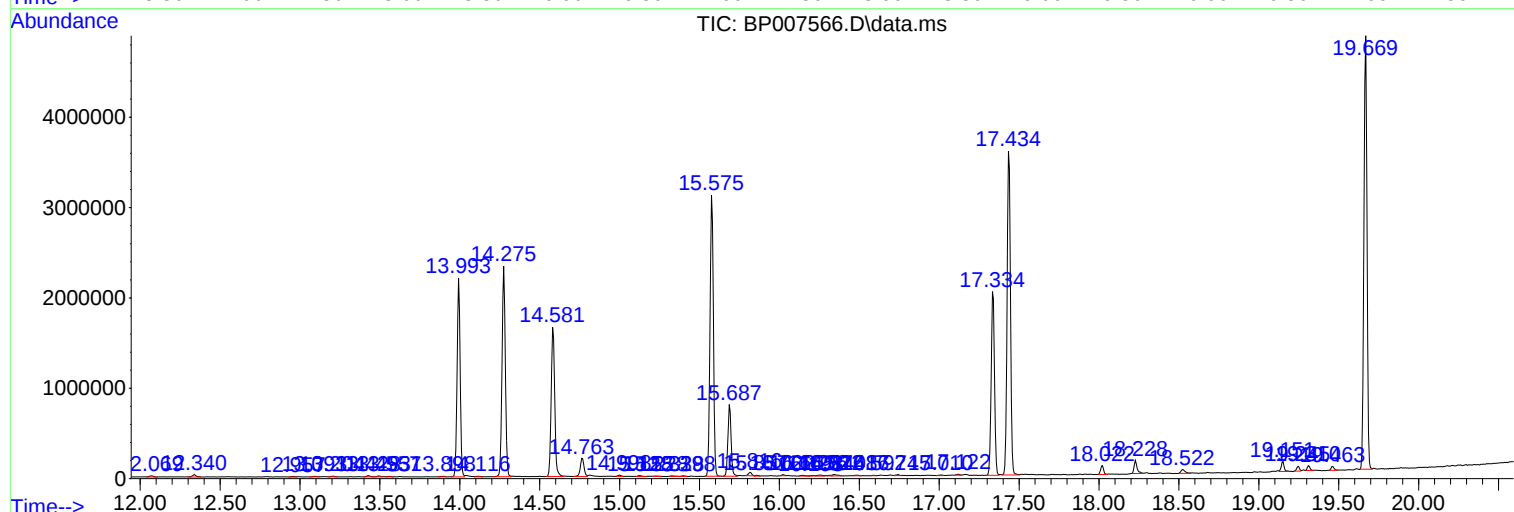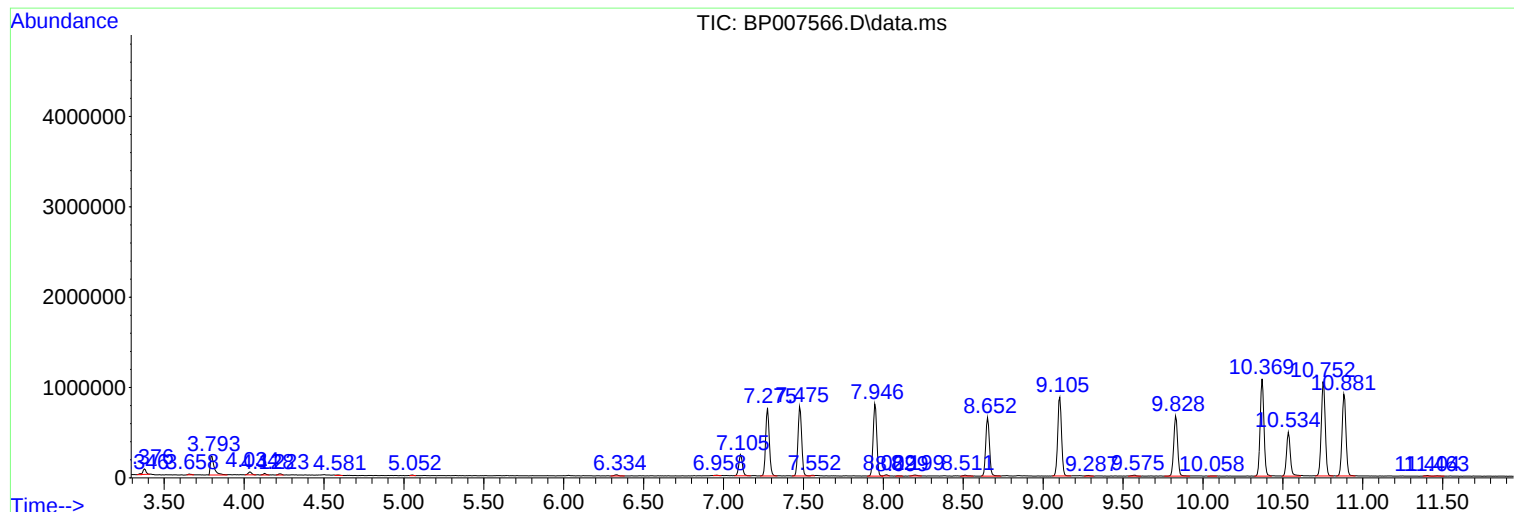

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007566.D
Acq On : 21 Oct 2021 22:03
Operator : CG/JU
Sample : M4262-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY92










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.534	8.82 ng/ul	794430	Naphthalene-d8	10.752

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	91
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5			Ethanol, 2-[2-(2-methylpropoxy)e...	162	C8H18O3	018912-80-6	72

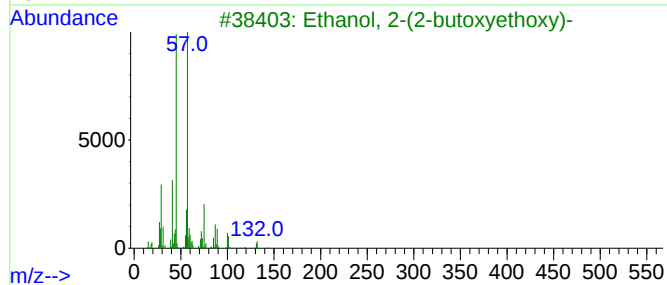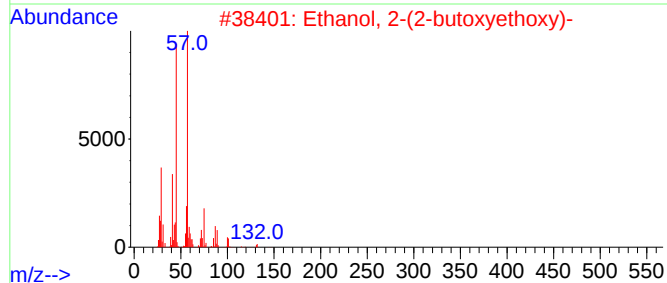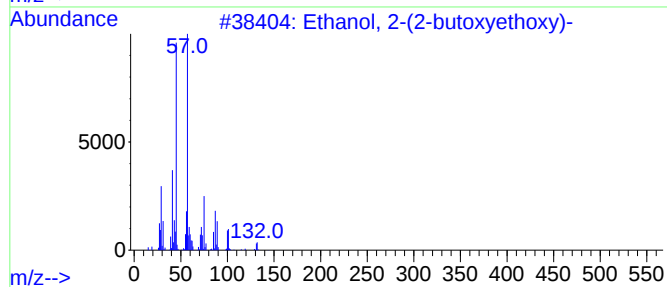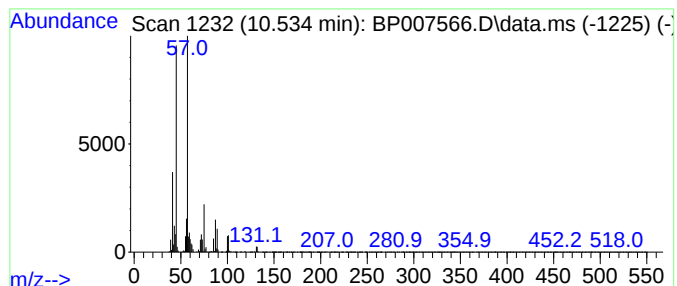

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007566.D
Acq On : 21 Oct 2021 22:03
Operator : CG/JU
Sample : M4262-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY92

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.534	8.8	ng/ul	794430	2	10.752	1802050	20.0