

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007567.D
 Acq On : 21 Oct 2021 22:37
 Operator : CG/JU
 Sample : M4217-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	19	rVB2	12275	13914	0.38%	0.054%
2	3.817	89	90	101	rVB2	11657	18069	0.49%	0.071%
3	4.040	122	128	134	rBV	49272	78281	2.12%	0.306%
4	4.128	139	143	149	rVB2	14487	19439	0.53%	0.076%
5	4.222	155	159	165	rVB	19454	30816	0.83%	0.120%
6	4.499	203	206	210	rVB5	9177	11797	0.32%	0.046%
7	4.581	218	220	227	rVB5	5989	11597	0.31%	0.045%
8	5.052	294	300	305	rVB	19467	31931	0.86%	0.125%
9	5.652	399	402	407	rVB7	2775	3850	0.10%	0.015%
10	6.328	512	517	523	rVB	19233	32510	0.88%	0.127%
11	7.105	642	649	658	rBV	206422	337619	9.13%	1.319%
12	7.275	671	678	686	rVB	170735	271712	7.35%	1.062%
13	7.393	696	698	704	rVB7	2676	4031	0.11%	0.016%
14	7.475	706	712	720	rBV	211021	336688	9.11%	1.316%
15	7.587	727	731	737	rVB9	5247	8889	0.24%	0.035%
16	7.763	758	761	768	rVB5	4663	7183	0.19%	0.028%
17	7.946	785	792	801	rBV	815835	1297389	35.10%	5.070%
18	8.199	830	835	838	rBV5	7556	11797	0.32%	0.046%
19	8.510	882	888	891	rBV8	5841	11196	0.30%	0.044%
20	8.652	905	912	920	rBV	258517	412054	11.15%	1.610%
21	8.769	927	932	938	rVB2	14370	23295	0.63%	0.091%
22	9.104	981	989	1000	rBV	192616	316803	8.57%	1.238%
23	9.569	1065	1068	1073	rVB7	5181	7901	0.21%	0.031%
24	9.828	1103	1112	1121	rBV	127925	218509	5.91%	0.854%
25	10.369	1197	1204	1213	rBV	244744	407432	11.02%	1.592%
26	10.534	1225	1232	1239	rBV	31756	56024	1.52%	0.219%
27	10.751	1256	1269	1280	rBV	1114553	1887466	51.07%	7.376%
28	10.881	1282	1291	1300	rBV	230010	388384	10.51%	1.518%
29	11.546	1399	1404	1410	rBV9	5192	10851	0.29%	0.042%
30	12.334	1532	1538	1543	rBV6	6004	11257	0.30%	0.044%
31	12.951	1639	1643	1645	rBV5	2920	4125	0.11%	0.016%
32	13.204	1682	1686	1691	rVB8	4616	5954	0.16%	0.023%
33	13.910	1802	1806	1811	rBV7	4034	6565	0.18%	0.026%
34	13.992	1813	1820	1826	rVV	434495	590670	15.98%	2.308%
35	14.040	1826	1828	1832	rVB5	3860	6081	0.16%	0.024%
36	14.275	1862	1868	1877	rVB	490446	705097	19.08%	2.755%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007567.D
 Acq On : 21 Oct 2021 22:37
 Operator : CG/JU
 Sample : M4217-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	14.587	1912	1921	1933	rBV	1688300	2600638	70.37%	10.163%
38	14.769	1941	1952	1962	rBV	103461	179528	4.86%	0.702%
39	14.998	1985	1991	1998	rBV3	36776	55294	1.50%	0.216%
40	15.051	1998	2000	2004	rVB5	3011	3808	0.10%	0.015%
41	15.404	2055	2060	2065	rBV9	3145	5013	0.14%	0.020%
42	15.575	2083	2089	2098	rBV	690629	955507	25.85%	3.734%
43	15.686	2102	2108	2115	rBV	58295	88232	2.39%	0.345%
44	15.816	2125	2130	2136	rVB7	8245	14624	0.40%	0.057%
45	16.022	2161	2165	2171	rBV9	3097	4422	0.12%	0.017%
46	16.139	2181	2185	2188	rBV5	3714	5134	0.14%	0.020%
47	17.122	2348	2352	2355	rBV2	8938	11898	0.32%	0.046%
48	17.333	2382	2388	2398	rBV	2174878	3132655	84.76%	12.242%
49	17.433	2399	2405	2414	rVV	703905	1016034	27.49%	3.970%
50	17.528	2417	2421	2426	rVB3	26610	36770	0.99%	0.144%
51	18.016	2500	2504	2509	rBV3	20257	24989	0.68%	0.098%
52	18.228	2536	2540	2544	rBV3	30229	40408	1.09%	0.158%
53	19.663	2779	2784	2793	rBV	959367	1290349	34.91%	5.042%
54	21.139	3032	3035	3039	rBV5	73487	102050	2.76%	0.399%
55	21.421	3078	3083	3089	rBV	2720381	3531776	95.56%	13.801%
56	23.710	3466	3472	3481	rVB2	590573	1197861	32.41%	4.681%
57	23.868	3492	3499	3511	rVB2	1822516	3695898	100.00%	14.443%




Sum of corrected areas: 25590064

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007567.D
Acq On : 21 Oct 2021 22:37
Operator : CG/JU
Sample : M4217-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGB5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

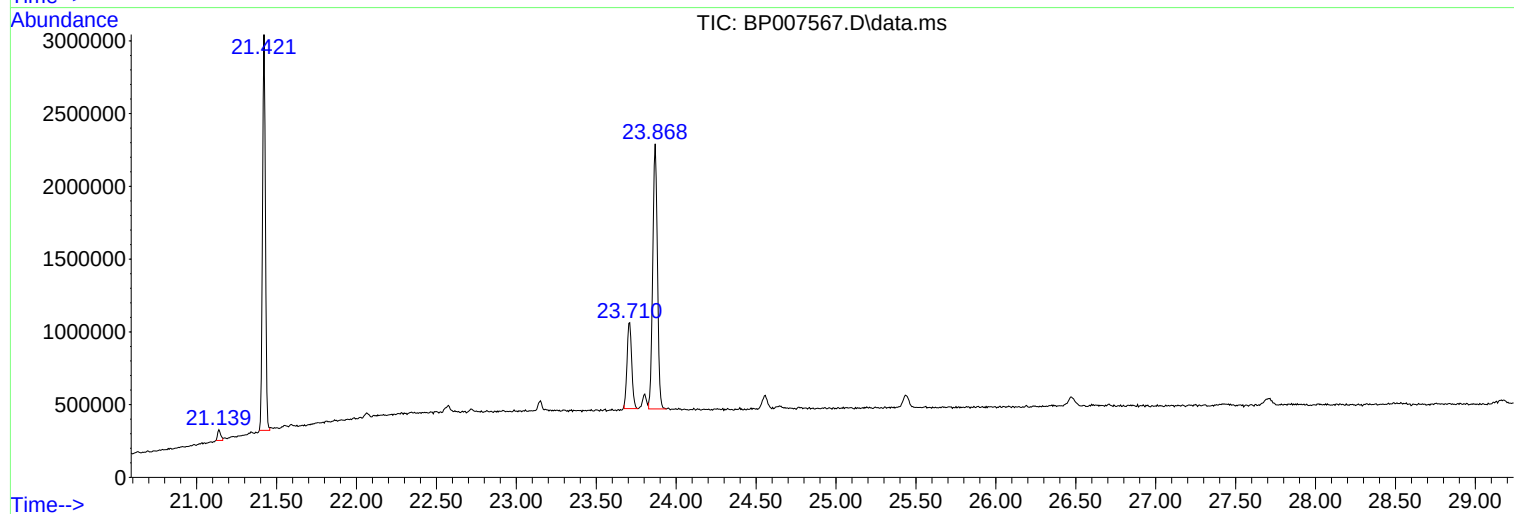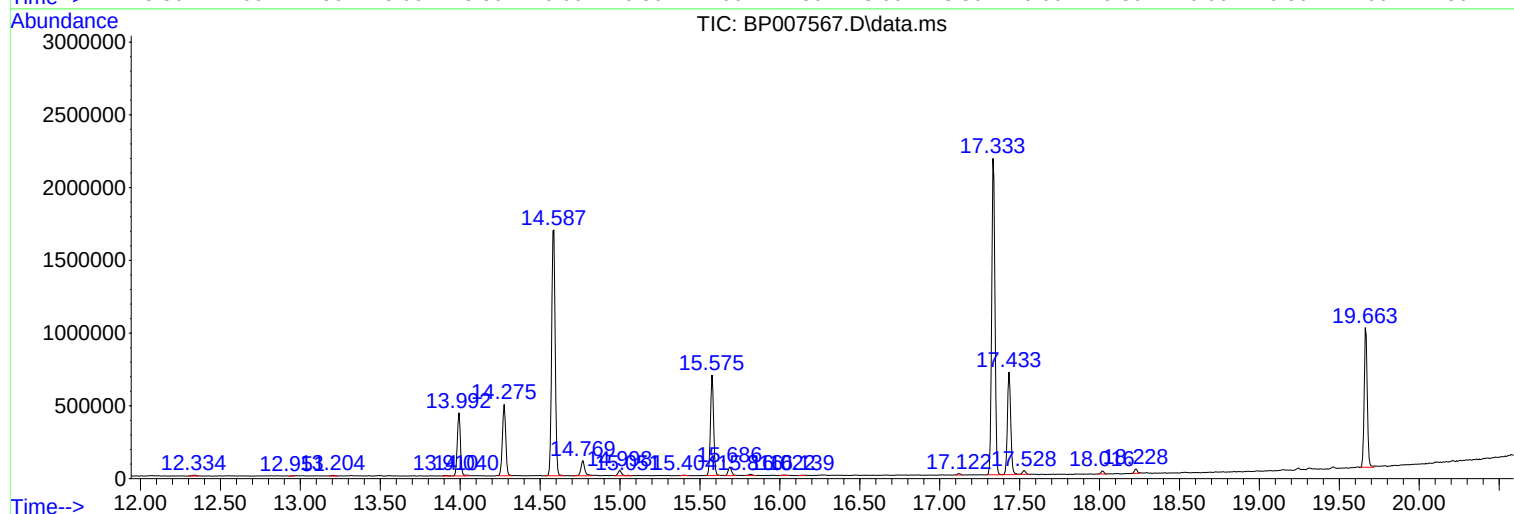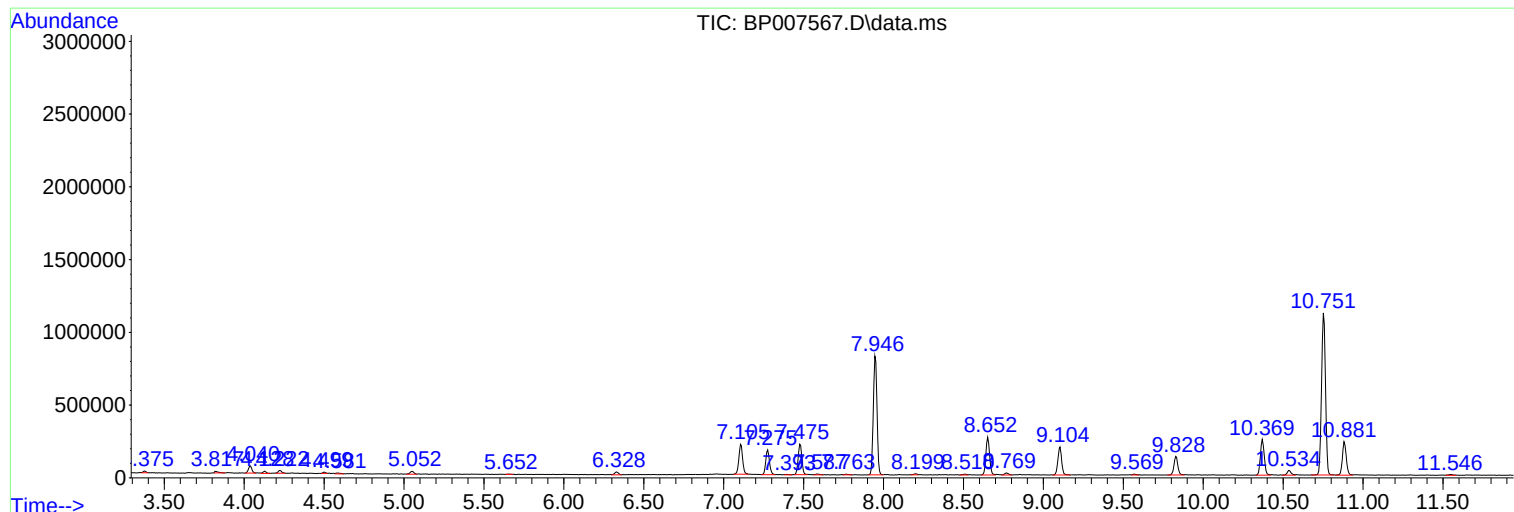

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007567.D
Acq On : 21 Oct 2021 22:37
Operator : CG/JU
Sample : M4217-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGB5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007567.D
Acq On : 21 Oct 2021 22:37
Operator : CG/JU
Sample : M4217-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGB5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
