

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007569.D
 Acq On : 22 Oct 2021 00:53
 Operator : CG/JU
 Sample : M4217-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007569.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.376	12	15	20	rVB	15973	19715	0.56%	0.073%
2	3.658	61	63	69	rBV7	5517	8363	0.24%	0.031%
3	3.805	86	88	99	rBV	51859	87543	2.50%	0.326%
4	4.040	122	128	135	rVB	53101	87417	2.50%	0.325%
5	4.128	139	143	150	rVV2	16292	23813	0.68%	0.089%
6	4.223	153	159	167	rVB3	21002	34473	0.99%	0.128%
7	4.505	202	207	211	rVB6	8885	12051	0.34%	0.045%
8	4.587	220	221	226	rVB3	8075	7729	0.22%	0.029%
9	4.922	276	278	283	rBV5	3414	4486	0.13%	0.017%
10	5.046	295	299	307	rVB	29726	44207	1.26%	0.164%
11	6.328	510	517	523	rBV2	20601	34925	1.00%	0.130%
12	6.605	561	564	568	rVB6	2717	3991	0.11%	0.015%
13	6.952	620	623	627	rBV5	3150	4683	0.13%	0.017%
14	7.105	641	649	660	rBV	248131	395713	11.31%	1.472%
15	7.275	672	678	686	rVB	206056	321626	9.19%	1.197%
16	7.475	704	712	724	rBV	247580	405522	11.59%	1.509%
17	7.587	727	731	737	rVB6	7412	11368	0.32%	0.042%
18	7.764	757	761	767	rBV4	5842	10522	0.30%	0.039%
19	7.946	785	792	801	rBV	743133	1190749	34.04%	4.430%
20	8.022	801	805	808	rVB6	2788	3924	0.11%	0.015%
21	8.099	815	818	822	rVB6	2859	4268	0.12%	0.016%
22	8.193	828	834	839	rBV6	8044	14689	0.42%	0.055%
23	8.505	882	887	890	rBV5	6591	10174	0.29%	0.038%
24	8.652	905	912	920	rBV	298227	469597	13.42%	1.747%
25	8.769	927	932	937	rBV	12885	23118	0.66%	0.086%
26	8.846	941	945	950	rBV8	2942	7346	0.21%	0.027%
27	9.105	982	989	996	rBV	215045	362265	10.35%	1.348%
28	9.281	1014	1019	1023	rBV8	5031	5789	0.17%	0.022%
29	9.569	1062	1068	1073	rVB5	6536	12121	0.35%	0.045%
30	9.681	1082	1087	1091	rVB8	2133	4003	0.11%	0.015%
31	9.828	1105	1112	1120	rBV	151853	255864	7.31%	0.952%
32	9.969	1130	1136	1140	rBV9	2499	4284	0.12%	0.016%
33	10.322	1189	1196	1197	rBV7	2720	4356	0.12%	0.016%
34	10.369	1197	1204	1214	rVV	291127	482793	13.80%	1.796%
35	10.534	1224	1232	1241	rBV	80108	135715	3.88%	0.505%
36	10.752	1261	1269	1283	rVB	1027791	1740554	49.75%	6.475%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007569.D
 Acq On : 22 Oct 2021 00:53
 Operator : CG/JU
 Sample : M4217-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	10.881	1283	1291	1300	rBV	266765	458193	13.10%	1.705%
38	11.546	1399	1404	1406	rBV6	4741	6423	0.18%	0.024%
39	12.069	1488	1493	1496	rBV7	3454	5196	0.15%	0.019%
40	12.340	1533	1539	1544	rBV5	6673	11690	0.33%	0.043%
41	12.957	1638	1644	1647	rBV7	4512	6698	0.19%	0.025%
42	13.199	1682	1685	1690	rVB6	5198	8776	0.25%	0.033%
43	13.316	1703	1705	1710	rBV5	3170	4361	0.12%	0.016%
44	13.428	1720	1724	1728	rBV7	2893	5099	0.15%	0.019%
45	13.493	1728	1735	1742	rVB7	4953	11327	0.32%	0.042%
46	13.557	1742	1746	1750	rBV7	3870	7031	0.20%	0.026%
47	13.910	1799	1806	1809	rBV9	4298	7168	0.20%	0.027%
48	13.993	1814	1820	1826	rBV	532726	730371	20.88%	2.717%
49	14.275	1858	1868	1877	rBV	597382	879851	25.15%	3.273%
50	14.581	1913	1920	1931	rVB	1631093	2450617	70.05%	9.117%
51	14.763	1941	1951	1962	rBV	88692	164955	4.72%	0.614%
52	14.998	1986	1991	2000	rVB3	33352	53026	1.52%	0.197%
53	15.404	2054	2060	2066	rBV9	5149	10810	0.31%	0.040%
54	15.575	2083	2089	2101	rVB	850894	1180187	33.73%	4.391%
55	15.687	2101	2108	2116	rBV	67491	102671	2.93%	0.382%
56	15.816	2126	2130	2135	rVB4	8649	14395	0.41%	0.054%
57	16.028	2161	2166	2170	rBV8	6421	8955	0.26%	0.033%
58	16.140	2182	2185	2190	rBV7	2786	3955	0.11%	0.015%
59	16.257	2201	2205	2209	rBV7	3900	4738	0.14%	0.018%
60	16.734	2283	2286	2290	rBV6	3368	4918	0.14%	0.018%
61	16.934	2317	2320	2324	rBV6	2208	3818	0.11%	0.014%
62	17.122	2346	2352	2356	rBV2	11569	18083	0.52%	0.067%
63	17.239	2368	2372	2377	rBV6	9100	15049	0.43%	0.056%
64	17.334	2380	2388	2398	rVV	2074441	2987856	85.40%	11.116%
65	17.434	2399	2405	2416	rVV	897381	1263770	36.12%	4.702%
66	17.528	2417	2421	2426	rVB5	25115	36456	1.04%	0.136%
67	18.016	2499	2504	2510	rBV2	35366	48009	1.37%	0.179%
68	18.116	2516	2521	2525	rBV7	8364	16676	0.48%	0.062%
69	18.169	2528	2530	2533	rBV4	5056	4582	0.13%	0.017%
70	18.228	2536	2540	2545	rBV2	44505	59529	1.70%	0.221%
71	18.522	2588	2590	2594	rVB5	6534	6907	0.20%	0.026%
72	19.457	2746	2749	2754	rBV7	20046	28149	0.80%	0.105%
73	19.663	2779	2784	2792	rBV	1159497	1561037	44.62%	5.807%
74	21.139	3032	3035	3039	rBV4	79643	103119	2.95%	0.384%
75	21.422	3078	3083	3089	rBV	2553222	3372520	96.40%	12.547%
76	23.704	3466	3471	3482	rVB	741829	1464552	41.86%	5.449%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007569.D
Acq On : 22 Oct 2021 00:53
Operator : CG/JU
Sample : M4217-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGG0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

77 23.869 3492 3499 3509 rVB2 1668217 3498496 100.00% 13.015%


Sum of corrected areas: 26879775

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007569.D
Acq On : 22 Oct 2021 00:53
Operator : CG/JU
Sample : M4217-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGG0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

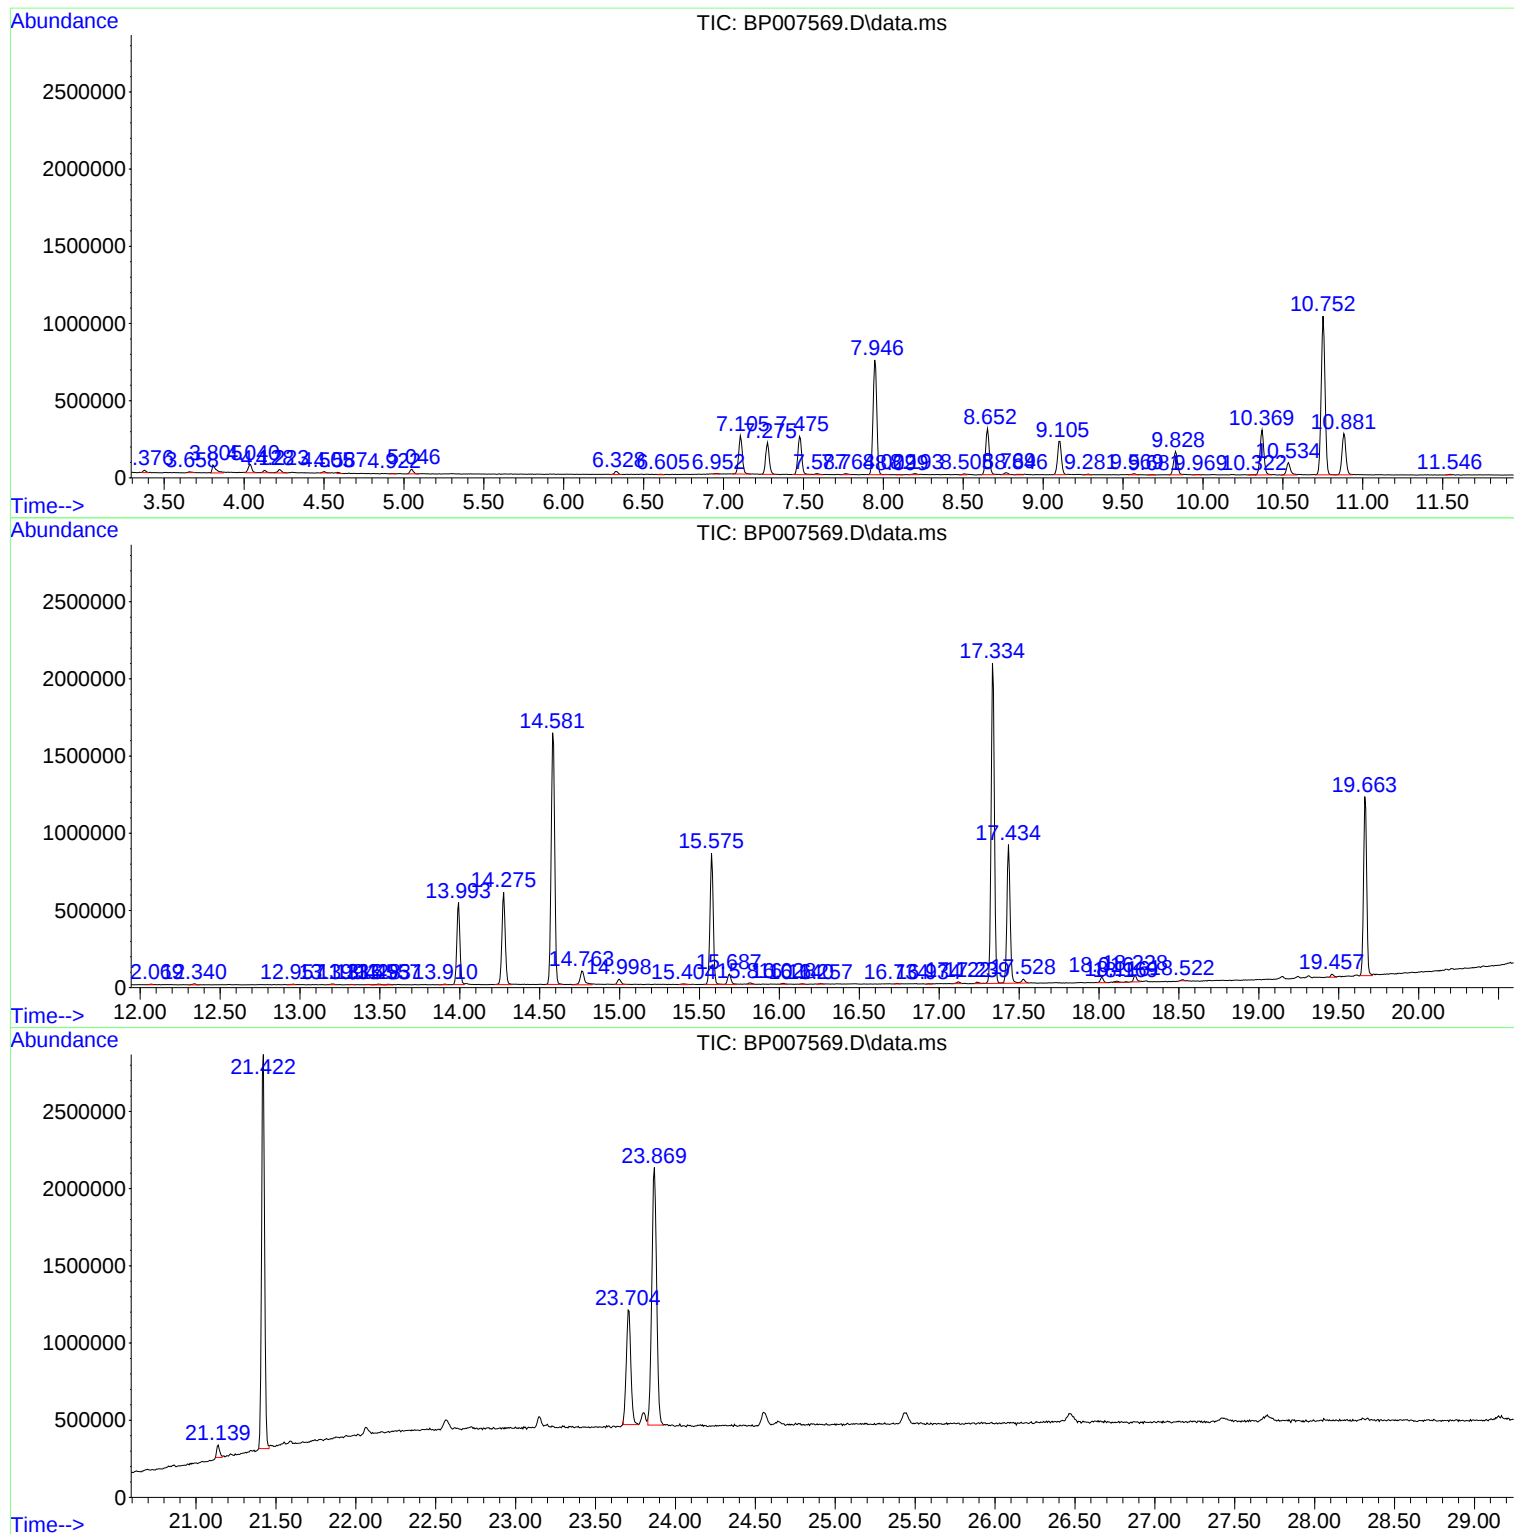

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007569.D
Acq On : 22 Oct 2021 00:53
Operator : CG/JU
Sample : M4217-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGG0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007569.D
Acq On : 22 Oct 2021 00:53
Operator : CG/JU
Sample : M4217-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGG0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
