

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007572.D
 Acq On : 22 Oct 2021 03:08
 Operator : CG/JU
 Sample : M4217-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	20	rVB2	15960	19636	0.55%	0.068%
2	3.658	61	63	69	rVB6	5816	7414	0.21%	0.026%
3	3.799	85	87	98	rBV	75646	117350	3.27%	0.406%
4	3.899	101	104	110	rVB2	15564	22348	0.62%	0.077%
5	4.034	123	127	135	rVB	47710	73604	2.05%	0.255%
6	4.128	138	143	148	rVB	21434	32412	0.90%	0.112%
7	4.222	155	159	164	rBV5	21375	30683	0.85%	0.106%
8	4.499	202	206	212	rVB8	8590	13084	0.36%	0.045%
9	5.046	294	299	304	rVB	27026	38699	1.08%	0.134%
10	5.652	400	402	407	rVB6	3712	4719	0.13%	0.016%
11	6.328	512	517	523	rVB	20155	31631	0.88%	0.109%
12	6.928	616	619	621	rBV4	3462	4521	0.13%	0.016%
13	7.105	641	649	660	rVB	256868	419047	11.67%	1.450%
14	7.275	671	678	689	rVB	215105	344376	9.59%	1.192%
15	7.475	706	712	719	rBV	262131	411913	11.47%	1.426%
16	7.569	725	728	729	rBV3	4626	4279	0.12%	0.015%
17	7.587	729	731	739	rVB7	6859	8771	0.24%	0.030%
18	7.763	757	761	766	rBV5	5792	7700	0.21%	0.027%
19	7.946	785	792	801	rBV	790737	1255119	34.96%	4.344%
20	8.087	811	816	817	rBV5	2487	3761	0.10%	0.013%
21	8.199	829	835	845	rBV5	8150	21291	0.59%	0.074%
22	8.446	874	877	881	rBV6	2659	4520	0.13%	0.016%
23	8.510	884	888	891	rVB6	4795	7869	0.22%	0.027%
24	8.652	904	912	922	rBV	308172	488500	13.60%	1.691%
25	8.769	926	932	939	rVB2	24350	43161	1.20%	0.149%
26	9.104	980	989	995	rBV	225912	378533	10.54%	1.310%
27	9.275	1017	1018	1024	rVV6	3727	5071	0.14%	0.018%
28	9.569	1064	1068	1072	rVB5	5663	10372	0.29%	0.036%
29	9.828	1105	1112	1120	rBV	158693	263248	7.33%	0.911%
30	10.069	1147	1153	1156	rBV8	3351	6143	0.17%	0.021%
31	10.193	1169	1174	1177	rVB7	3546	4346	0.12%	0.015%
32	10.322	1191	1196	1198	rBV2	4340	6066	0.17%	0.021%
33	10.369	1198	1204	1213	rVB	302581	493527	13.74%	1.708%
34	10.534	1226	1232	1241	rBV	122713	208003	5.79%	0.720%
35	10.751	1261	1269	1279	rBV	1080253	1811020	50.44%	6.268%
36	10.881	1284	1291	1302	rBV	266511	449429	12.52%	1.555%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007572.D
 Acq On : 22 Oct 2021 03:08
 Operator : CG/JU
 Sample : M4217-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGE3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	11.293	1359	1361	1366	rVB6	3681	3798	0.11%	0.013%
38	11.534	1399	1402	1403	rBV3	4294	4202	0.12%	0.015%
39	12.069	1488	1493	1496	rBV7	4477	7771	0.22%	0.027%
40	12.246	1517	1523	1528	rBV9	3516	7745	0.22%	0.027%
41	12.340	1531	1539	1543	rVV7	7498	13903	0.39%	0.048%
42	12.957	1638	1644	1649	rVV10	5352	10822	0.30%	0.037%
43	13.204	1680	1686	1689	rBV6	6409	9428	0.26%	0.033%
44	13.422	1720	1723	1727	rBV6	3129	4465	0.12%	0.015%
45	13.493	1730	1735	1740	rVV8	5919	9789	0.27%	0.034%
46	13.563	1742	1747	1750	rVB7	2664	4753	0.13%	0.016%
47	13.869	1794	1799	1801	rBV6	2932	4742	0.13%	0.016%
48	13.904	1801	1805	1809	rBV7	5540	9710	0.27%	0.034%
49	13.992	1813	1820	1827	rBV	525464	758546	21.13%	2.625%
50	14.040	1827	1828	1832	rVB4	6571	6631	0.18%	0.023%
51	14.275	1859	1868	1877	rBV	605528	904252	25.18%	3.130%
52	14.581	1912	1920	1931	rBV	1669289	2479284	69.05%	8.581%
53	14.763	1944	1951	1963	rBV	84480	146672	4.08%	0.508%
54	14.916	1972	1977	1981	rBV7	4450	9069	0.25%	0.031%
55	14.998	1986	1991	1996	rVV5	21218	33986	0.95%	0.118%
56	15.063	1999	2002	2007	rVB7	5014	6626	0.18%	0.023%
57	15.404	2055	2060	2063	rBV6	5550	9387	0.26%	0.032%
58	15.575	2082	2089	2100	rBV	855838	1238068	34.48%	4.285%
59	15.687	2102	2108	2114	rVV	67560	99764	2.78%	0.345%
60	15.816	2126	2130	2135	rVB6	11155	16852	0.47%	0.058%
61	16.022	2160	2165	2172	rVB10	5714	10832	0.30%	0.037%
62	16.128	2180	2183	2185	rBV4	2958	4037	0.11%	0.014%
63	16.257	2202	2205	2207	rVV4	3905	5082	0.14%	0.018%
64	16.310	2211	2214	2219	rVB6	4312	5628	0.16%	0.019%
65	16.457	2231	2239	2240	rBV8	3465	6068	0.17%	0.021%
66	16.481	2240	2243	2246	rVB5	2459	4345	0.12%	0.015%
67	16.739	2283	2287	2291	rBV7	9534	12546	0.35%	0.043%
68	17.081	2341	2345	2348	rBV6	9338	14199	0.40%	0.049%
69	17.122	2348	2352	2357	rVV2	12629	25537	0.71%	0.088%
70	17.163	2357	2359	2363	rVB5	7024	8289	0.23%	0.029%
71	17.233	2368	2371	2376	rBV6	13145	20435	0.57%	0.071%
72	17.333	2380	2388	2397	rVV	2078858	3039815	84.66%	10.521%
73	17.433	2398	2405	2413	rVV	935026	1328436	37.00%	4.598%
74	17.522	2417	2420	2427	rVB6	19362	32650	0.91%	0.113%
75	17.781	2460	2464	2465	rBV4	4812	6422	0.18%	0.022%
76	18.016	2501	2504	2509	rVB2	32091	38552	1.07%	0.133%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007572.D
 Acq On : 22 Oct 2021 03:08
 Operator : CG/JU
 Sample : M4217-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGE3

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

77	18.110	2514	2520	2525	rBV6	38310	78371	2.18%	0.271%
78	18.163	2527	2529	2534	rVB4	14114	19106	0.53%	0.066%
79	18.228	2536	2540	2548	rVV2	87859	123299	3.43%	0.427%
80	18.922	2655	2658	2661	rBV4	15729	23250	0.65%	0.080%
81	19.310	2721	2724	2727	rBV2	16302	20241	0.56%	0.070%
82	19.457	2745	2749	2754	rBV4	44626	60471	1.68%	0.209%
83	19.663	2779	2784	2792	rBV	1307924	1720501	47.92%	5.955%
84	20.204	2874	2876	2880	rVB4	30929	33585	0.94%	0.116%
85	21.139	3031	3035	3039	rBV3	128774	195556	5.45%	0.677%
86	21.416	3077	3082	3088	rBV	2667505	3491346	97.24%	12.083%
87	22.057	3189	3191	3198	rVB3	121620	171230	4.77%	0.593%
88	23.145	3372	3376	3380	rBV	228095	331799	9.24%	1.148%
89	23.704	3465	3471	3481	rVB	847235	1619295	45.10%	5.604%
90	23.863	3492	3498	3512	rVB2	1696503	3590613	100.00%	12.427%




Sum of corrected areas: 28893967

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007572.D
Acq On : 22 Oct 2021 03:08
Operator : CG/JU
Sample : M4217-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

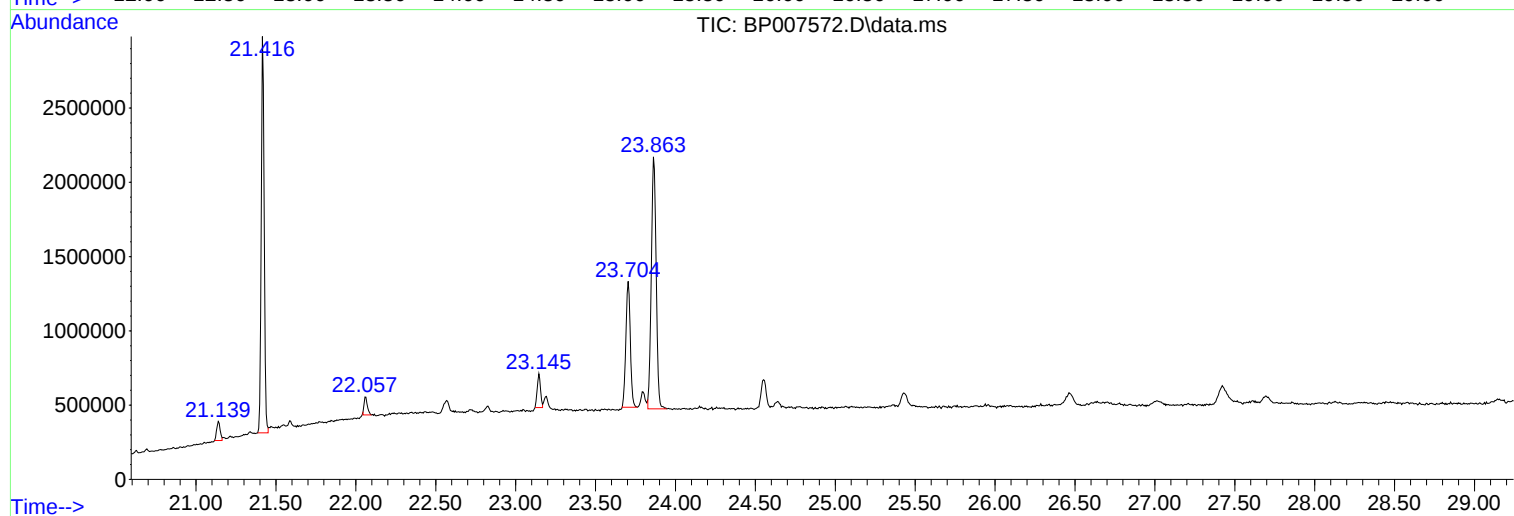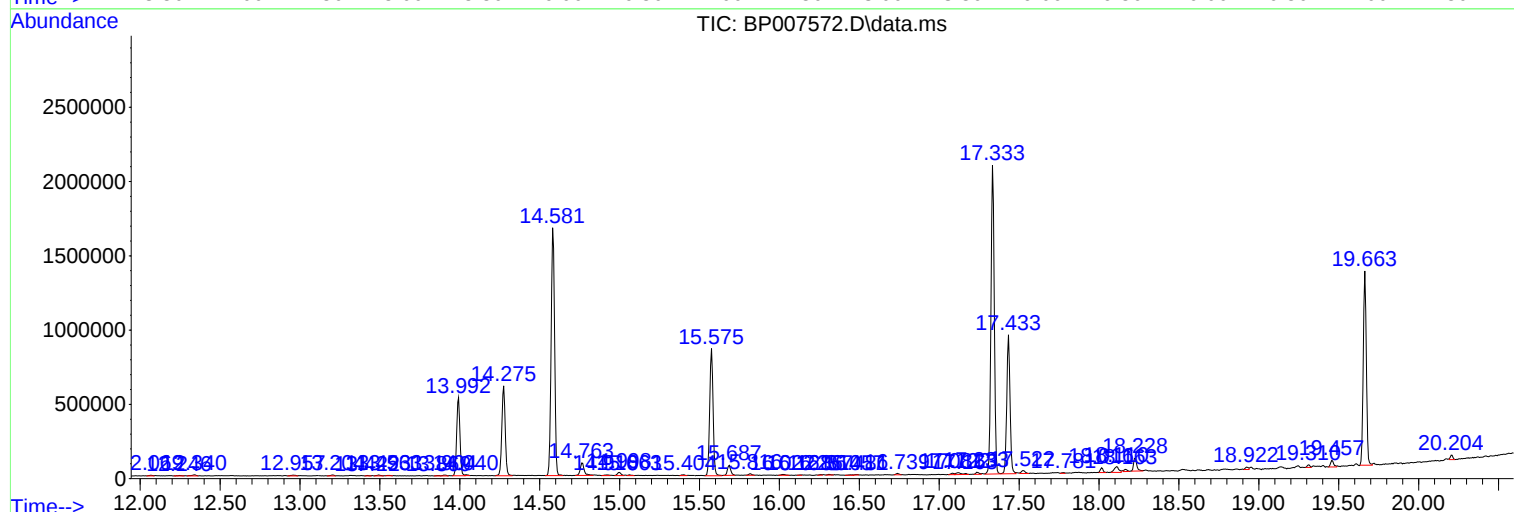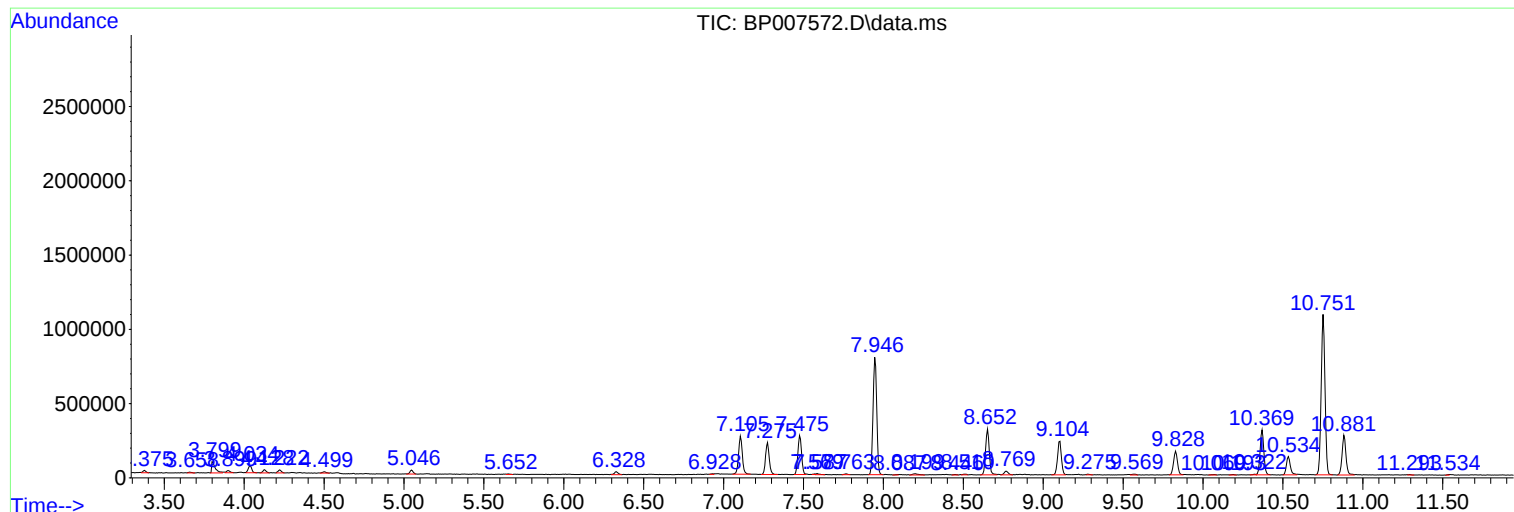

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007572.D
Acq On : 22 Oct 2021 03:08
Operator : CG/JU
Sample : M4217-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007572.D
Acq On : 22 Oct 2021 03:08
Operator : CG/JU
Sample : M4217-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGE3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
