

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007576.D
 Acq On : 22 Oct 2021 06:31
 Operator : CG/JU
 Sample : PB140021BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK021

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	22	rBV	62354	79196	1.43%	0.134%
2	3.787	83	85	103	rBV	805878	1256880	22.76%	2.124%
3	4.128	139	143	148	rBV	15295	22782	0.41%	0.039%
4	7.105	641	649	663	rBV	970316	1536813	27.83%	2.597%
5	7.275	669	678	686	rVB	757132	1190338	21.56%	2.012%
6	7.475	705	712	724	rBV	983157	1556954	28.20%	2.631%
7	7.946	785	792	800	rBV	855600	1358318	24.60%	2.296%
8	8.651	904	912	922	rBV	1196165	1922816	34.83%	3.250%
9	9.104	980	989	998	rBV	876473	1463831	26.51%	2.474%
10	9.828	1103	1112	1120	rBV	714754	1172983	21.24%	1.982%
11	10.369	1196	1204	1214	rBV	1169961	1966841	35.62%	3.324%
12	10.751	1260	1269	1282	rVB	1148370	1935614	35.06%	3.271%
13	10.881	1282	1291	1303	rBV	1133154	1913570	34.66%	3.234%
14	12.340	1532	1539	1546	rVB2	23263	39974	0.72%	0.068%
15	13.545	1741	1744	1751	rVB5	4627	9368	0.17%	0.016%
16	13.992	1813	1820	1833	rBV	2050117	2805809	50.82%	4.742%
17	14.275	1858	1868	1879	rBV	2311250	3411945	61.80%	5.766%
18	14.581	1913	1920	1930	rBV	1816679	2641500	47.84%	4.464%
19	14.763	1942	1951	1965	rBV	897701	1356787	24.57%	2.293%
20	15.228	2025	2030	2035	rBV9	4556	8640	0.16%	0.015%
21	15.575	2082	2089	2099	rBV	2902189	4257435	77.11%	7.195%
22	15.686	2101	2108	2119	rBV	639331	878446	15.91%	1.485%
23	15.816	2125	2130	2135	rVB	38075	55582	1.01%	0.094%
24	16.145	2182	2186	2191	rVB8	3522	6317	0.11%	0.011%
25	16.257	2200	2205	2210	rBV8	5751	10635	0.19%	0.018%
26	16.357	2220	2222	2229	rVB7	4235	8872	0.16%	0.015%
27	17.016	2328	2334	2338	rVB9	6947	11971	0.22%	0.020%
28	17.122	2346	2352	2355	rBV4	10124	16868	0.31%	0.029%
29	17.333	2381	2388	2398	rBV	2229959	3183703	57.66%	5.381%
30	17.433	2398	2405	2417	rBV	3276501	4658622	84.38%	7.873%
31	17.569	2425	2428	2435	rBV7	7690	14495	0.26%	0.024%
32	17.710	2447	2452	2456	rBV3	7539	14656	0.27%	0.025%
33	18.010	2499	2503	2508	rVB7	10811	15373	0.28%	0.026%
34	18.222	2536	2539	2543	rBV6	7301	11926	0.22%	0.020%
35	19.245	2709	2713	2719	rVB2	46716	63849	1.16%	0.108%
36	19.310	2721	2724	2729	rVB	46400	59053	1.07%	0.100%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007576.D
Acq On : 22 Oct 2021 06:31
Operator : CG/JU
Sample : PB140021BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK021

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	19.669	2779	2785	2792	rBV	4000020	5465721	98.99%	9.237%
38	21.421	3078	3083	3088	rBV	2802351	3563718	64.54%	6.023%
39	23.710	3465	3472	3482	rVB2	2817076	5521312	100.00%	9.331%
40	23.868	3492	3499	3508	rVB2	1757899	3701272	67.04%	6.255%




Sum of corrected areas: 59170785

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007576.D
Acq On : 22 Oct 2021 06:31
Operator : CG/JU
Sample : PB140021BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

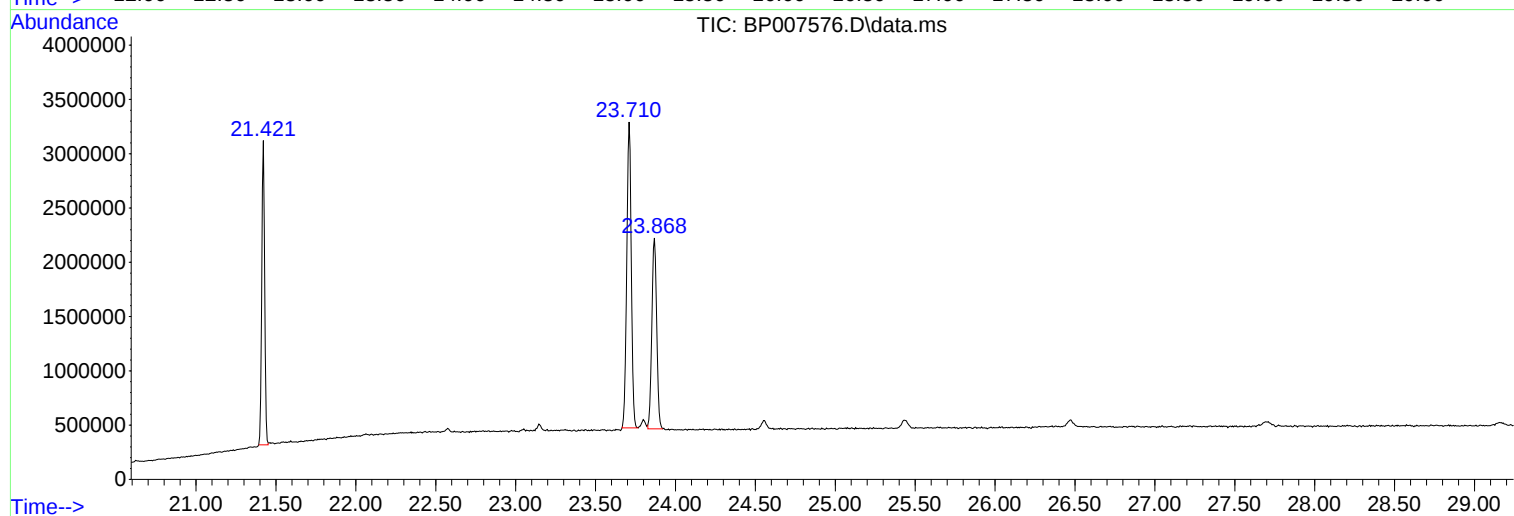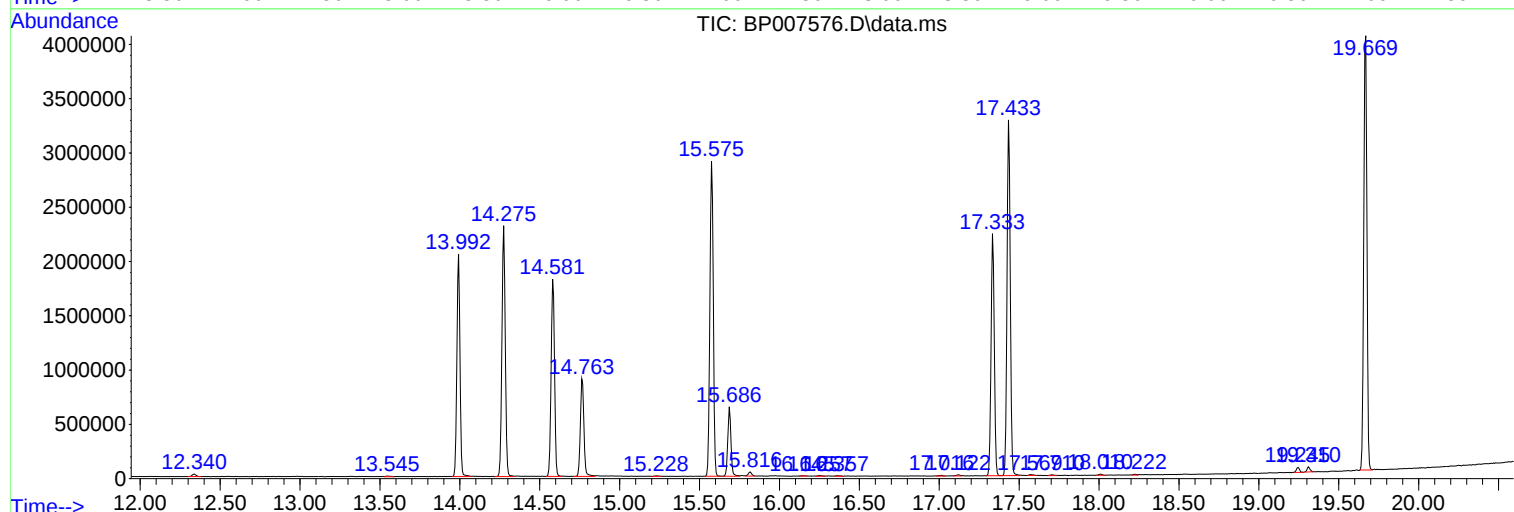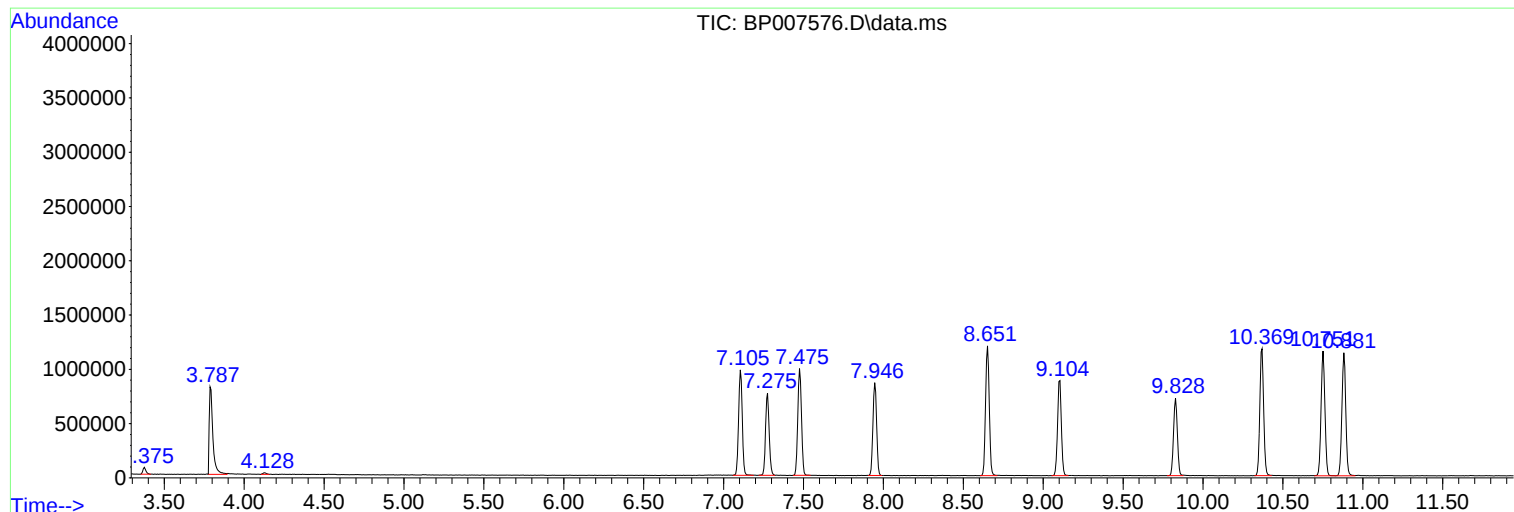

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007576.D
Acq On : 22 Oct 2021 06:31
Operator : CG/JU
Sample : PB140021BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007576.D
Acq On : 22 Oct 2021 06:31
Operator : CG/JU
Sample : PB140021BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
