

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007578.D
 Acq On : 22 Oct 2021 07:39
 Operator : CG/JU
 Sample : M4217-16
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGD3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	21	rVB4	16741	22938	0.60%	0.078%
2	3.658	59	63	68	rBV2	9614	14797	0.39%	0.050%
3	3.799	84	87	100	rBV	130705	206878	5.45%	0.699%
4	3.899	100	104	111	rVV	44592	62868	1.66%	0.213%
5	3.975	114	117	123	rVV4	10584	18224	0.48%	0.062%
6	4.034	123	127	137	rVB2	49695	78502	2.07%	0.265%
7	4.128	138	143	149	rVB	17183	26665	0.70%	0.090%
8	4.222	155	159	165	rVB3	18093	27196	0.72%	0.092%
9	4.499	202	206	210	rBV6	8426	12978	0.34%	0.044%
10	4.681	233	237	242	rVB5	7357	10515	0.28%	0.036%
11	4.840	259	264	268	rBV8	3119	6379	0.17%	0.022%
12	5.046	294	299	307	rVB	28428	43981	1.16%	0.149%
13	5.140	310	315	318	rBV4	7273	10940	0.29%	0.037%
14	6.328	512	517	522	rVB	19311	30164	0.79%	0.102%
15	6.528	546	551	553	rBV6	3236	3933	0.10%	0.013%
16	6.952	618	623	627	rBV7	3636	7298	0.19%	0.025%
17	7.105	641	649	658	rVV	255769	411370	10.83%	1.391%
18	7.275	669	678	689	rVB	198746	326557	8.60%	1.104%
19	7.475	706	712	720	rBV	256954	405107	10.67%	1.370%
20	7.581	723	730	736	rVB9	6638	15264	0.40%	0.052%
21	7.763	756	761	767	rVB2	5177	10380	0.27%	0.035%
22	7.946	785	792	800	rVV	816328	1277713	33.64%	4.320%
23	8.016	800	804	810	rVB8	4006	7467	0.20%	0.025%
24	8.199	825	835	840	rBV7	7916	17798	0.47%	0.060%
25	8.510	883	888	891	rBV6	4429	7002	0.18%	0.024%
26	8.652	904	912	919	rBV2	175146	297794	7.84%	1.007%
27	8.769	926	932	939	rBV	21196	36325	0.96%	0.123%
28	8.840	941	944	950	rVV8	2943	6976	0.18%	0.024%
29	9.104	981	989	996	rBV	221378	374597	9.86%	1.266%
30	9.281	1016	1019	1021	rBV4	3949	4286	0.11%	0.014%
31	9.569	1062	1068	1078	rVB8	6688	15255	0.40%	0.052%
32	9.828	1105	1112	1121	rBV	165384	276670	7.28%	0.935%
33	10.193	1169	1174	1177	rVB7	2880	5106	0.13%	0.017%
34	10.369	1194	1204	1213	rBV	296330	482839	12.71%	1.632%
35	10.534	1224	1232	1244	rBV	136694	234893	6.18%	0.794%
36	10.751	1261	1269	1281	rVB	1085031	1839328	48.43%	6.219%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007578.D
 Acq On : 22 Oct 2021 07:39
 Operator : CG/JU
 Sample : M4217-16
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	10.881	1284	1291	1299	rBV	251887	440672	11.60%	1.490%
38	11.287	1358	1360	1365	rVB6	4110	5203	0.14%	0.018%
39	11.545	1397	1404	1407	rBV8	4544	8983	0.24%	0.030%
40	12.245	1520	1523	1526	rBV5	3781	4070	0.11%	0.014%

41	12.334	1532	1538	1546	rVB4	7940	16172	0.43%	0.055%
42	12.957	1640	1644	1646	rBV4	5986	8656	0.23%	0.029%
43	13.204	1681	1686	1692	rVB8	8715	13127	0.35%	0.044%
44	13.322	1700	1706	1708	rBV7	3491	5454	0.14%	0.018%
45	13.492	1730	1735	1740	rBV3	7494	12872	0.34%	0.044%

46	13.904	1801	1805	1808	rBV6	4712	5287	0.14%	0.018%
47	13.992	1814	1820	1827	rBV	549420	746277	19.65%	2.523%
48	14.275	1858	1868	1877	rBV	618022	901290	23.73%	3.047%
49	14.581	1913	1920	1931	rBV	1698803	2529919	66.61%	8.554%
50	14.763	1943	1951	1964	rBV	182512	296362	7.80%	1.002%

51	14.922	1974	1978	1981	rBV6	3672	5860	0.15%	0.020%
52	14.998	1986	1991	1996	rVB5	23593	33850	0.89%	0.114%
53	15.398	2054	2059	2063	rBV2	24118	34022	0.90%	0.115%
54	15.575	2082	2089	2098	rBV	857736	1225530	32.27%	4.143%
55	15.686	2102	2108	2115	rBV	109601	157817	4.16%	0.534%

56	15.816	2126	2130	2137	rVB3	8592	13408	0.35%	0.045%
57	16.022	2160	2165	2170	rBV9	7368	16058	0.42%	0.054%
58	16.275	2198	2208	2211	rBV9	4845	12228	0.32%	0.041%
59	16.339	2216	2219	2223	rVV4	6146	8132	0.21%	0.027%
60	16.480	2238	2243	2245	rVV6	3591	5333	0.14%	0.018%

61	16.739	2285	2287	2292	rVB5	5108	6448	0.17%	0.022%
62	16.880	2306	2311	2314	rBV2	17588	23445	0.62%	0.079%
63	17.122	2347	2352	2356	rBV2	12078	18585	0.49%	0.063%
64	17.169	2356	2360	2363	rVV5	5775	8986	0.24%	0.030%
65	17.333	2381	2388	2399	rBV	2189788	3079426	81.08%	10.411%

66	17.433	2399	2405	2416	rVV2	935622	1322154	34.81%	4.470%
67	17.528	2416	2421	2428	rVB9	25594	42531	1.12%	0.144%
68	17.845	2473	2475	2478	rBV4	4346	5096	0.13%	0.017%
69	18.016	2500	2504	2510	rVB	50475	67872	1.79%	0.229%
70	18.227	2536	2540	2547	rBV2	101743	140896	3.71%	0.476%

71	19.145	2693	2696	2701	rVB	46624	49583	1.31%	0.168%
72	19.245	2710	2713	2716	rBV4	16400	21512	0.57%	0.073%
73	19.274	2716	2718	2721	rBV3	14278	17999	0.47%	0.061%
74	19.457	2746	2749	2755	rBV4	45225	62519	1.65%	0.211%
75	19.663	2779	2784	2792	rBV	1349600	1787496	47.06%	6.043%

76	20.569	2935	2938	2942	rBV	219564	252550	6.65%	0.854%
----	--------	------	------	------	-----	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007578.D
Acq On : 22 Oct 2021 07:39
Operator : CG/JU
Sample : M4217-16
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

77	20.957	3001	3004	3006	rBV	59913	67490	1.78%	0.228%
78	21.139	3032	3035	3039	rBV4	125512	166232	4.38%	0.562%
79	21.339	3066	3069	3073	rBV	139533	163461	4.30%	0.553%
80	21.421	3078	3083	3089	rVV	2766892	3600280	94.80%	12.172%
81	23.704	3465	3471	3480	rVB2	851228	1731334	45.59%	5.854%
82	23.868	3492	3499	3513	rVB2	1792584	3797960	100.00%	12.841%




Sum of corrected areas: 29577420

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007578.D
Acq On : 22 Oct 2021 07:39
Operator : CG/JU
Sample : M4217-16
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

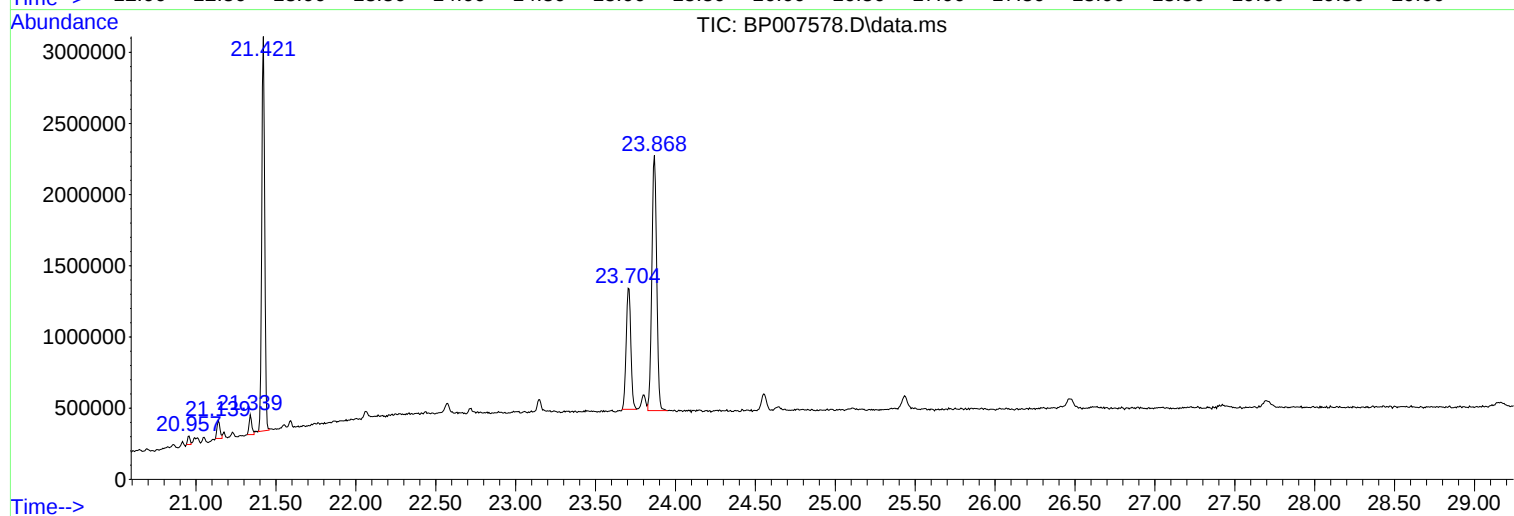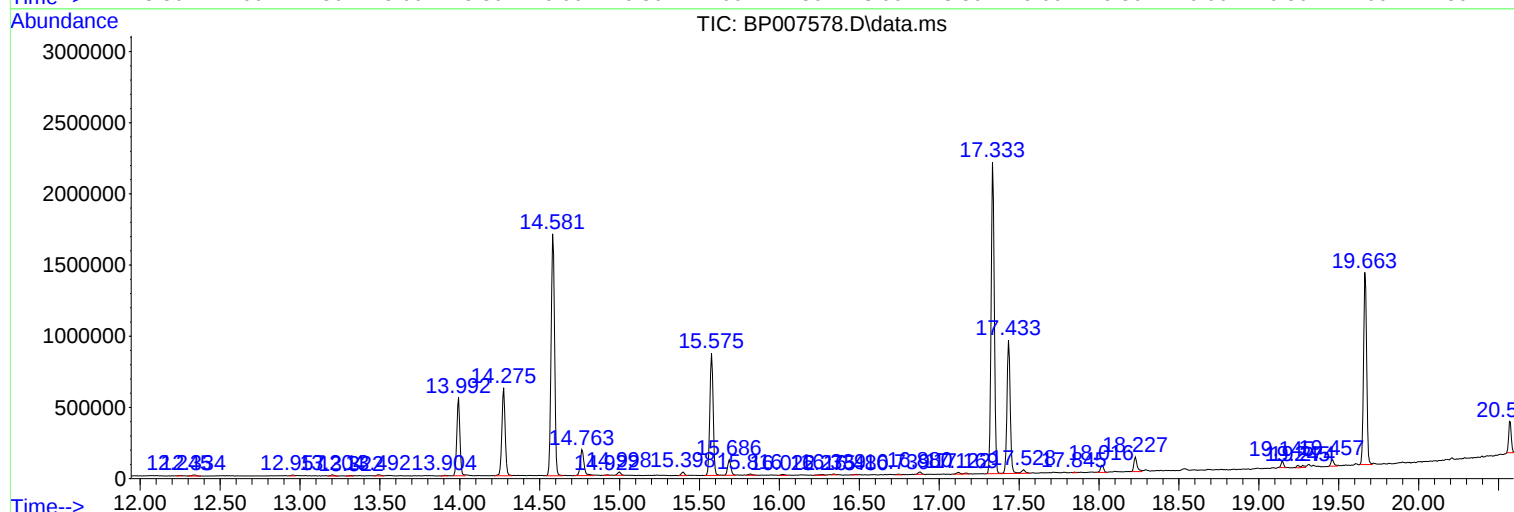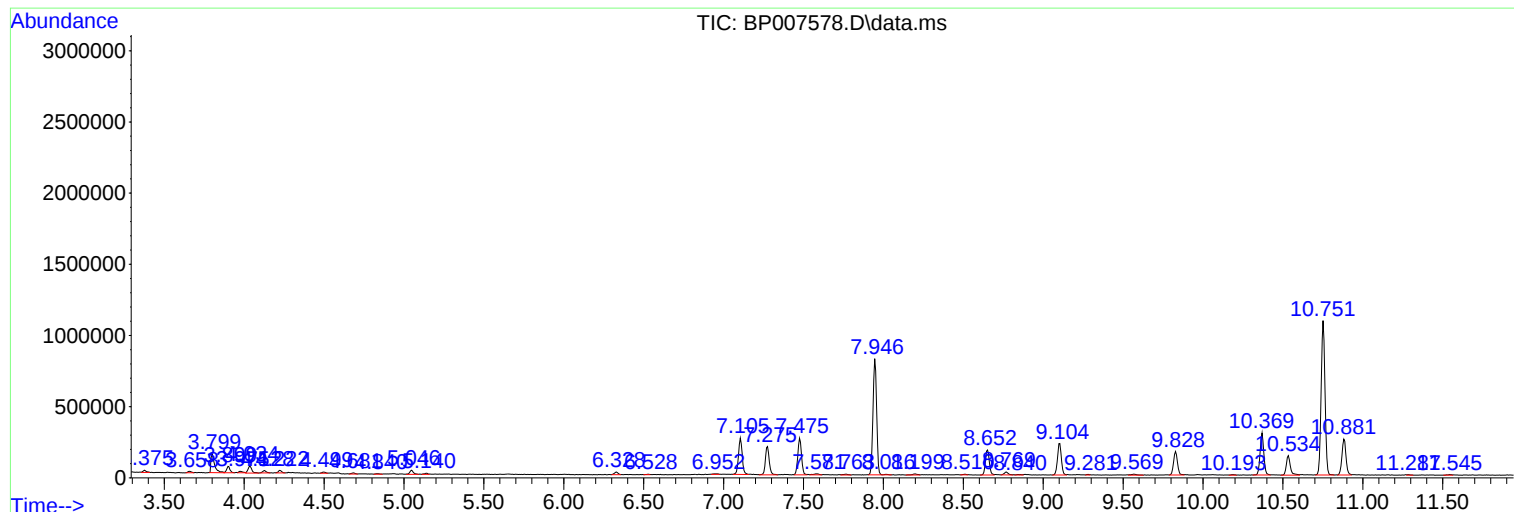

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007578.D
Acq On : 22 Oct 2021 07:39
Operator : CG/JU
Sample : M4217-16
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD3










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.534	2.55 ng/ul	234893	Naphthalene-d8	10.751

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

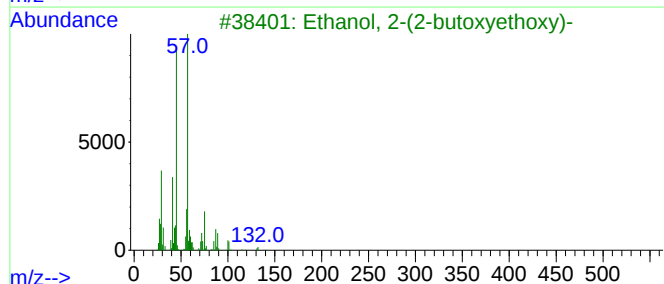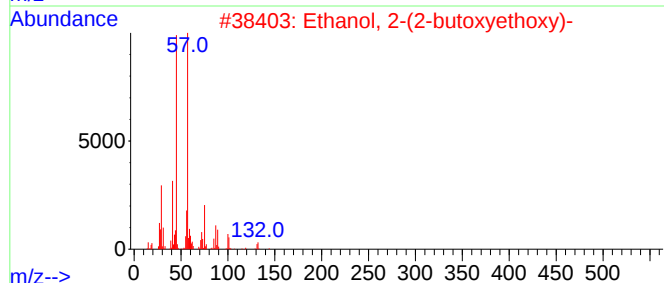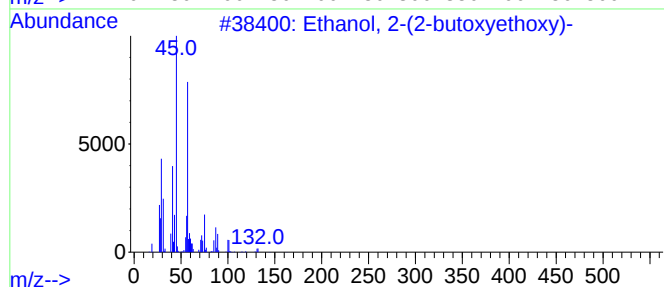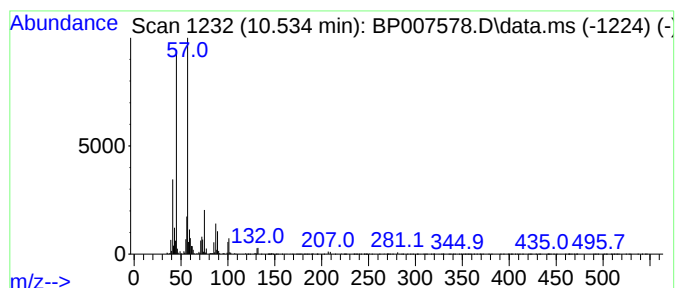

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007578.D
Acq On : 22 Oct 2021 07:39
Operator : CG/JU
Sample : M4217-16
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.534	2.5	ng/u1	234893	2	10.751	1839330	20.0