

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007581.D
 Acq On : 22 Oct 2021 09:27
 Operator : CG/JU
 Sample : PB140090BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	21	rBV	64356	83628	1.39%	0.140%
2	3.458	25	29	38	rVB2	13817	32617	0.54%	0.055%
3	3.787	82	85	107	rBV	866480	1360968	22.69%	2.281%
4	4.128	139	143	149	rVB	13938	21821	0.36%	0.037%
5	5.122	309	312	319	rVB8	5263	9204	0.15%	0.015%
6	7.104	642	649	659	rVB	995977	1600374	26.68%	2.682%
7	7.275	671	678	689	rVB	791707	1233397	20.56%	2.067%
8	7.475	705	712	723	rBV	1009112	1611102	26.86%	2.700%
9	7.946	786	792	800	rVB	714230	1132594	18.88%	1.898%
10	8.651	904	912	927	rBV	1247994	2010316	33.51%	3.369%
11	9.104	981	989	998	rBV	931661	1517548	25.30%	2.543%
12	9.828	1102	1112	1120	rBV	723578	1206422	20.11%	2.022%
13	10.369	1194	1204	1218	rBV	1254497	2074744	34.59%	3.477%
14	10.751	1260	1269	1279	rVB	984401	1641357	27.36%	2.751%
15	10.887	1284	1292	1306	rBV	1140669	2058150	34.31%	3.449%
16	12.339	1533	1539	1548	rVB	26676	44181	0.74%	0.074%
17	13.551	1740	1745	1751	rVB6	5778	10145	0.17%	0.017%
18	13.992	1813	1820	1835	rBV	2046098	3000228	50.02%	5.028%
19	14.275	1861	1868	1878	rBV	2406186	3562833	59.40%	5.971%
20	14.586	1912	1921	1931	rBV	1496907	2260358	37.68%	3.788%
21	14.769	1945	1952	1966	rBV	1008364	1471040	24.52%	2.465%
22	15.004	1988	1992	1996	rVB7	4695	6862	0.11%	0.012%
23	15.233	2028	2031	2035	rBV6	3928	6999	0.12%	0.012%
24	15.580	2083	2090	2098	rBV	3156868	4481436	74.71%	7.511%
25	15.692	2102	2109	2121	rVV	674727	939734	15.67%	1.575%
26	15.822	2124	2131	2136	rVB2	36611	60286	1.01%	0.101%
27	15.951	2149	2153	2159	rBV9	4948	7824	0.13%	0.013%
28	16.145	2178	2186	2188	rBV8	5248	9328	0.16%	0.016%
29	16.263	2200	2206	2211	rVB9	7348	12712	0.21%	0.021%
30	16.363	2220	2223	2227	rBV6	4576	6664	0.11%	0.011%
31	17.016	2331	2334	2339	rVB7	6214	9378	0.16%	0.016%
32	17.121	2348	2352	2359	rVB2	8221	12825	0.21%	0.021%
33	17.339	2382	2389	2398	rBV	1904022	2701116	45.03%	4.527%
34	17.439	2399	2406	2424	rVV	3462143	5023238	83.74%	8.419%
35	17.580	2426	2430	2434	rBV7	6355	10039	0.17%	0.017%
36	17.710	2449	2452	2456	rBV4	5572	7076	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007581.D
Acq On : 22 Oct 2021 09:27
Operator : CG/JU
Sample : PB140090BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK090

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	18.227	2537	2540	2544	rBV6	8063	12353	0.21%	0.021%
38	18.539	2589	2593	2596	rBV5	5381	9682	0.16%	0.016%
39	19.251	2709	2714	2719	rBV2	51342	71607	1.19%	0.120%
40	19.315	2721	2725	2735	rBV	51455	81542	1.36%	0.137%
41	19.668	2779	2785	2793	rBV	4217219	5932090	98.89%	9.942%
42	21.421	3078	3083	3090	rBV	2315774	3123655	52.07%	5.235%
43	23.715	3466	3473	3484	rVB2	3016707	5998469	100.00%	10.053%
44	23.874	3493	3500	3511	rVB2	1583485	3197816	53.31%	5.360%




Sum of corrected areas: 59665758

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007581.D
Acq On : 22 Oct 2021 09:27
Operator : CG/JU
Sample : PB140090BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK090

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

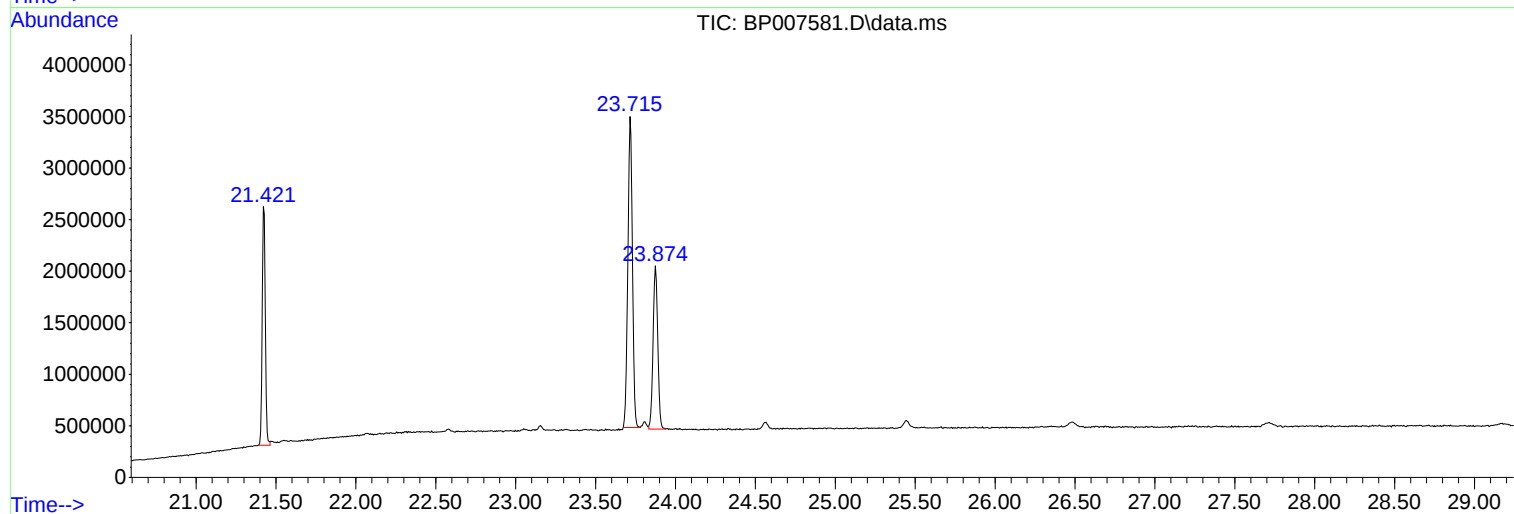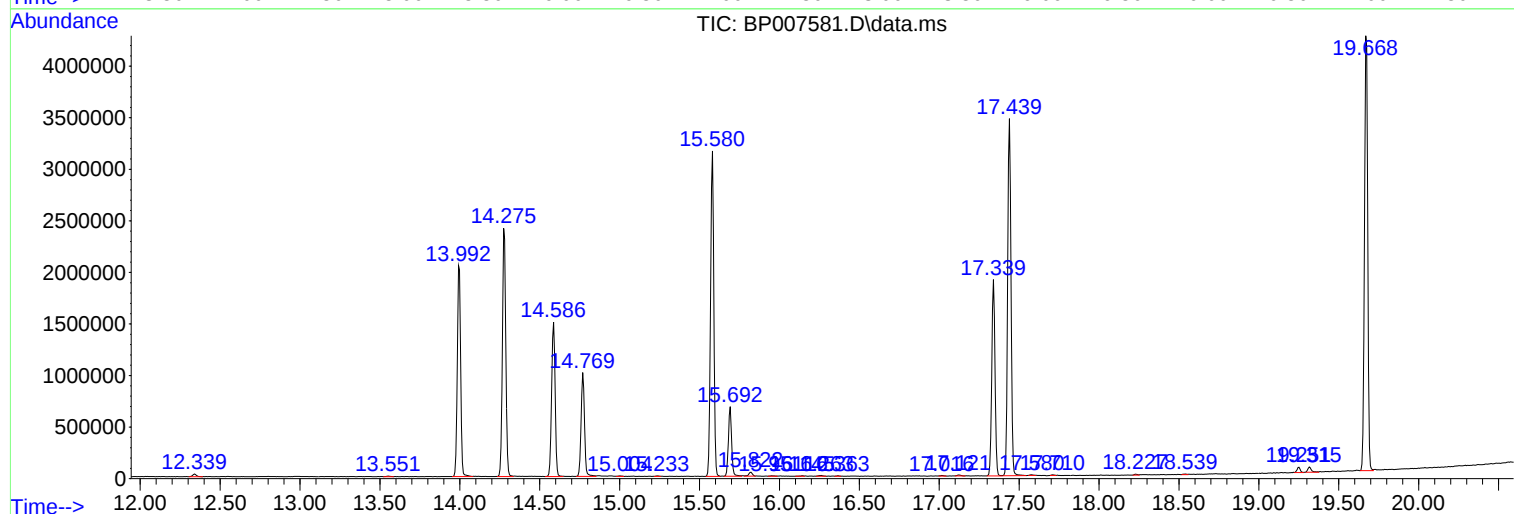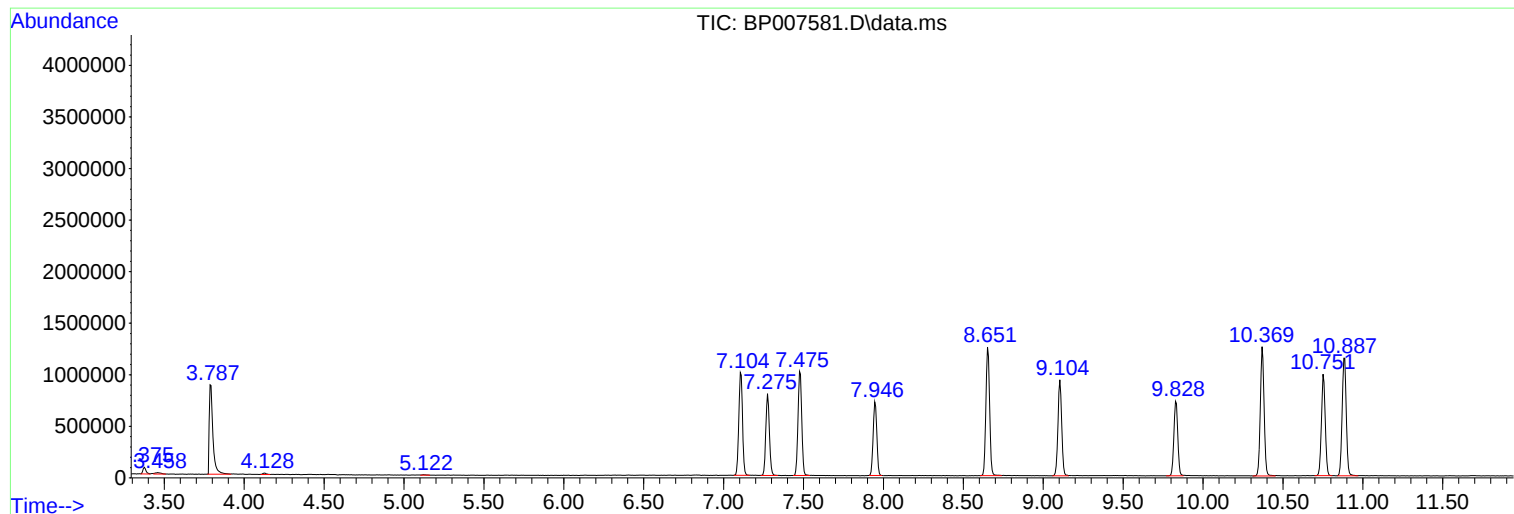

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007581.D
Acq On : 22 Oct 2021 09:27
Operator : CG/JU
Sample : PB140090BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK090

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007581.D
Acq On : 22 Oct 2021 09:27
Operator : CG/JU
Sample : PB140090BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK090

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
