

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007587.D
 Acq On : 22 Oct 2021 13:33
 Operator : CG/JU
 Sample : M4281-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	20	rVB	45898	54204	0.96%	0.112%
2	3.657	60	63	70	rVB3	5968	9137	0.16%	0.019%
3	3.793	83	86	99	rBV	239937	381849	6.77%	0.787%
4	4.034	123	127	132	rVB	27959	40584	0.72%	0.084%
5	4.128	139	143	152	rBV2	13083	21179	0.38%	0.044%
6	4.222	154	159	164	rBV5	13297	21020	0.37%	0.043%
7	4.499	203	206	211	rVB7	3768	6643	0.12%	0.014%
8	5.052	297	300	305	rVB4	5264	7946	0.14%	0.016%
9	6.034	463	467	471	rVB4	6802	8819	0.16%	0.018%
10	6.328	513	517	523	rVB3	10545	17356	0.31%	0.036%
11	7.104	641	649	659	rVB	194560	321749	5.70%	0.663%
12	7.275	671	678	689	rVB	632582	1005706	17.83%	2.073%
13	7.475	705	712	724	rBV	663529	1037110	18.39%	2.138%
14	7.581	724	730	733	rBV8	4711	8598	0.15%	0.018%
15	7.945	780	792	799	rBV	628195	991506	17.58%	2.044%
16	8.016	801	804	812	rVB3	8144	14188	0.25%	0.029%
17	8.193	831	834	840	rBV7	4347	5896	0.10%	0.012%
18	8.510	883	888	893	rBV9	4375	7606	0.13%	0.016%
19	8.651	904	912	921	rBV	543626	855037	15.16%	1.763%
20	9.104	981	989	998	rBV	734536	1214927	21.54%	2.505%
21	9.569	1061	1068	1073	rVB3	9849	18044	0.32%	0.037%
22	9.828	1103	1112	1123	rBV	569911	937004	16.61%	1.932%
23	10.369	1196	1204	1215	rBV	956076	1526030	27.06%	3.146%
24	10.534	1225	1232	1244	rBV	92954	171625	3.04%	0.354%
25	10.751	1259	1269	1279	rBV	852981	1431207	25.38%	2.950%
26	10.881	1283	1291	1301	rBV	848243	1429034	25.34%	2.946%
27	12.069	1488	1493	1499	rBV5	6690	11125	0.20%	0.023%
28	12.339	1534	1539	1551	rBV3	19010	36386	0.65%	0.075%
29	13.428	1720	1724	1729	rVB8	6172	8855	0.16%	0.018%
30	13.498	1729	1736	1740	rBV8	7264	12314	0.22%	0.025%
31	13.892	1798	1803	1810	rBV4	9605	15717	0.28%	0.032%
32	13.992	1813	1820	1827	rBV	1850941	2509368	44.49%	5.173%
33	14.116	1837	1841	1846	rVB7	4786	8208	0.15%	0.017%
34	14.275	1856	1868	1876	rBV	1944441	2884914	51.15%	5.947%
35	14.580	1913	1920	1932	rBV	1293159	1975350	35.02%	4.072%
36	14.763	1943	1951	1958	rBV	154143	258835	4.59%	0.534%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007587.D
 Acq On : 22 Oct 2021 13:33
 Operator : CG/JU
 Sample : M4281-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	15.004	1986	1992	1996	rBV8	7359	12651	0.22%	0.026%
38	15.127	2010	2013	2018	rVB4	4433	5991	0.11%	0.012%
39	15.233	2026	2031	2033	rBV6	4488	7227	0.13%	0.015%
40	15.398	2054	2059	2065	rBV8	4003	7693	0.14%	0.016%
41	15.574	2081	2089	2098	rBV	2610505	3887130	68.92%	8.013%
42	15.686	2102	2108	2122	rVV	629116	883596	15.67%	1.822%
43	15.816	2125	2130	2135	rVB2	32776	52269	0.93%	0.108%
44	16.027	2161	2166	2169	rBV7	6042	8710	0.15%	0.018%
45	16.139	2182	2185	2194	rVB7	4800	9305	0.16%	0.019%
46	16.251	2201	2204	2211	rVB9	4933	11126	0.20%	0.023%
47	16.363	2220	2223	2229	rVB8	7697	9939	0.18%	0.020%
48	16.492	2239	2245	2246	rBV6	3379	5857	0.10%	0.012%
49	16.598	2258	2263	2266	rBV7	3842	6903	0.12%	0.014%
50	16.739	2283	2287	2293	rBV8	7129	11847	0.21%	0.024%
51	17.016	2327	2334	2337	rBV9	5771	13356	0.24%	0.028%
52	17.121	2345	2352	2356	rBV2	10441	19929	0.35%	0.041%
53	17.333	2381	2388	2398	rBV	1627366	2379591	42.19%	4.906%
54	17.433	2398	2405	2417	rBV	3194538	4551138	80.69%	9.382%
55	17.569	2426	2428	2433	rVB5	7135	10987	0.19%	0.023%
56	17.704	2448	2451	2456	rBV5	4138	7223	0.13%	0.015%
57	17.963	2492	2495	2498	rVB5	12650	14499	0.26%	0.030%
58	18.021	2501	2505	2511	rVB	21255	29190	0.52%	0.060%
59	18.227	2536	2540	2549	rBV2	130075	172332	3.06%	0.355%
60	18.292	2549	2551	2557	rVB5	7491	12317	0.22%	0.025%
61	19.245	2709	2713	2718	rBV2	47511	67445	1.20%	0.139%
62	19.315	2721	2725	2729	rVV	44534	60960	1.08%	0.126%
63	19.463	2746	2750	2754	rBV4	30720	42132	0.75%	0.087%
64	19.668	2779	2785	2792	rBV	4100316	5579109	98.92%	11.502%
65	21.145	3032	3036	3040	rBV4	102838	154128	2.73%	0.318%
66	21.421	3078	3083	3089	rBV	2002394	2740241	48.58%	5.649%
67	23.715	3465	3473	3483	rBV2	2760495	5640130	100.00%	11.627%
68	23.868	3493	3499	3511	rVB2	1340200	2827278	50.13%	5.829%




Sum of corrected areas: 48507305

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007587.D
Acq On : 22 Oct 2021 13:33
Operator : CG/JU
Sample : M4281-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY63

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

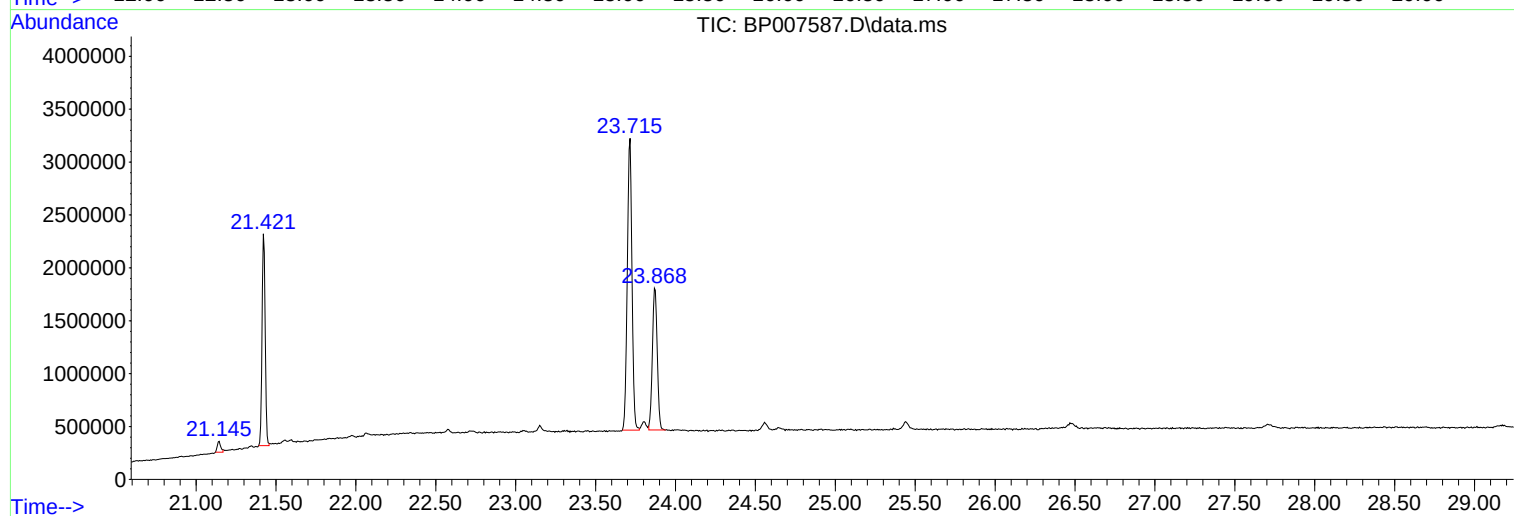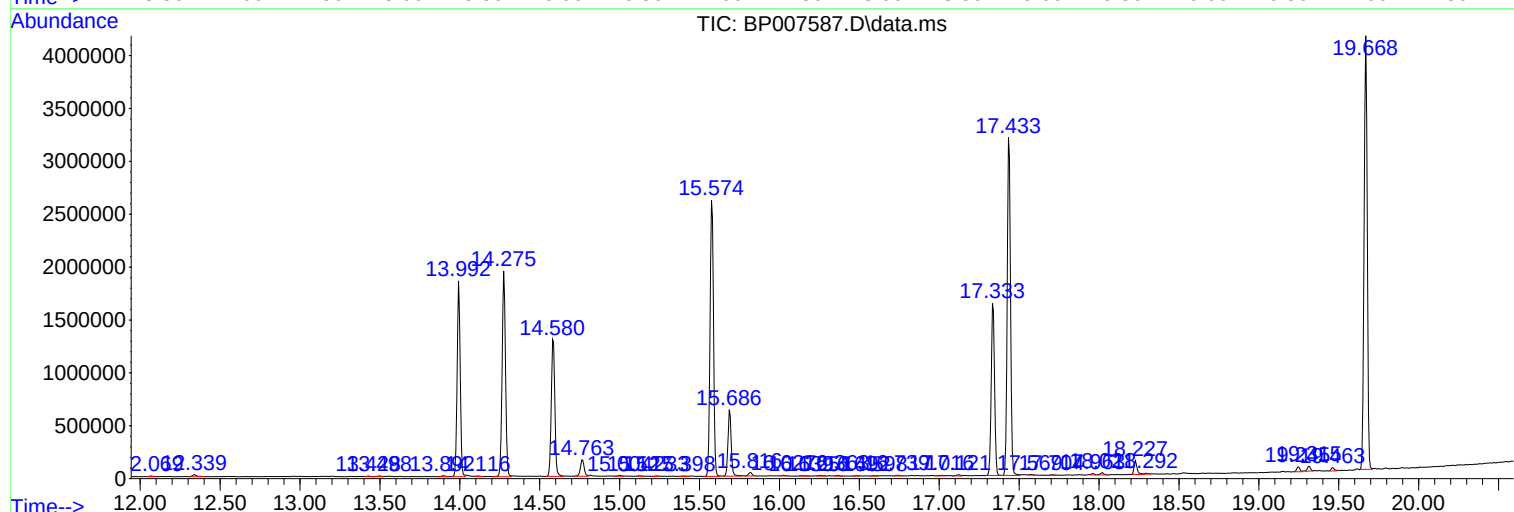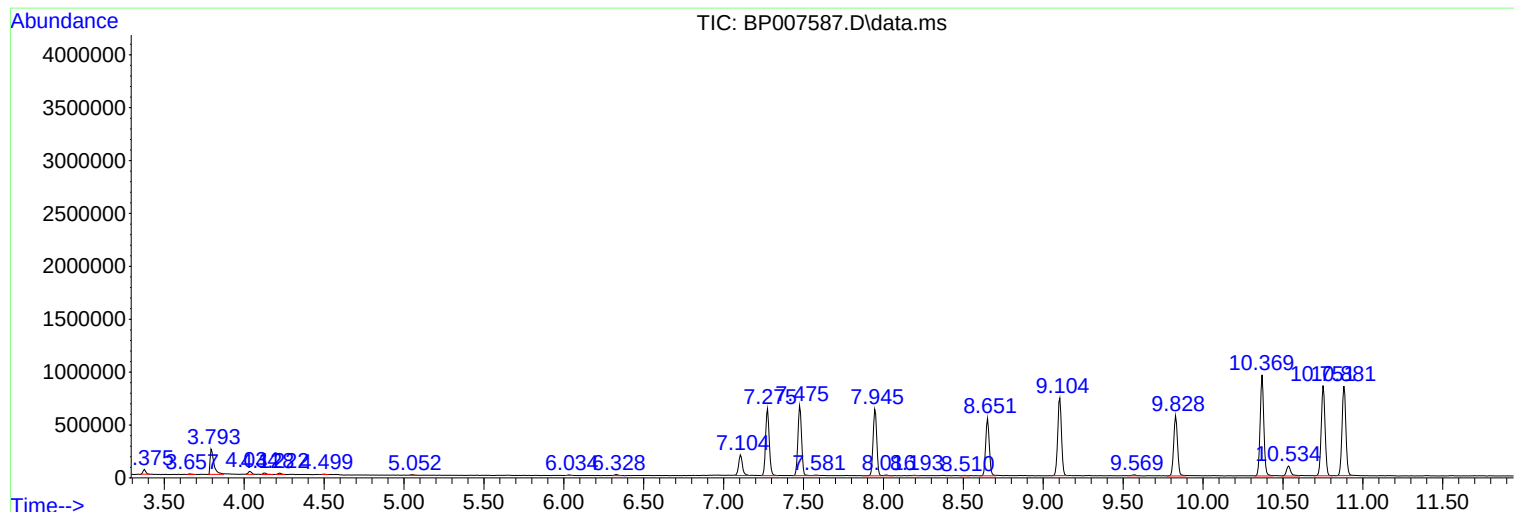

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007587.D
Acq On : 22 Oct 2021 13:33
Operator : CG/JU
Sample : M4281-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY63










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.534	2.40 ng/ul	171625	Naphthalene-d8	10.751

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90

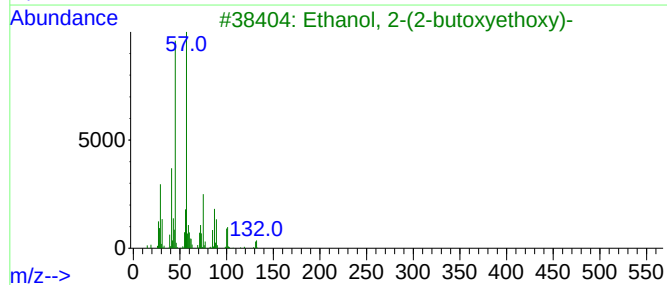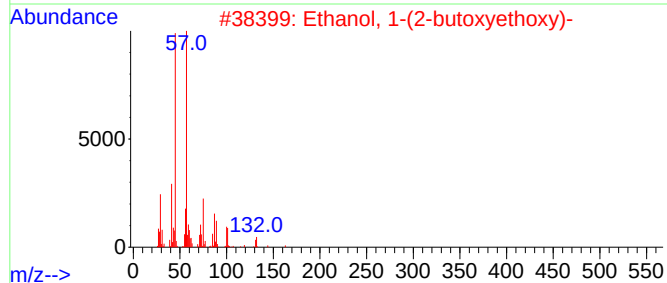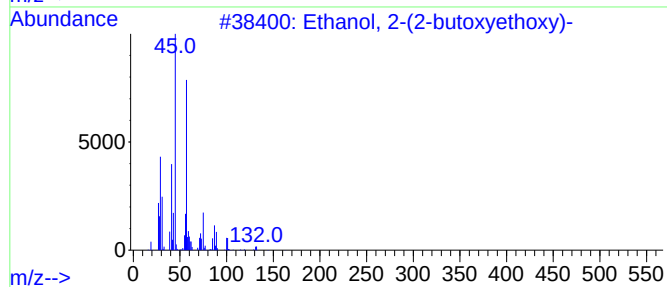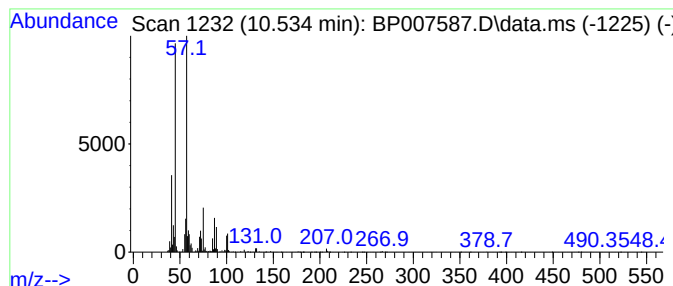

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007587.D
Acq On : 22 Oct 2021 13:33
Operator : CG/JU
Sample : M4281-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY63

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.534	2.4	ng/ul	171625	2	10.751	1431210	20.0