

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007594.D
 Acq On : 22 Oct 2021 17:31
 Operator : CG/JU
 Sample : M4281-01
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	5	10	28	rVB2	251500	439133	7.71%	0.890%
2	3.652	59	62	69	rVB	9994	14813	0.26%	0.030%
3	3.799	84	87	98	rBV	128934	199776	3.51%	0.405%
4	4.034	123	127	134	rVB	28480	45510	0.80%	0.092%
5	4.122	139	142	150	rVB	11761	18799	0.33%	0.038%
6	4.222	155	159	164	rVB5	12460	16177	0.28%	0.033%
7	5.052	297	300	306	rVB5	6398	10310	0.18%	0.021%
8	6.028	462	466	470	rVB2	6791	8115	0.14%	0.016%
9	6.328	512	517	522	rVB2	9713	15910	0.28%	0.032%
10	6.934	615	620	622	rBV5	4920	7382	0.13%	0.015%
11	7.110	643	650	658	rVB	191790	313351	5.50%	0.635%
12	7.275	671	678	687	rVB	604553	954857	16.77%	1.936%
13	7.475	705	712	721	rBV	638771	1017718	17.87%	2.063%
14	7.551	721	725	730	rVV3	7864	12469	0.22%	0.025%
15	7.946	785	792	801	rBV	652627	1020356	17.92%	2.069%
16	8.016	801	804	808	rVB2	8850	11773	0.21%	0.024%
17	8.375	860	865	871	rBV5	6328	11562	0.20%	0.023%
18	8.651	906	912	921	rBV	516627	812126	14.26%	1.647%
19	9.104	981	989	997	rBV	737948	1217976	21.39%	2.469%
20	9.275	1016	1018	1023	rVB6	5208	7034	0.12%	0.014%
21	9.569	1061	1068	1073	rVB5	10362	19913	0.35%	0.040%
22	9.745	1092	1098	1103	rVB10	2815	6819	0.12%	0.014%
23	9.828	1103	1112	1125	rBV	559094	943633	16.57%	1.913%
24	10.057	1146	1151	1153	rBV6	4531	6575	0.12%	0.013%
25	10.369	1197	1204	1215	rBV	909235	1510742	26.53%	3.063%
26	10.534	1225	1232	1242	rBV	393488	622621	10.93%	1.262%
27	10.751	1257	1269	1281	rVB	860744	1471018	25.83%	2.982%
28	10.881	1281	1291	1303	rBV	745218	1313574	23.06%	2.663%
29	11.404	1374	1380	1383	rBV7	4615	7519	0.13%	0.015%
30	11.492	1391	1395	1399	rBV7	3735	6355	0.11%	0.013%
31	12.281	1524	1529	1533	rBV	13113	20020	0.35%	0.041%
32	12.339	1534	1539	1548	rVB3	17777	31900	0.56%	0.065%
33	12.786	1610	1615	1621	rBV7	9156	18022	0.32%	0.037%
34	12.957	1638	1644	1647	rBV3	8466	13732	0.24%	0.028%
35	13.204	1681	1686	1693	rBV3	13728	21656	0.38%	0.044%
36	13.428	1719	1724	1728	rBV8	4856	7425	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007594.D
 Acq On : 22 Oct 2021 17:31
 Operator : CG/JU
 Sample : M4281-01
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	13.492	1728	1735	1740	rBV10	9939	18673	0.33%	0.038%
38	13.551	1742	1745	1750	rVB6	4211	6098	0.11%	0.012%
39	13.786	1780	1785	1789	rBV8	8767	14673	0.26%	0.030%
40	13.851	1793	1796	1801	rVB7	6252	8732	0.15%	0.018%

41	13.992	1813	1820	1826	rBV	1768691	2385989	41.89%	4.838%
42	14.275	1856	1868	1881	rBV	1949097	2845782	49.97%	5.770%
43	14.433	1891	1895	1899	rBV7	5029	8418	0.15%	0.017%
44	14.498	1902	1906	1912	rVV	17224	30792	0.54%	0.062%
45	14.580	1912	1920	1938	rVB	1320666	2063436	36.23%	4.184%

46	14.769	1942	1952	1963	rBV	184113	284906	5.00%	0.578%
47	14.922	1972	1978	1980	rBV7	4626	8169	0.14%	0.017%
48	14.998	1988	1991	1994	rBV4	8169	10975	0.19%	0.022%
49	15.033	1994	1997	2003	rVB6	8879	15544	0.27%	0.032%
50	15.116	2008	2011	2016	rVB5	5785	8588	0.15%	0.017%

51	15.233	2026	2031	2038	rVB6	18440	30051	0.53%	0.061%
52	15.327	2042	2047	2052	rVB9	4464	7714	0.14%	0.016%
53	15.398	2054	2059	2063	rBV2	44760	59169	1.04%	0.120%
54	15.575	2081	2089	2101	rBV	2527880	3677129	64.57%	7.455%
55	15.686	2102	2108	2116	rBV	248552	345083	6.06%	0.700%

56	15.816	2125	2130	2135	rBV	31570	46260	0.81%	0.094%
57	15.939	2149	2151	2156	rVB5	7580	10434	0.18%	0.021%
58	16.022	2160	2165	2172	rVV7	13583	30113	0.53%	0.061%
59	16.145	2181	2186	2187	rBV5	7796	13568	0.24%	0.028%
60	16.345	2216	2220	2222	rBV4	8788	11990	0.21%	0.024%

61	16.474	2240	2242	2248	rVB7	5656	8386	0.15%	0.017%
62	16.992	2325	2330	2337	rBV	23101	49265	0.87%	0.100%
63	17.116	2349	2351	2354	rBV3	6641	7761	0.14%	0.016%
64	17.333	2382	2388	2398	rVB	1693639	2466298	43.30%	5.000%
65	17.433	2398	2405	2415	rBV2	2990510	4327636	75.99%	8.774%

66	17.574	2426	2429	2434	rBV7	10901	18697	0.33%	0.038%
67	17.633	2436	2439	2444	rBV2	12746	17217	0.30%	0.035%
68	17.751	2456	2459	2467	rVB6	19716	33554	0.59%	0.068%
69	17.939	2488	2491	2495	rVB4	19632	22728	0.40%	0.046%
70	18.016	2500	2504	2509	rBV	98181	119771	2.10%	0.243%

71	18.227	2536	2540	2548	rBV	197636	275432	4.84%	0.558%
72	18.680	2615	2617	2623	rVV7	14688	17271	0.30%	0.035%
73	18.751	2626	2629	2635	rVB3	30535	41206	0.72%	0.084%
74	18.951	2660	2663	2677	rVB	25509	65840	1.16%	0.133%
75	19.245	2710	2713	2717	rVB3	45043	53550	0.94%	0.109%

76	19.316	2721	2725	2728	rBV	43800	62039	1.09%	0.126%
----	--------	------	------	------	-----	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007594.D
Acq On : 22 Oct 2021 17:31
Operator : CG/JU
Sample : M4281-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY57

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

77	19.463	2747	2750	2758	rVB4	49249	67570	1.19%	0.137%
78	19.668	2779	2785	2793	rBV	4106003	5432769	95.39%	11.015%
79	21.139	3031	3035	3041	rBV2	246357	333343	5.85%	0.676%
80	21.421	3078	3083	3088	rBV	2291614	2972811	52.20%	6.027%
81	23.709	3465	3472	3481	rVB2	2861611	5695209	100.00%	11.547%
82	23.868	3492	3499	3507	rVB2	1536211	3115194	54.70%	6.316%




Sum of corrected areas: 49322504

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007594.D
Acq On : 22 Oct 2021 17:31
Operator : CG/JU
Sample : M4281-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

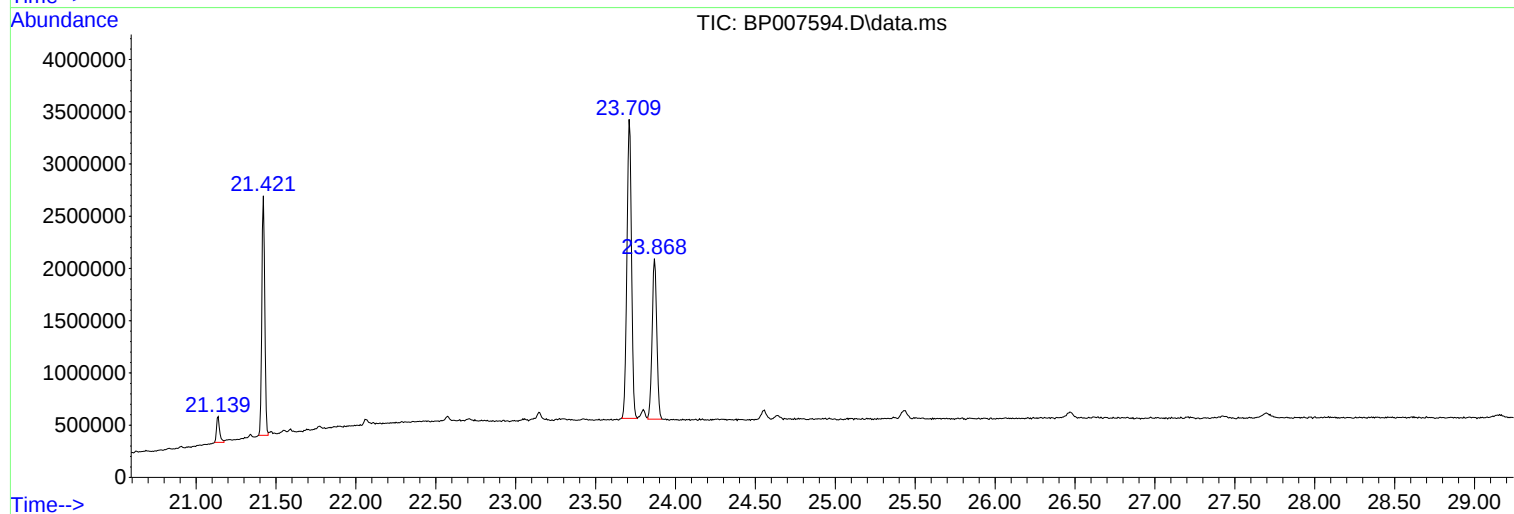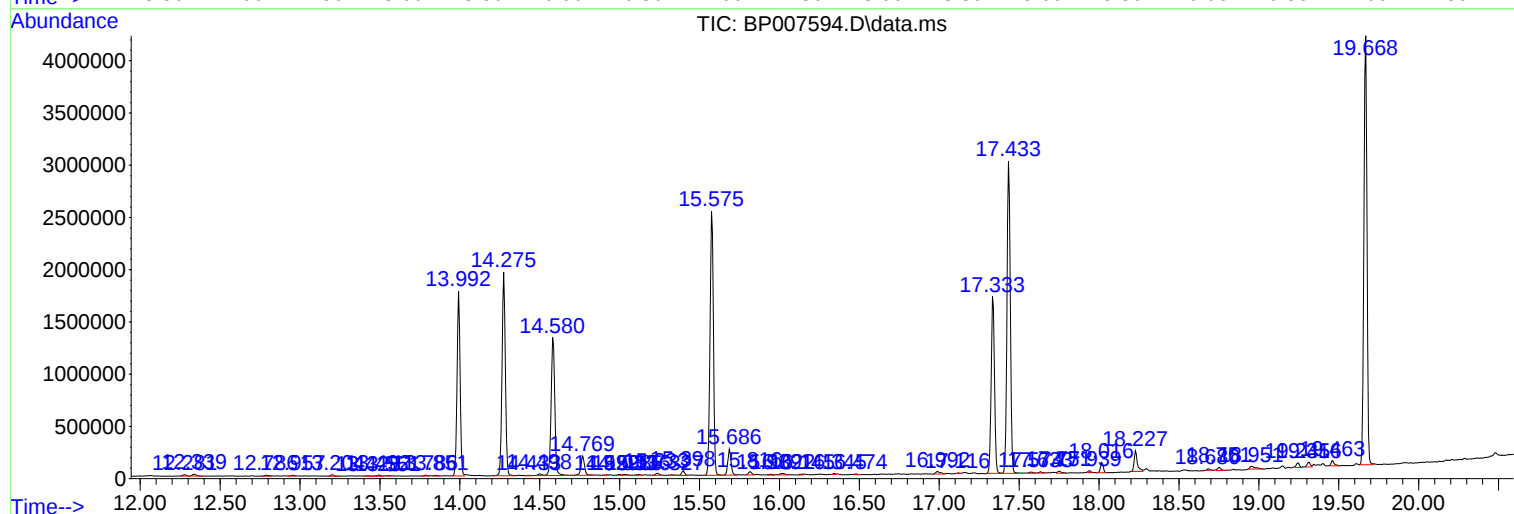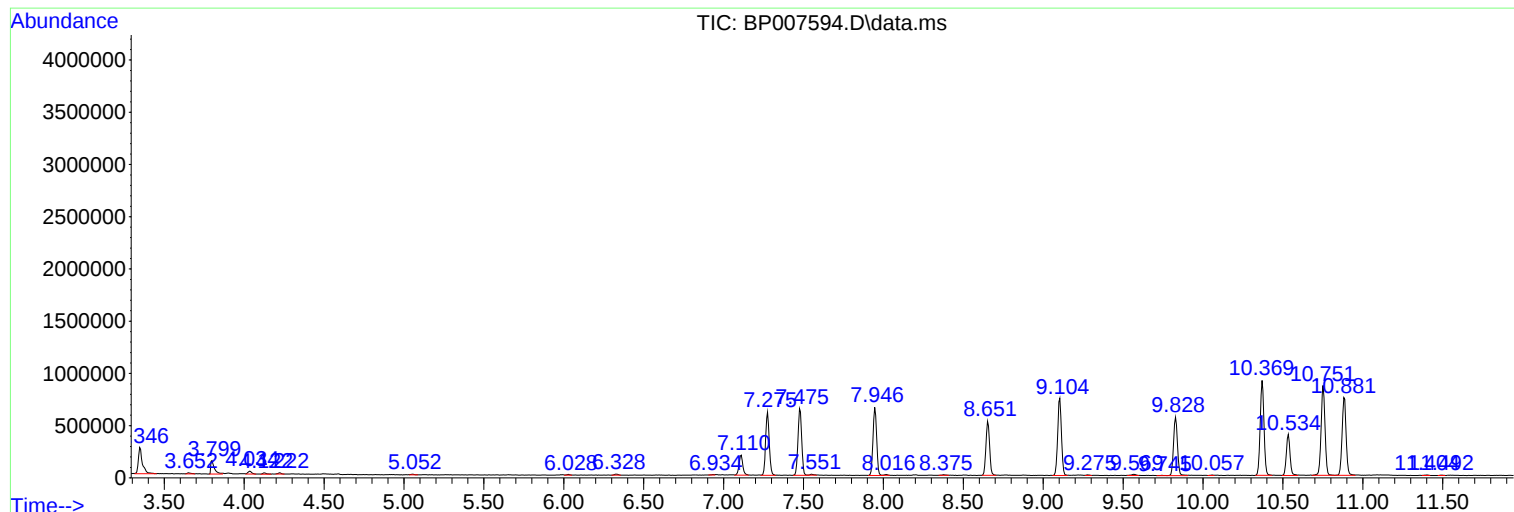

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007594.D
Acq On : 22 Oct 2021 17:31
Operator : CG/JU
Sample : M4281-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007594.D
Acq On : 22 Oct 2021 17:31
Operator : CG/JU
Sample : M4281-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
