

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007599.D
 Acq On : 22 Oct 2021 20:55
 Operator : CG/JU
 Sample : PB140091BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK091

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.376	10	15	22	rBV	62579	83608	1.27%	0.136%
2	3.787	82	85	100	rBV	833151	1283487	19.50%	2.093%
3	4.128	138	143	149	rVB	13137	22635	0.34%	0.037%
4	5.128	309	313	317	rVB6	5885	7917	0.12%	0.013%
5	7.105	642	649	660	rVB	1050819	1695458	25.76%	2.765%
6	7.275	670	678	687	rVB	782994	1231954	18.72%	2.009%
7	7.475	703	712	721	rBV	1078319	1696780	25.78%	2.767%
8	7.946	785	792	801	rVB	699602	1107042	16.82%	1.805%
9	8.652	904	912	921	rBV	1335711	2115613	32.14%	3.450%
10	9.105	979	989	997	rBV	918381	1561487	23.72%	2.547%
11	9.828	1103	1112	1120	rBV	783144	1296631	19.70%	2.115%
12	10.369	1195	1204	1216	rBV	1323303	2210869	33.59%	3.606%
13	10.752	1260	1269	1277	rBV	943944	1598891	24.29%	2.608%
14	10.881	1282	1291	1303	rBV	1221870	2108917	32.04%	3.439%
15	11.105	1318	1329	1332	rBV10	5566	15581	0.24%	0.025%
16	11.540	1398	1403	1412	rBV10	5285	10645	0.16%	0.017%
17	11.687	1422	1428	1433	rBV6	5996	12891	0.20%	0.021%
18	12.334	1534	1538	1545	rVB2	28105	42255	0.64%	0.069%
19	13.551	1740	1745	1750	rVB8	4791	9392	0.14%	0.015%
20	13.993	1810	1820	1826	rBV	2245088	3093786	47.00%	5.046%
21	14.275	1859	1868	1880	rBV	2483132	3711719	56.39%	6.053%
22	14.510	1902	1908	1913	rBV2	11537	22719	0.35%	0.037%
23	14.581	1913	1920	1930	rVB	1508445	2205679	33.51%	3.597%
24	14.769	1945	1952	1964	rBV	1126360	1582157	24.04%	2.580%
25	15.034	1995	1997	2007	rVB5	6207	14045	0.21%	0.023%
26	15.116	2007	2011	2013	rBV5	5679	8759	0.13%	0.014%
27	15.240	2025	2032	2040	rVB2	35624	56471	0.86%	0.092%
28	15.575	2082	2089	2098	rBV	3220783	4629233	70.33%	7.550%
29	15.687	2102	2108	2116	rBV	257233	363069	5.52%	0.592%
30	15.816	2125	2130	2135	rVB	38916	60345	0.92%	0.098%
31	16.151	2182	2187	2192	rBV9	5861	11098	0.17%	0.018%
32	16.251	2198	2204	2207	rBV8	7374	14059	0.21%	0.023%
33	16.363	2218	2223	2227	rBV8	5566	9737	0.15%	0.016%
34	16.992	2326	2330	2337	rBV2	15496	35095	0.53%	0.057%
35	17.116	2348	2351	2354	rBV2	6891	7797	0.12%	0.013%
36	17.210	2364	2367	2371	rVB6	11720	15211	0.23%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007599.D
 Acq On : 22 Oct 2021 20:55
 Operator : CG/JU
 Sample : PB140091BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK091

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	17.334	2382	2388	2398	rBV	1870346	2694204	40.93%	4.394%
38	17.434	2398	2405	2416	rVV2	3617588	5244311	79.67%	8.553%
39	17.575	2425	2429	2434	rVB6	13609	23446	0.36%	0.038%
40	17.704	2448	2451	2456	rBV4	8161	14965	0.23%	0.024%
41	18.222	2537	2539	2542	rBV3	9754	10593	0.16%	0.017%
42	18.951	2660	2663	2667	rBV2	19109	26875	0.41%	0.044%
43	19.245	2708	2713	2718	rVB2	55591	80718	1.23%	0.132%
44	19.310	2720	2724	2729	rBV	56609	78040	1.19%	0.127%
45	19.669	2779	2785	2792	rBV	4486964	6211970	94.37%	10.131%
46	21.422	3078	3083	3088	rBV	2370952	3139540	47.70%	5.120%
47	23.710	3464	3472	3481	rVB2	3161865	6582461	100.00%	10.735%
48	23.863	3492	3498	3508	rVB2	1553157	3256002	49.46%	5.310%




Sum of corrected areas: 61316157

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007599.D
Acq On : 22 Oct 2021 20:55
Operator : CG/JU
Sample : PB140091BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK091

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

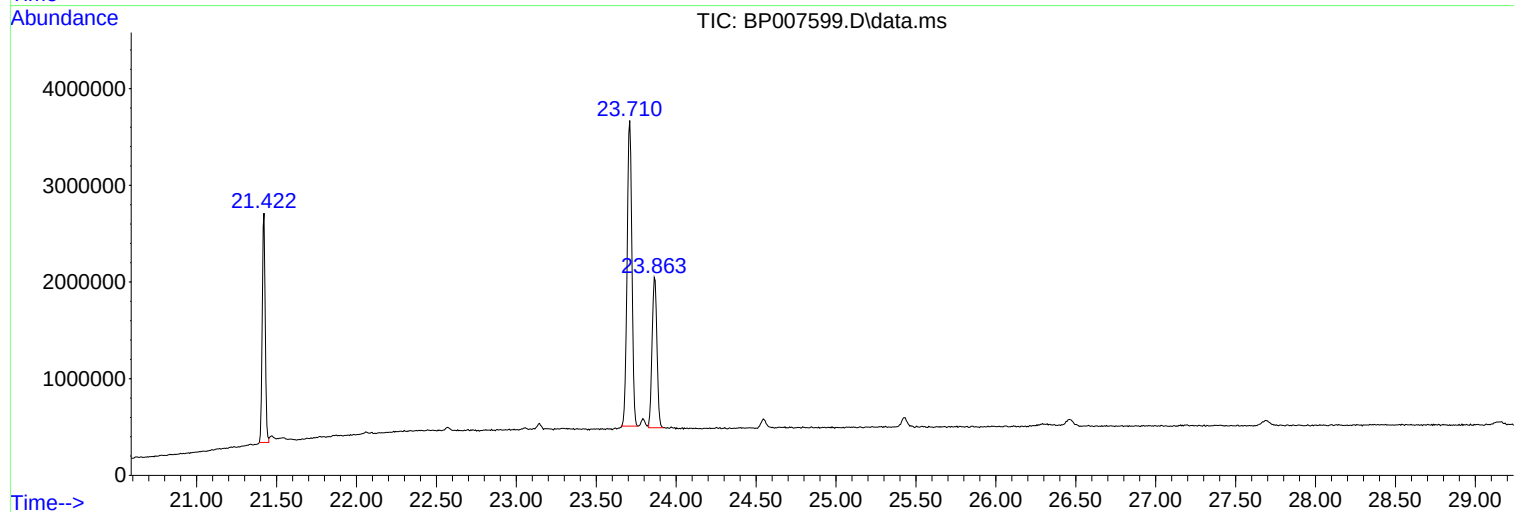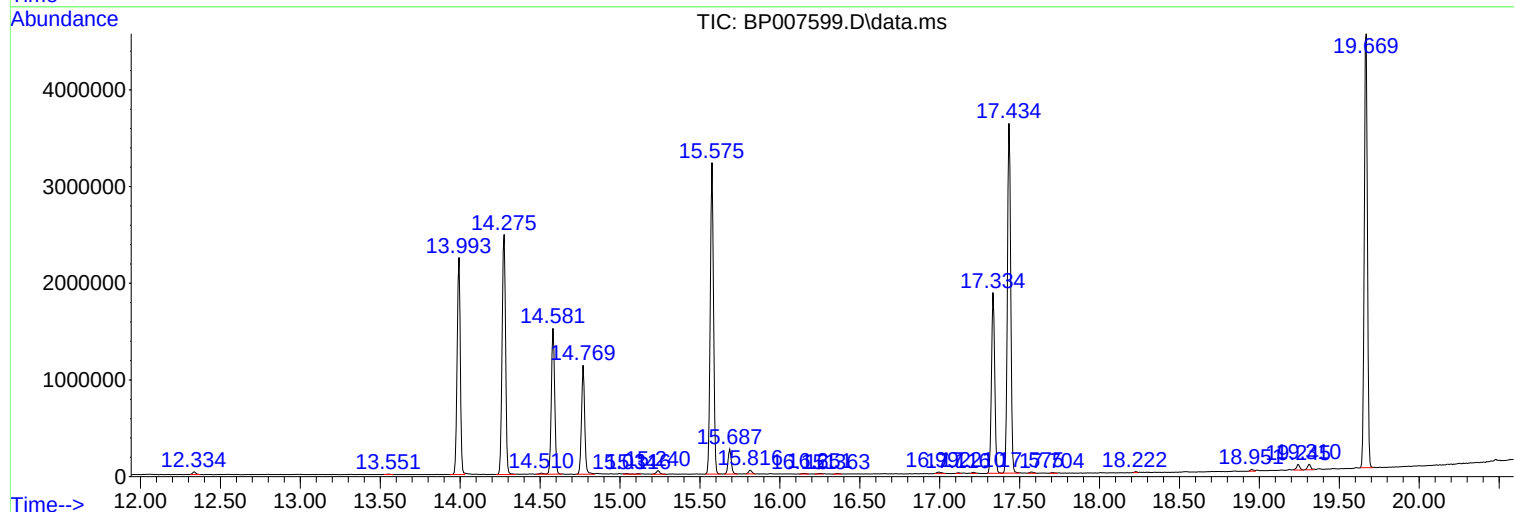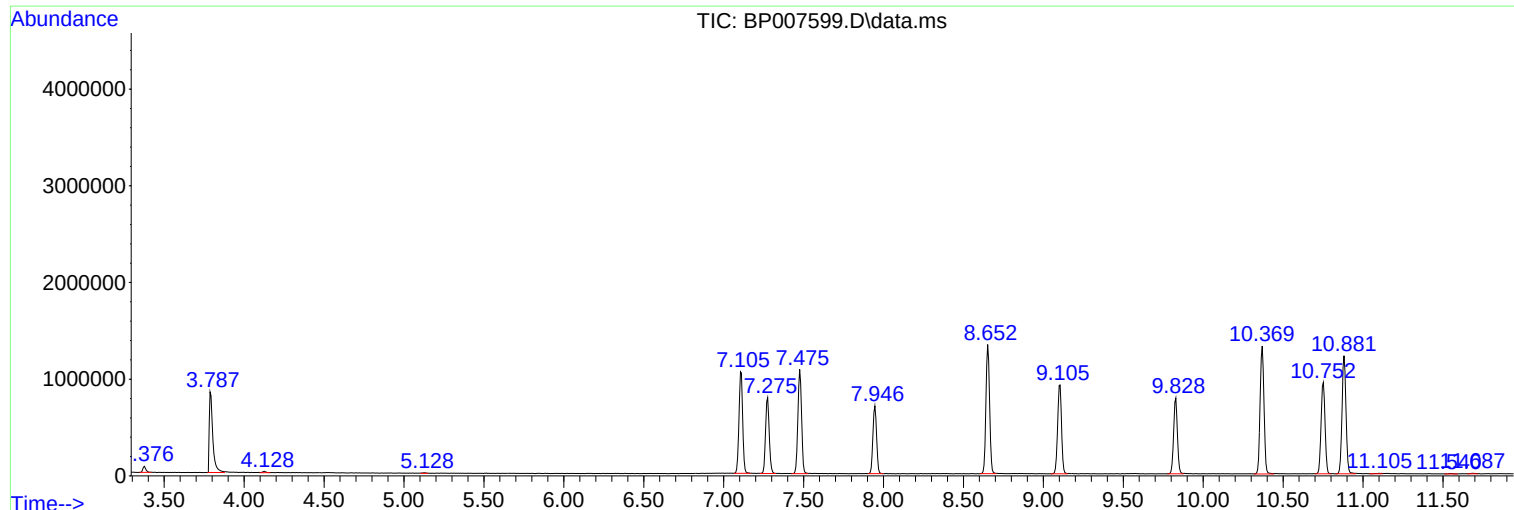

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007599.D
Acq On : 22 Oct 2021 20:55
Operator : CG/JU
Sample : PB140091BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK091

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007599.D
Acq On : 22 Oct 2021 20:55
Operator : CG/JU
Sample : PB140091BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK091

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------