

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007618.D
 Acq On : 23 Oct 2021 08:12
 Operator : CG/JU
 Sample : PB140107BL
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	10	15	24	rVB	68737	93253	1.32%	0.136%
2	3.658	60	63	69	rVB6	4976	8856	0.13%	0.013%
3	3.787	81	85	103	rBV	939050	1447433	20.47%	2.116%
4	4.122	139	142	148	rVB	14662	19281	0.27%	0.028%
5	5.122	305	312	316	rBV10	4774	9249	0.13%	0.014%
6	7.111	641	650	664	rVB	1140878	1856930	26.26%	2.714%
7	7.269	670	677	689	rVB	857328	1355037	19.16%	1.981%
8	7.475	705	712	723	rBV	1187045	1840959	26.04%	2.691%
9	7.946	784	792	800	rVB	834403	1342987	18.99%	1.963%
10	8.652	905	912	930	rBV	1445949	2323531	32.86%	3.397%
11	9.099	981	988	998	rBV	1050423	1715230	24.26%	2.507%
12	9.828	1104	1112	1124	rBV	849717	1437133	20.32%	2.101%
13	10.369	1196	1204	1219	rBV	1434999	2416616	34.18%	3.533%
14	10.746	1260	1268	1276	rBV	1123617	1932046	27.32%	2.824%
15	10.881	1282	1291	1302	rBV	1360656	2307422	32.63%	3.373%
16	11.152	1334	1337	1345	rVB10	4103	7879	0.11%	0.012%
17	11.687	1419	1428	1434	rBV8	6146	13462	0.19%	0.020%
18	12.334	1532	1538	1545	rBV2	28126	46957	0.66%	0.069%
19	12.998	1643	1651	1658	rVB2	2456	7450	0.11%	0.011%
20	13.993	1812	1820	1835	rBV	2450937	3397958	48.06%	4.967%
21	14.275	1859	1868	1885	rBV	2691446	4091709	57.87%	5.981%
22	14.581	1912	1920	1933	rBV	1827240	2672595	37.80%	3.907%
23	14.775	1946	1953	1966	rBV	1125617	1683980	23.82%	2.462%
24	15.240	2026	2032	2036	rBV3	23680	36341	0.51%	0.053%
25	15.575	2082	2089	2099	rBV	3491686	5078330	71.82%	7.423%
26	15.687	2102	2108	2119	rBV	420463	567947	8.03%	0.830%
27	15.816	2124	2130	2136	rVB	43701	70647	1.00%	0.103%
28	15.945	2147	2152	2157	rBV7	5868	12254	0.17%	0.018%
29	16.151	2180	2187	2193	rBV10	6953	16662	0.24%	0.024%
30	16.251	2198	2204	2214	rBV10	7680	18788	0.27%	0.027%
31	16.363	2219	2223	2227	rVV6	5250	7668	0.11%	0.011%
32	17.004	2326	2332	2339	rBV10	9269	24373	0.34%	0.036%
33	17.116	2346	2351	2356	rBV2	10829	17932	0.25%	0.026%
34	17.216	2364	2368	2374	rVB9	7087	14158	0.20%	0.021%
35	17.334	2381	2388	2398	rBV	2303728	3235075	45.75%	4.729%
36	17.434	2398	2405	2420	rVV	4019773	5707080	80.71%	8.343%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007618.D
 Acq On : 23 Oct 2021 08:12
 Operator : CG/JU
 Sample : PB140107BL
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK107

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	17.575	2426	2429	2435	rVB4	11990	15602	0.22%	0.023%
38	17.710	2447	2452	2455	rBV2	8527	13842	0.20%	0.020%
39	18.004	2500	2502	2508	rVB6	9298	11017	0.16%	0.016%
40	18.228	2537	2540	2544	rBV6	5757	8914	0.13%	0.013%
41	19.245	2708	2713	2717	rVB	56358	76973	1.09%	0.113%
42	19.310	2720	2724	2729	rVV	63100	80406	1.14%	0.118%
43	19.669	2779	2785	2796	rBV	4883238	6711379	94.92%	9.811%
44	21.422	3077	3083	3088	rBV	2904269	3753581	53.09%	5.487%
45	23.710	3464	3472	3482	rBV2	3480948	7070865	100.00%	10.336%
46	23.869	3492	3499	3508	rVB2	1845151	3831719	54.19%	5.601%




Sum of corrected areas: 68409506

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007618.D
Acq On : 23 Oct 2021 08:12
Operator : CG/JU
Sample : PB140107BL
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK107

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

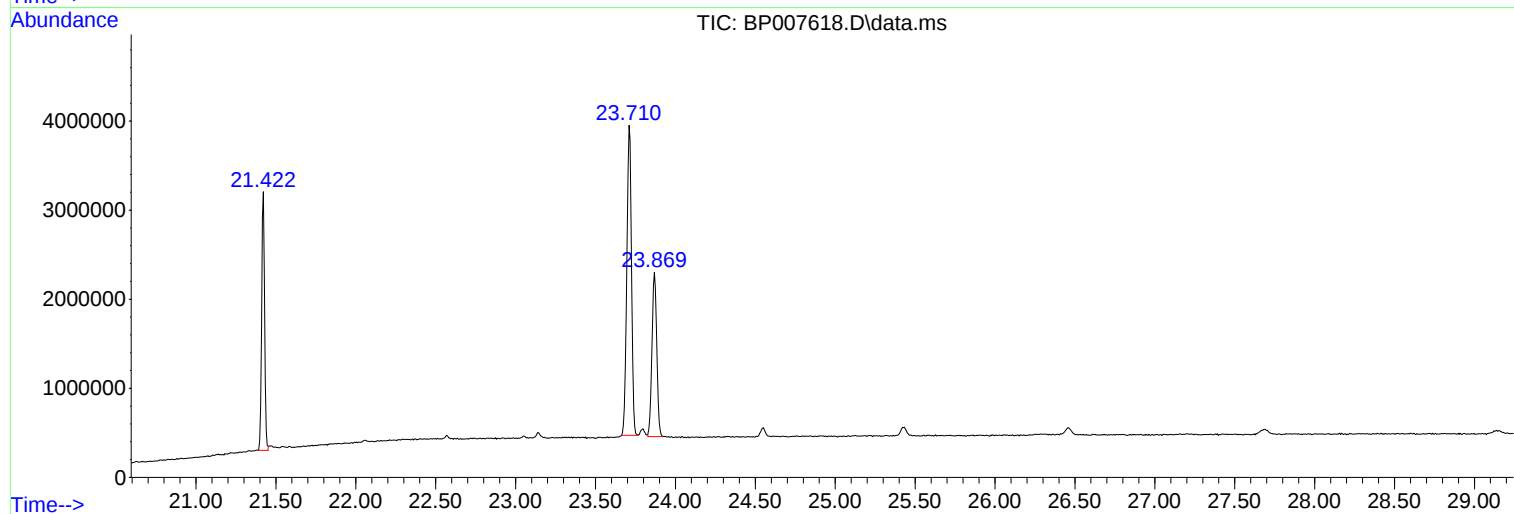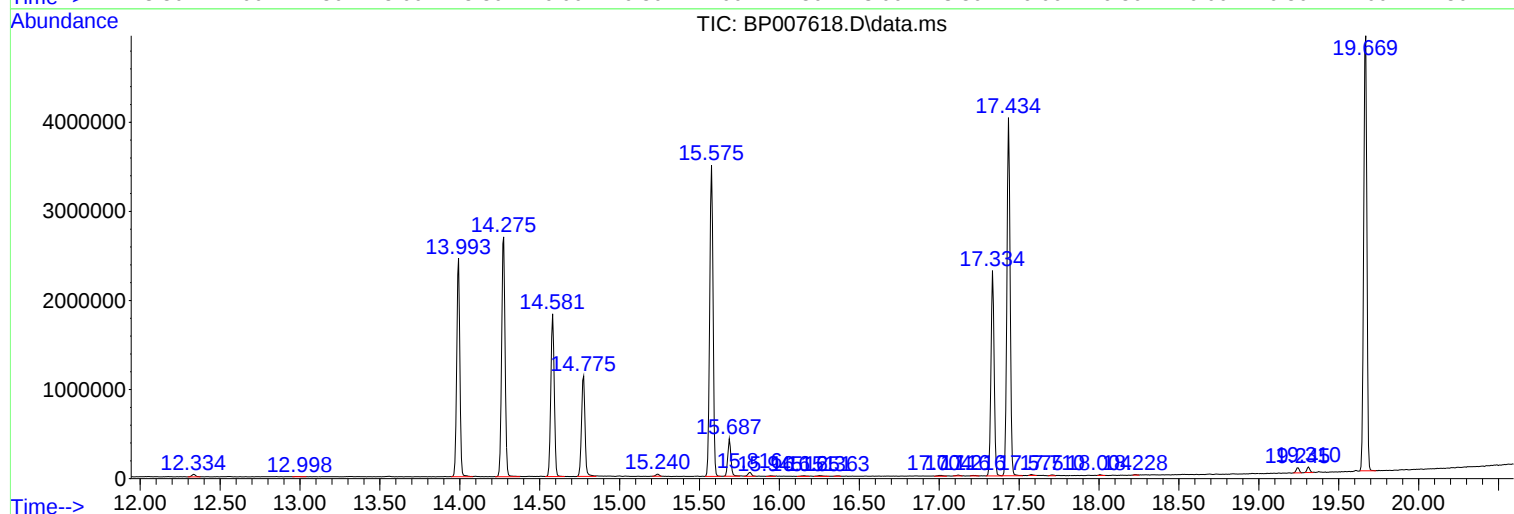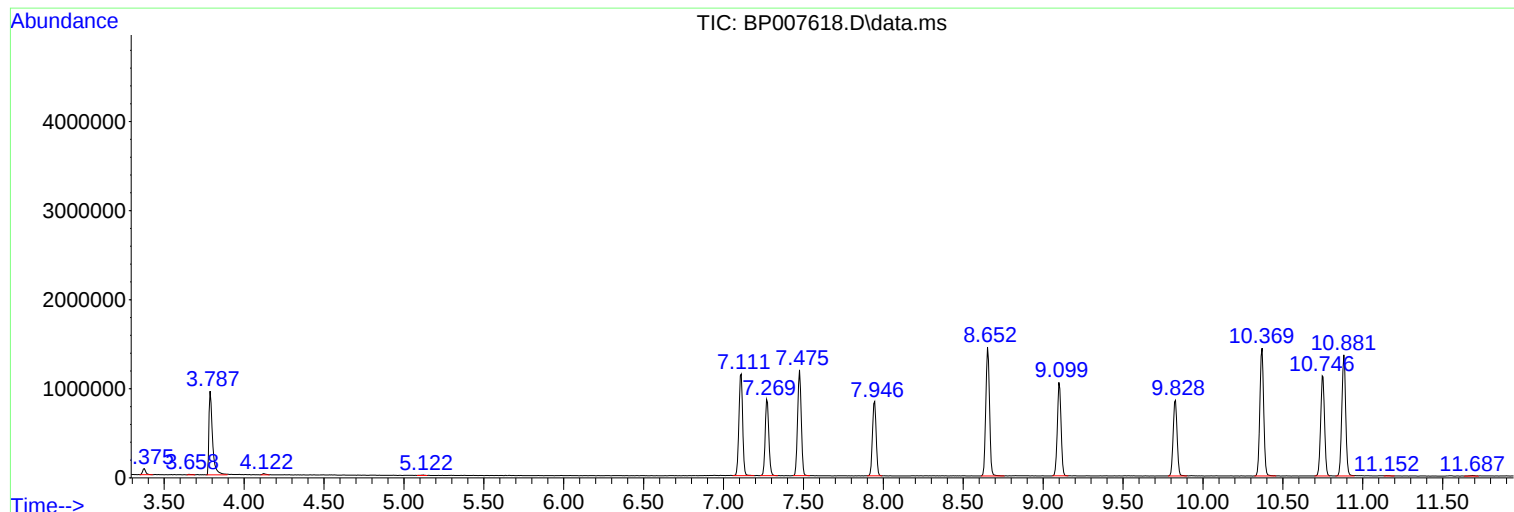

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007618.D
Acq On : 23 Oct 2021 08:12
Operator : CG/JU
Sample : PB140107BL
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK107

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007618.D
Acq On : 23 Oct 2021 08:12
Operator : CG/JU
Sample : PB140107BL
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK107

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
