

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007620.D
 Acq On : 23 Oct 2021 09:20
 Operator : CG/JU
 Sample : PB140072BL
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK072

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	27	rVB	77885	105198	1.27%	0.134%
2	3.787	81	85	103	rBV	1089259	1682229	20.30%	2.142%
3	4.122	139	142	148	rVB2	15672	24381	0.29%	0.031%
4	7.110	641	650	661	rBV	1357768	2176788	26.27%	2.771%
5	7.269	671	677	688	rVB	1009985	1604381	19.36%	2.043%
6	7.475	704	712	721	rBV	1380513	2168863	26.17%	2.761%
7	7.940	784	791	801	rBV	876199	1439252	17.37%	1.832%
8	8.652	903	912	922	rBV	1684094	2724066	32.87%	3.468%
9	9.099	980	988	996	rBV	1232515	2025393	24.44%	2.579%
10	9.828	1104	1112	1127	rBV	999548	1702532	20.55%	2.168%
11	10.369	1196	1204	1212	rBV	1671365	2833902	34.20%	3.608%
12	10.746	1260	1268	1276	rBV	1201185	2072036	25.00%	2.638%
13	10.881	1282	1291	1300	rBV	1613675	2704888	32.64%	3.444%
14	11.687	1423	1428	1431	rBV6	5952	9470	0.11%	0.012%
15	12.334	1531	1538	1545	rBV	33556	57504	0.69%	0.073%
16	13.557	1739	1746	1750	rVB5	7168	15157	0.18%	0.019%
17	13.992	1812	1820	1836	rBV	2800363	3985916	48.10%	5.075%
18	14.275	1858	1868	1880	rBV	3179662	4787288	57.77%	6.095%
19	14.581	1913	1920	1928	rBV	1929732	2826833	34.11%	3.599%
20	14.769	1946	1952	1966	rBV	1327231	2025851	24.45%	2.579%
21	14.992	1987	1990	1996	rVV7	5849	10319	0.12%	0.013%
22	15.239	2026	2032	2037	rVB2	23582	39939	0.48%	0.051%
23	15.575	2082	2089	2101	rVB	4157712	5915622	71.39%	7.531%
24	15.686	2101	2108	2121	rBV	586184	802340	9.68%	1.021%
25	15.816	2125	2130	2136	rVB2	51920	82551	1.00%	0.105%
26	16.145	2182	2186	2191	rBV8	5560	9747	0.12%	0.012%
27	16.257	2199	2205	2212	rBV8	8752	17700	0.21%	0.023%
28	16.357	2218	2222	2228	rBV9	5435	12114	0.15%	0.015%
29	17.010	2328	2333	2338	rVB9	8366	15708	0.19%	0.020%
30	17.116	2346	2351	2355	rBV	12047	19070	0.23%	0.024%
31	17.333	2381	2388	2396	rBV	2418366	3455211	41.70%	4.399%
32	17.433	2398	2405	2416	rVV2	4645118	6680342	80.62%	8.505%
33	17.575	2424	2429	2440	rBV10	13072	30378	0.37%	0.039%
34	17.710	2446	2452	2455	rBV3	9926	17854	0.22%	0.023%
35	18.222	2535	2539	2542	rBV6	9137	13516	0.16%	0.017%
36	19.239	2708	2712	2718	rBV	66066	91576	1.11%	0.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007620.D
Acq On : 23 Oct 2021 09:20
Operator : CG/JU
Sample : PB140072BL
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	19.310	2720	2724	2729	rVV	69485	89756	1.08%	0.114%
38	19.663	2778	2784	2791	rBV	5617432	7874231	95.02%	10.025%
39	21.421	3077	3083	3088	rBV	3011471	4004804	48.33%	5.099%
40	23.710	3464	3472	3481	rVB2	4166545	8286531	100.00%	10.550%
41	23.868	3491	3499	3507	rVB2	1977805	4106268	49.55%	5.228%




Sum of corrected areas: 78547505

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007620.D
Acq On : 23 Oct 2021 09:20
Operator : CG/JU
Sample : PB140072BL
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

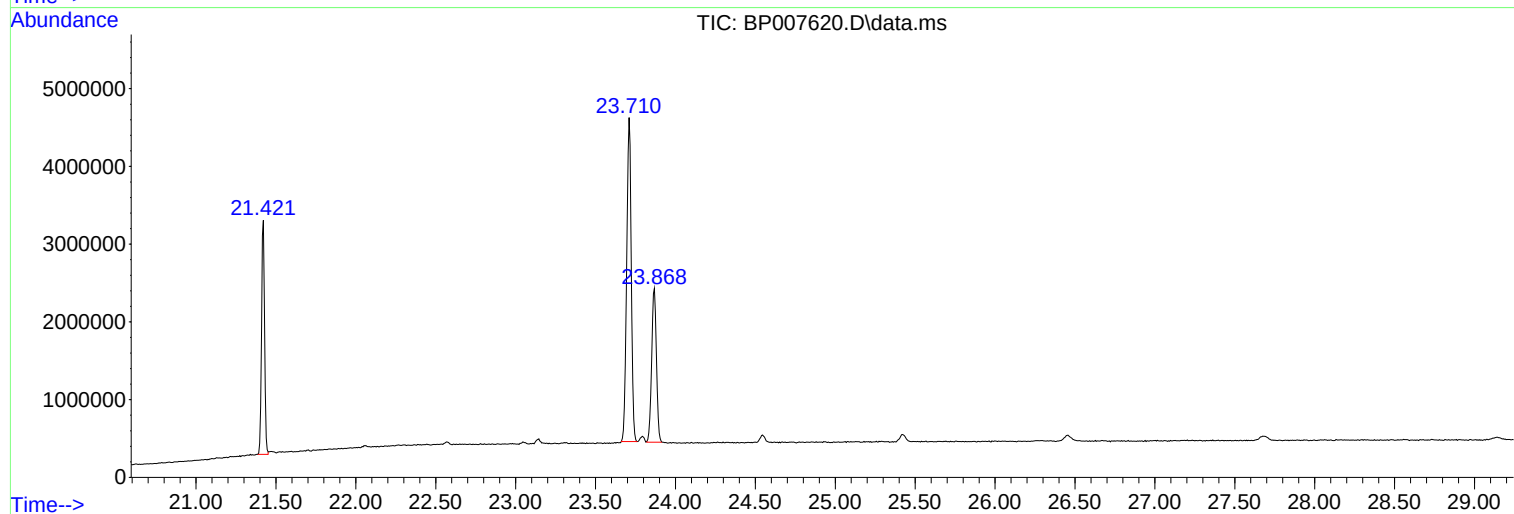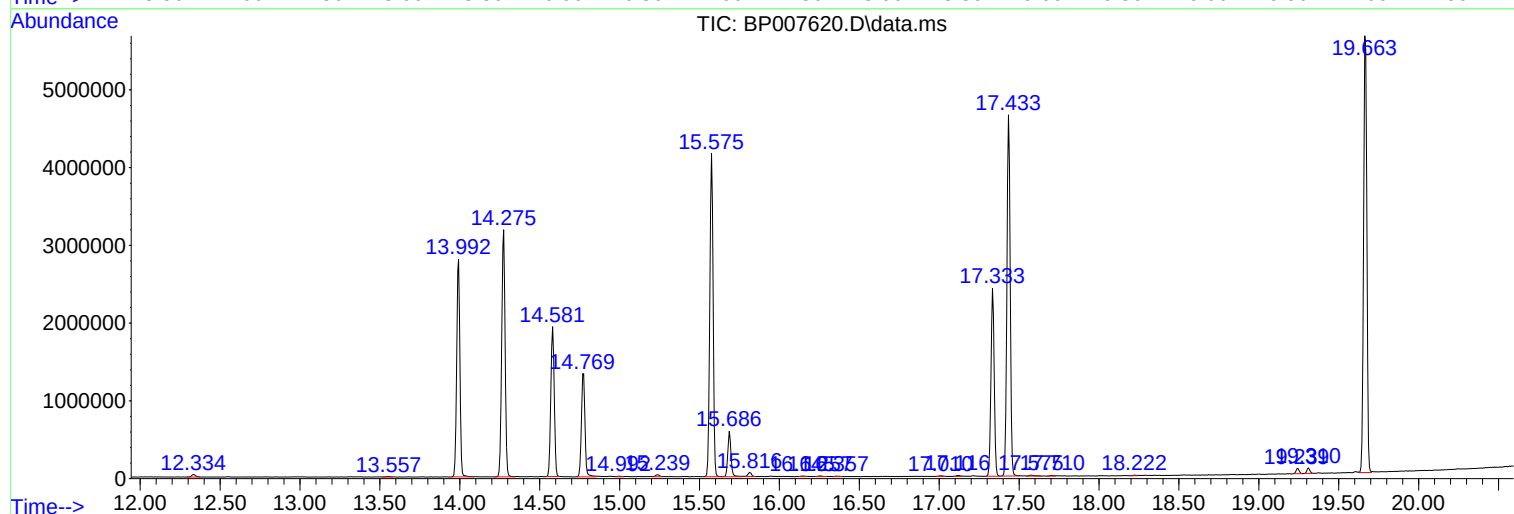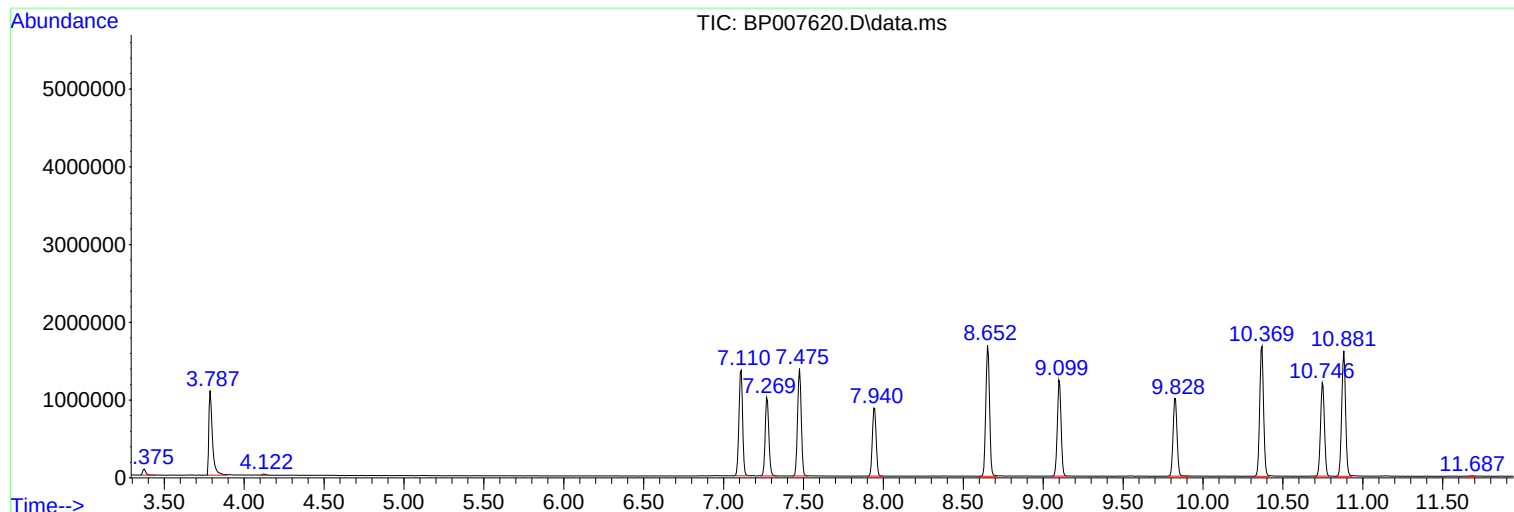

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007620.D
Acq On : 23 Oct 2021 09:20
Operator : CG/JU
Sample : PB140072BL
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007620.D
Acq On : 23 Oct 2021 09:20
Operator : CG/JU
Sample : PB140072BL
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
