
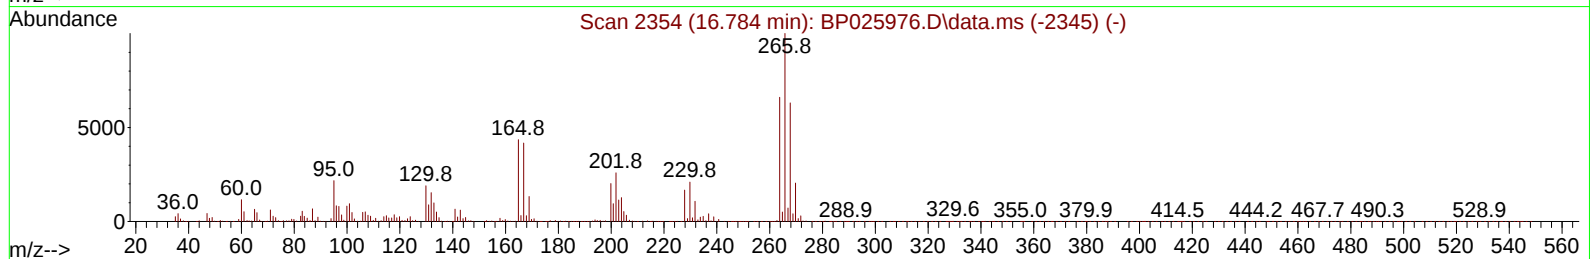
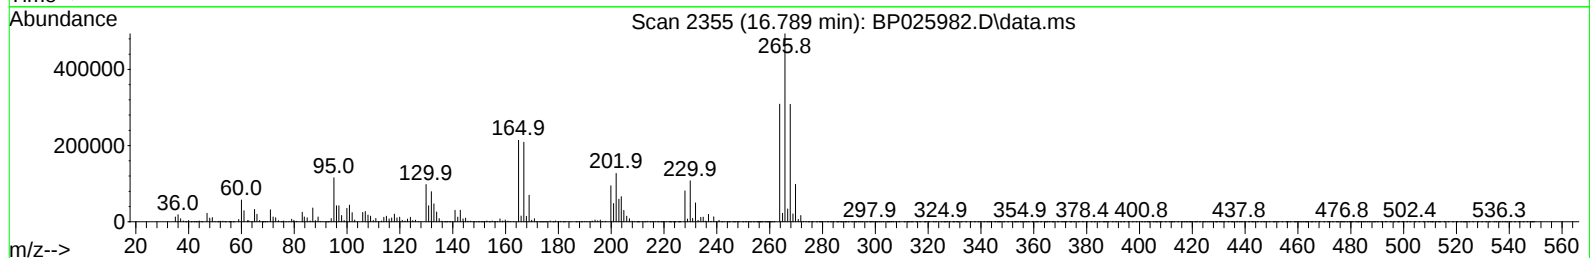


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102125\
Data File : BP025982.D
Acq On : 21 Oct 2025 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 12:28:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

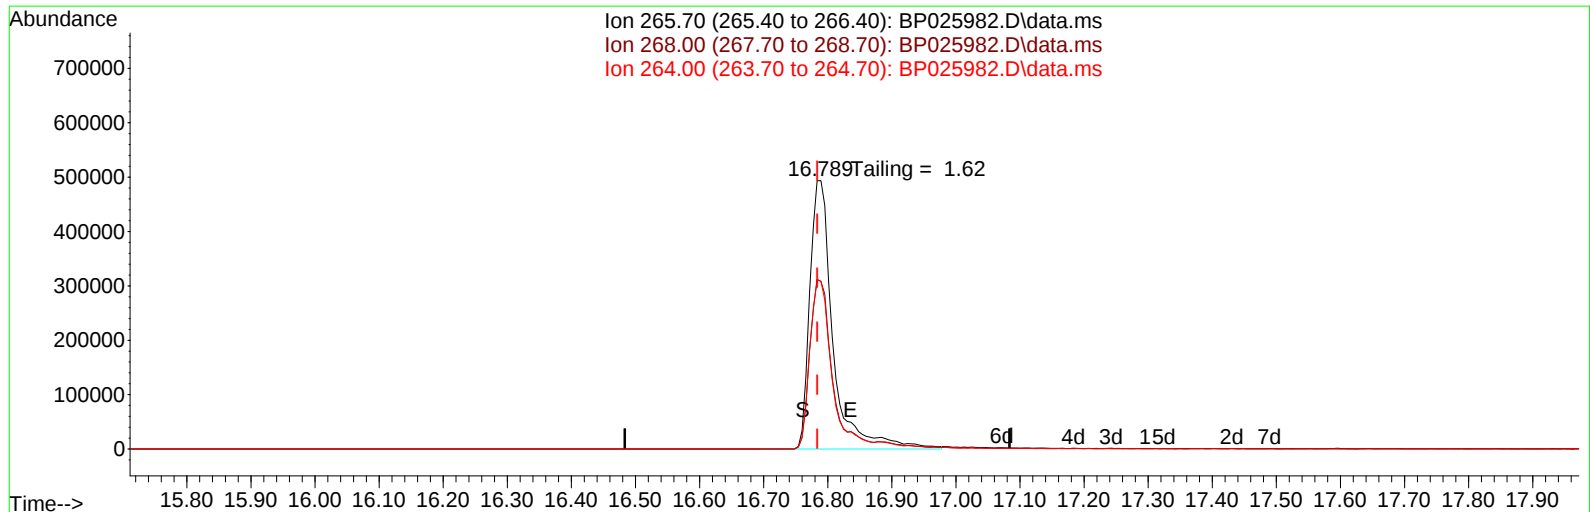

TIC: BP025982.D\data.ms

(70) Pentachlorophenol (C)




16.789min (+ 0.006) 113678.97 ng m

response 1252591

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.44
264.00	66.10	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102125\
Data File : BP025982.D
Acq On : 21 Oct 2025 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 12:28:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

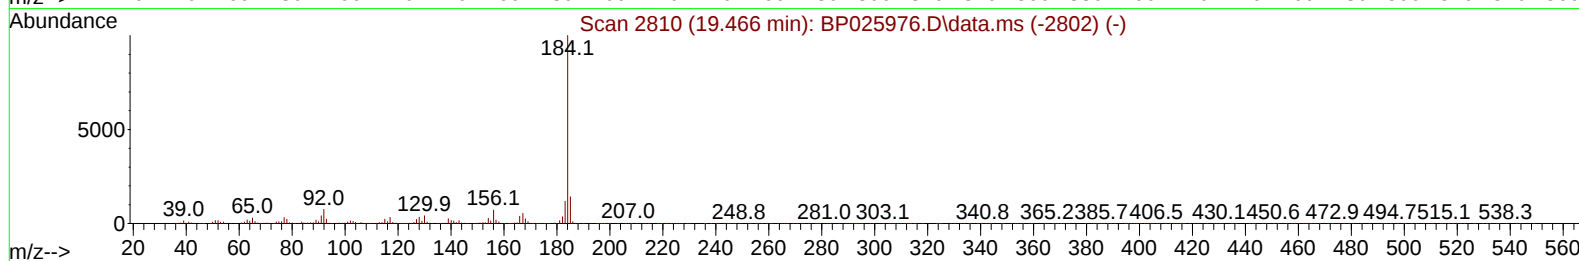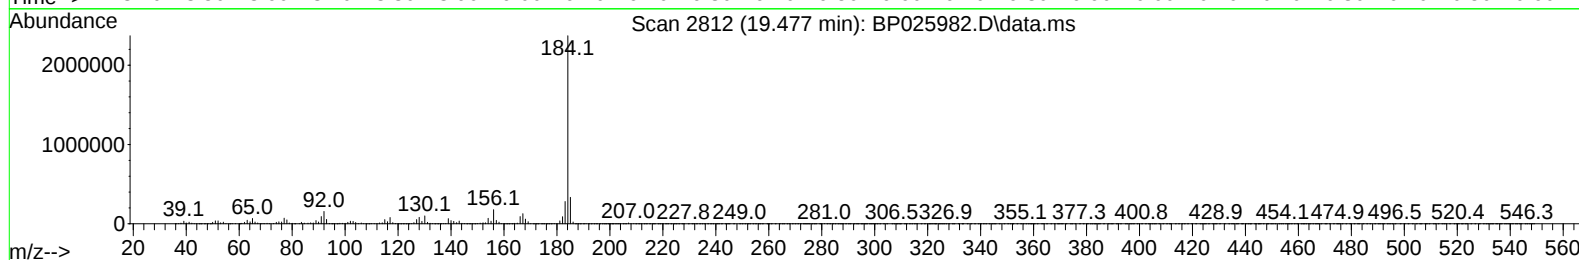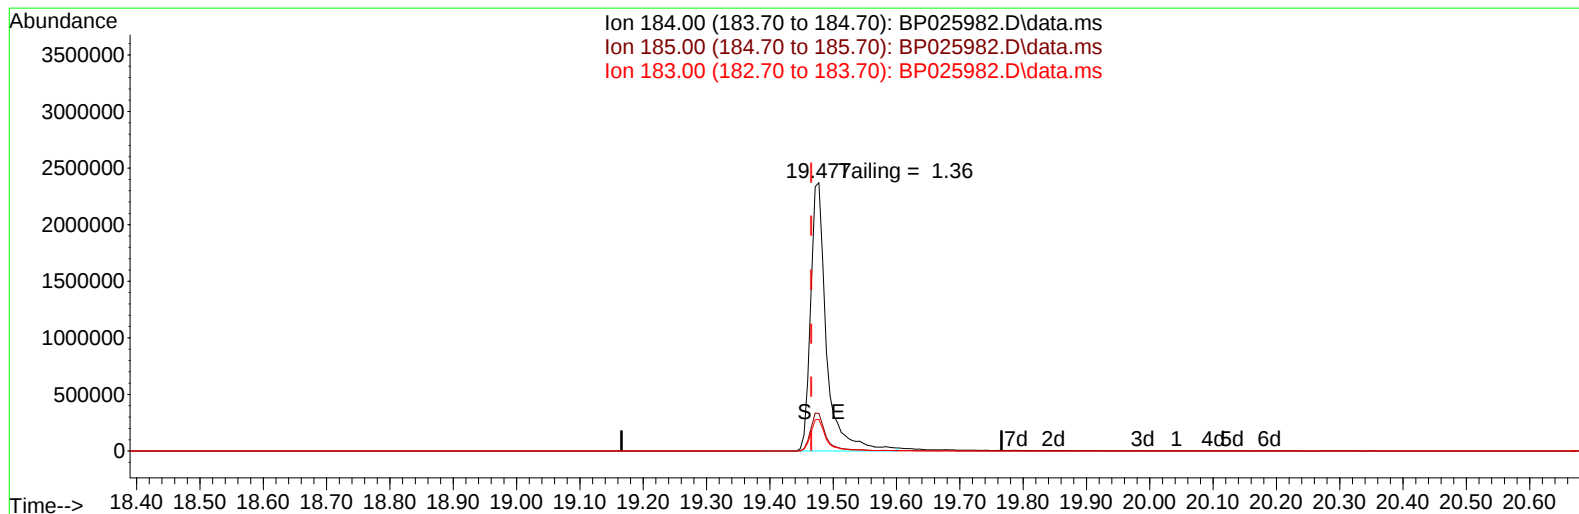

TIC: BP025982.D\data.ms

(77) Benzidine

19.477min (+ 0.012) 4661866.51 ng m

response 4182485

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.01
183.00	11.80	11.84
0.00	0.00	0.00