


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102125\
Data File : BP025982.D
Acq On : 21 Oct 2025 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 15 23:48:51 2025

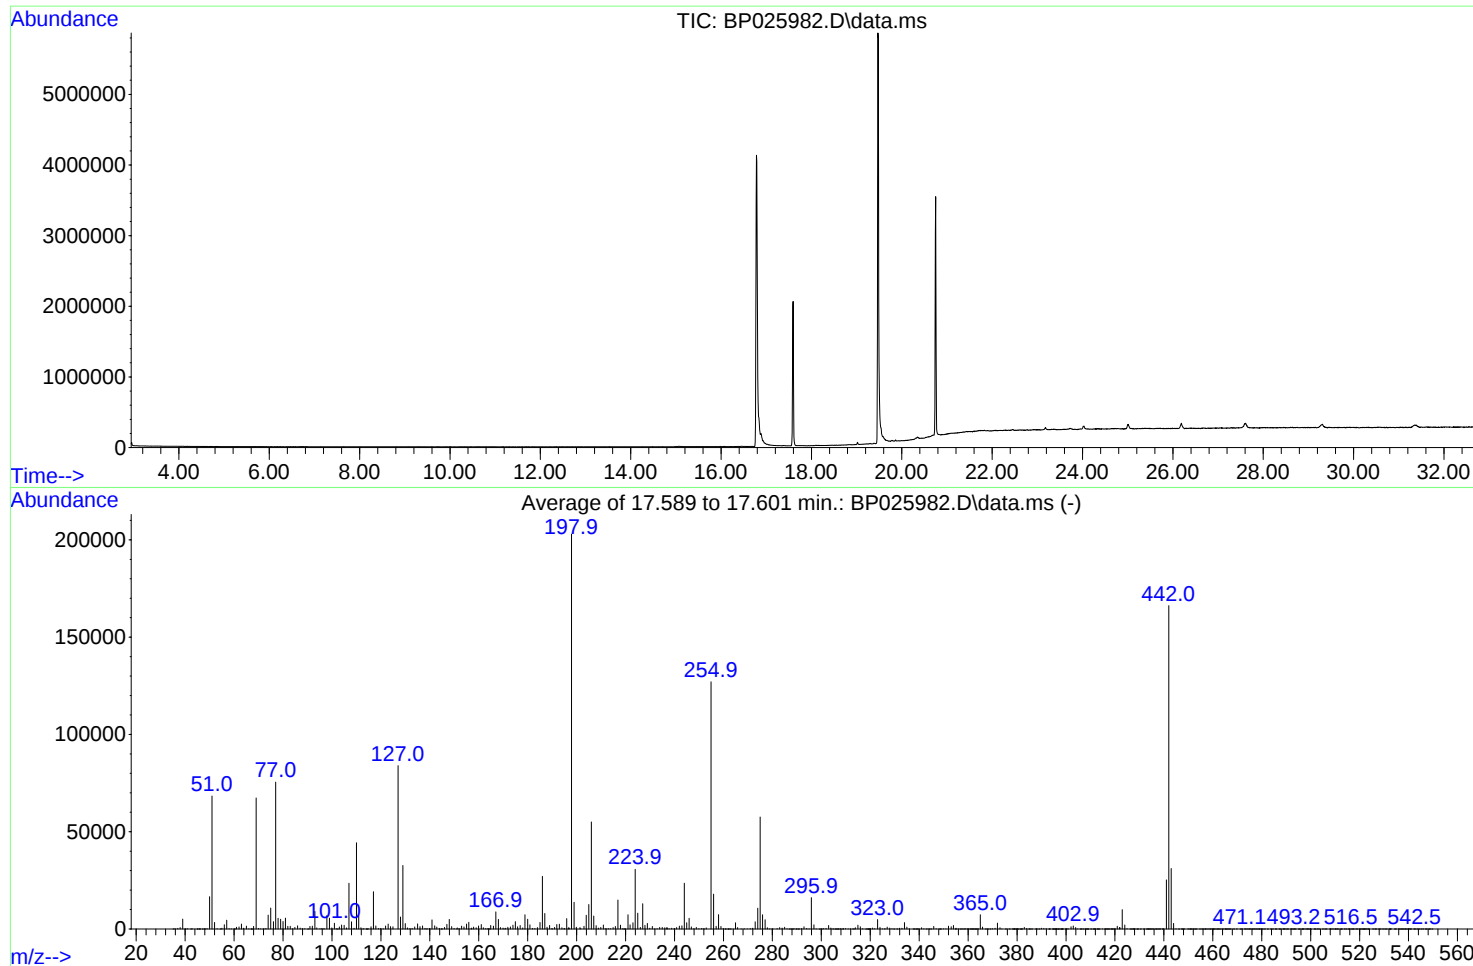

Spectrum Information: Average of 17.589 to 17.601 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1288	PASS
69	69	100	100	100.0	67398	PASS
70	69	0.00	2	0.5	306	PASS
197	198	0.00	2	0.2	506	PASS
198	198	100	100	100.0	202931	PASS
199	198	5	9	6.8	13762	PASS
365	198	1	100	3.6	7299	PASS
441	443	0.01	150	81.1	25227	PASS
442	442	100	100	100.0	166208	PASS
443	442	15	24	18.7	31119	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/20/2025	BNA_P	<u>BP025982.D</u>
Compound Name	Response	Retention Time
DDT	848060	20.748
DDD	6367	20.342
DDE	0	20.072
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6367	854427	0.75

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102125\
Data File : BP025982.D
Acq On : 21 Oct 2025 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 21 12:28:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

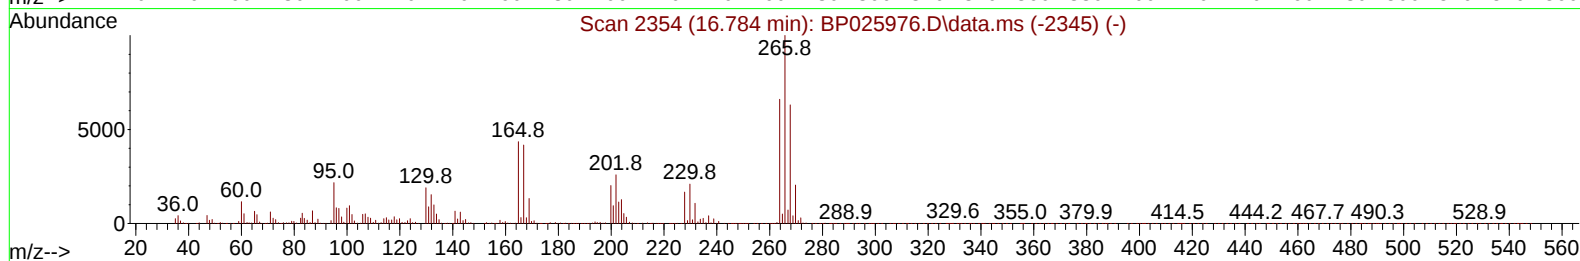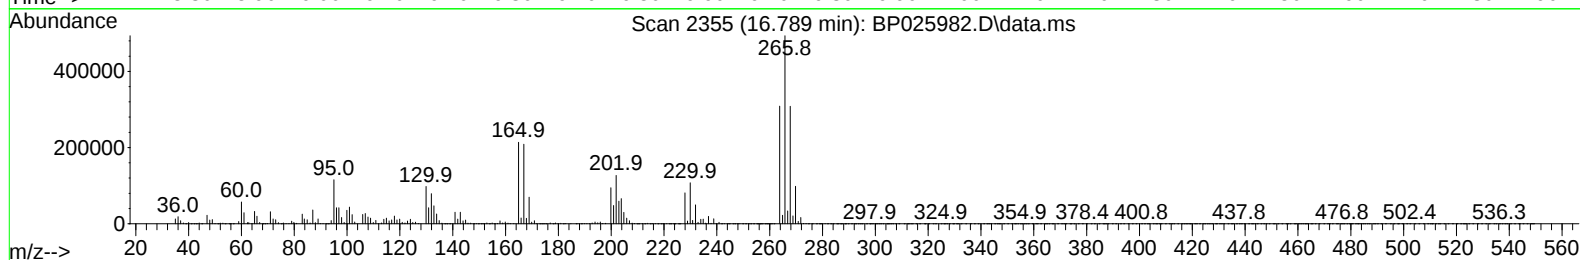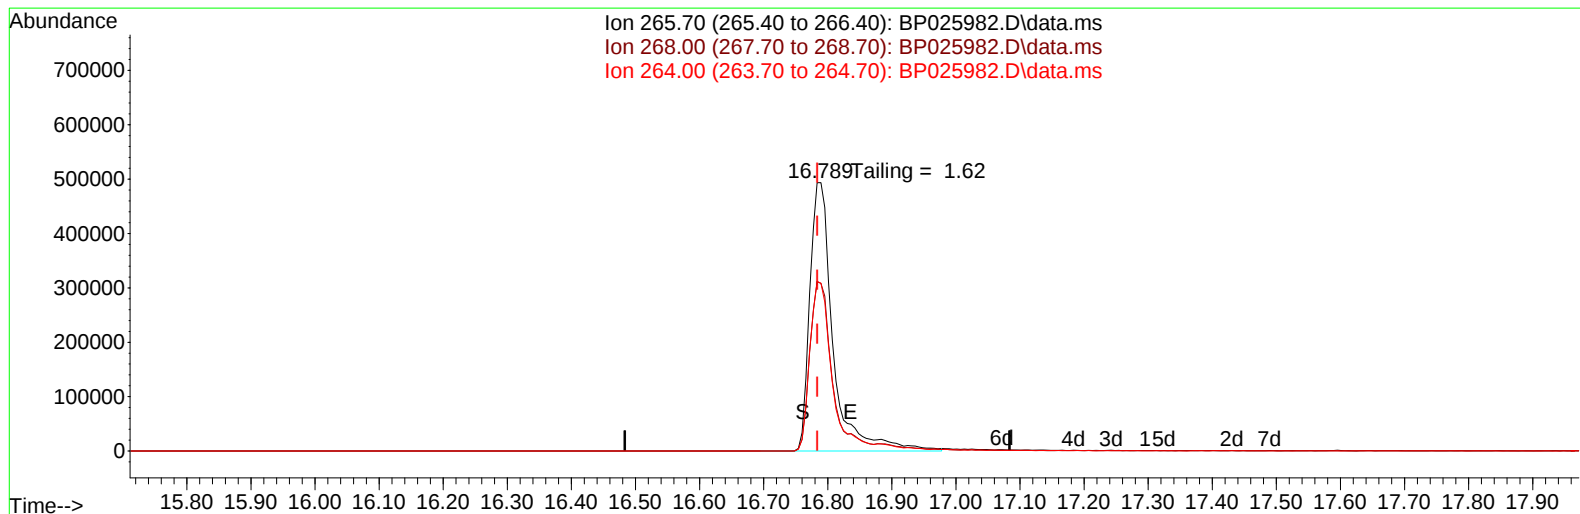

TIC: BP025982.D\data.ms

(70) Pentachlorophenol (C)

16.789min (+ 0.006) 113678.97 ng m




response 1252591

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.44
264.00	66.10	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102125\
Data File : BP025982.D
Acq On : 21 Oct 2025 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 21 12:28:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

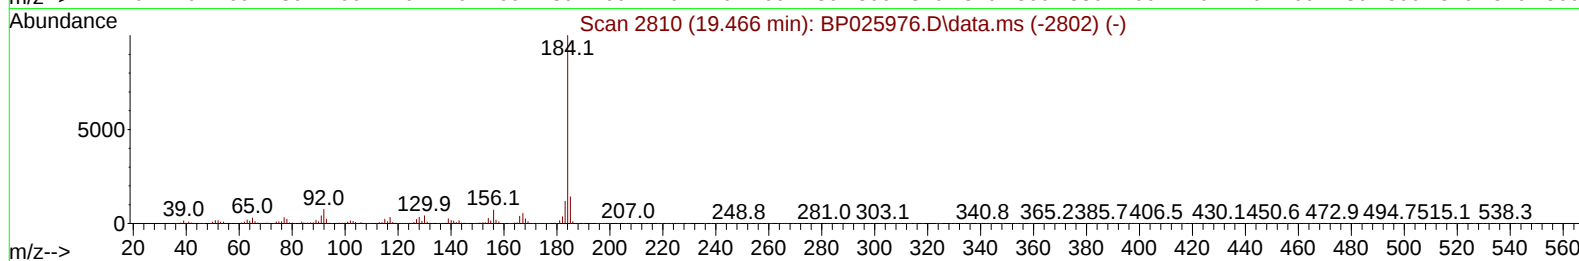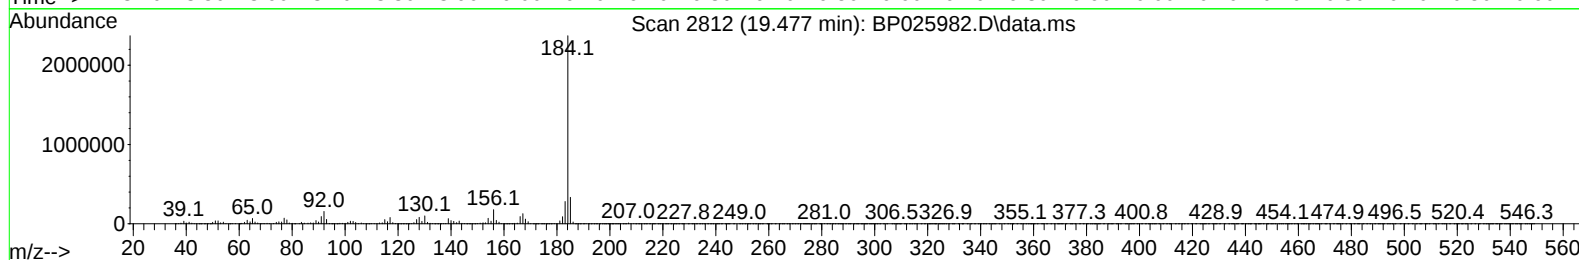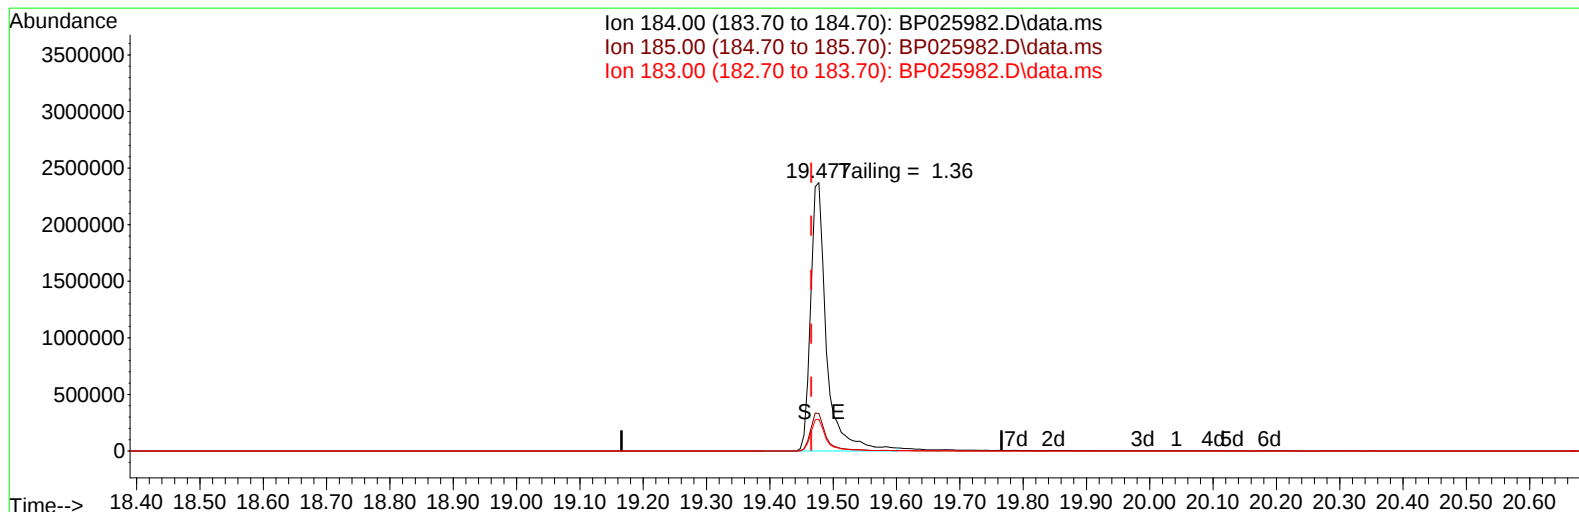

TIC: BP025982.D\data.ms

(77) Benzidine

19.477min (+ 0.012) 4661866.51 ng m

response 4182485

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.01
183.00	11.80	11.84
0.00	0.00	0.00