
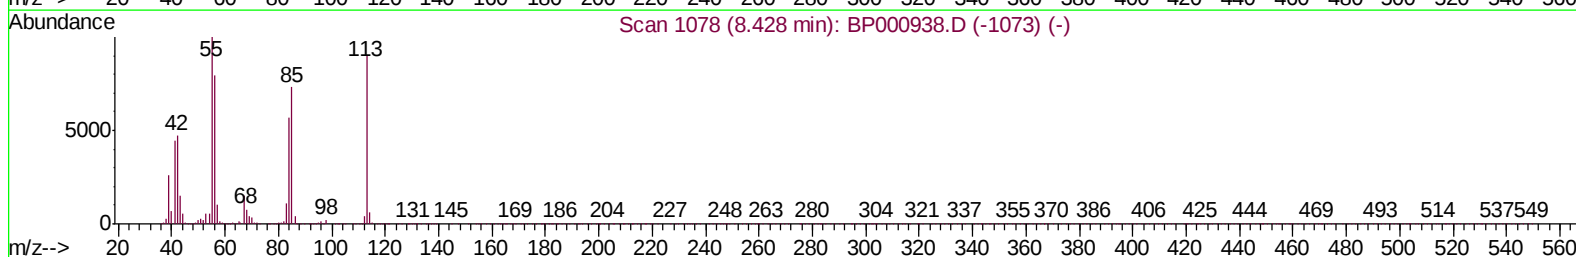
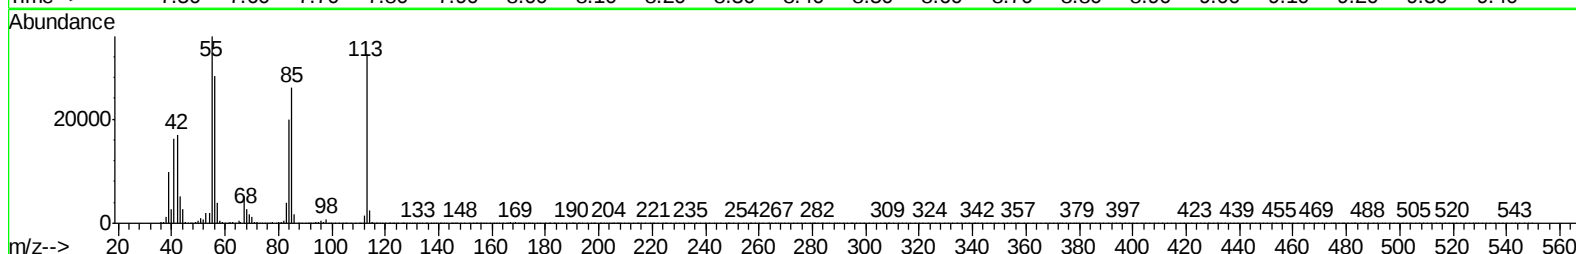


Data File : BP000942.D
Acq On : 22 Oct 2019 15:10
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 23 05:32:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 19 22:14:11 2019
Response via : Initial Calibration

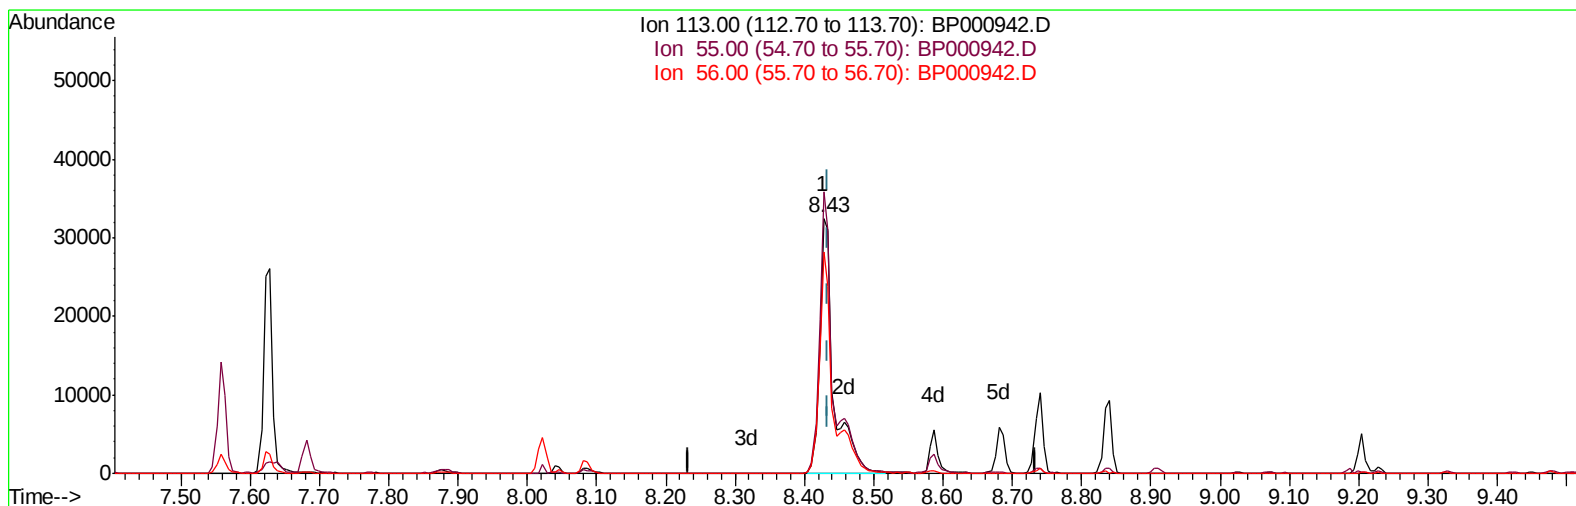

TIC: BP000942.D

(32) Caprolactam

8.428min (-0.006) 19.28ng/ul m

response 45955

Ion	Exp%	Act%
113.00	100	100
55.00	116.30	110.34
56.00	86.80	86.80
0.00	0.00	0.00