
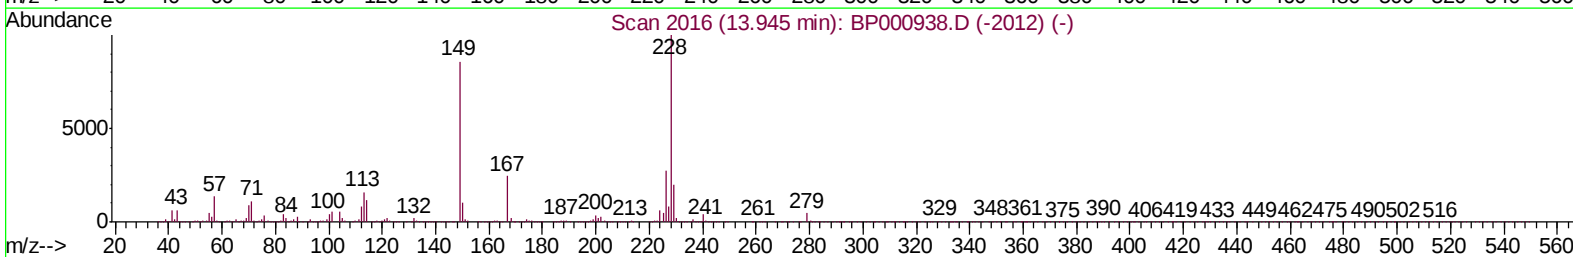
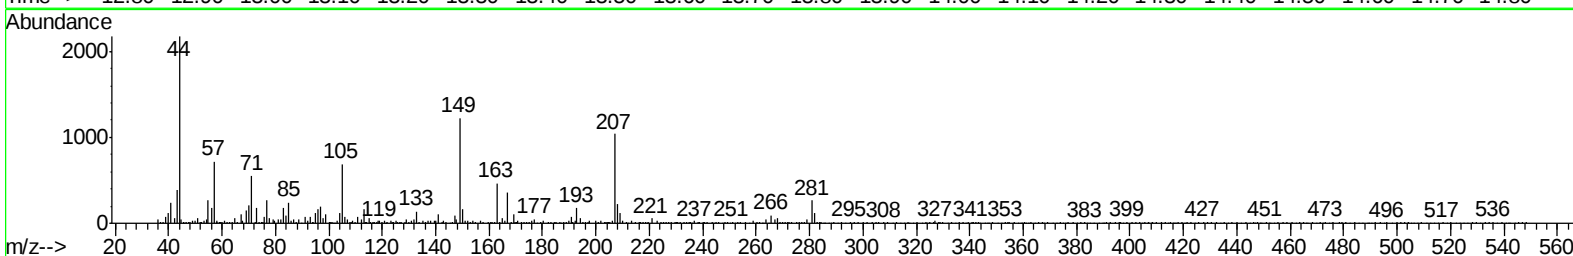


Data File : BP000942.D
Acq On : 22 Oct 2019 15:10
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 23 05:32:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 19 22:14:11 2019
Response via : Initial Calibration

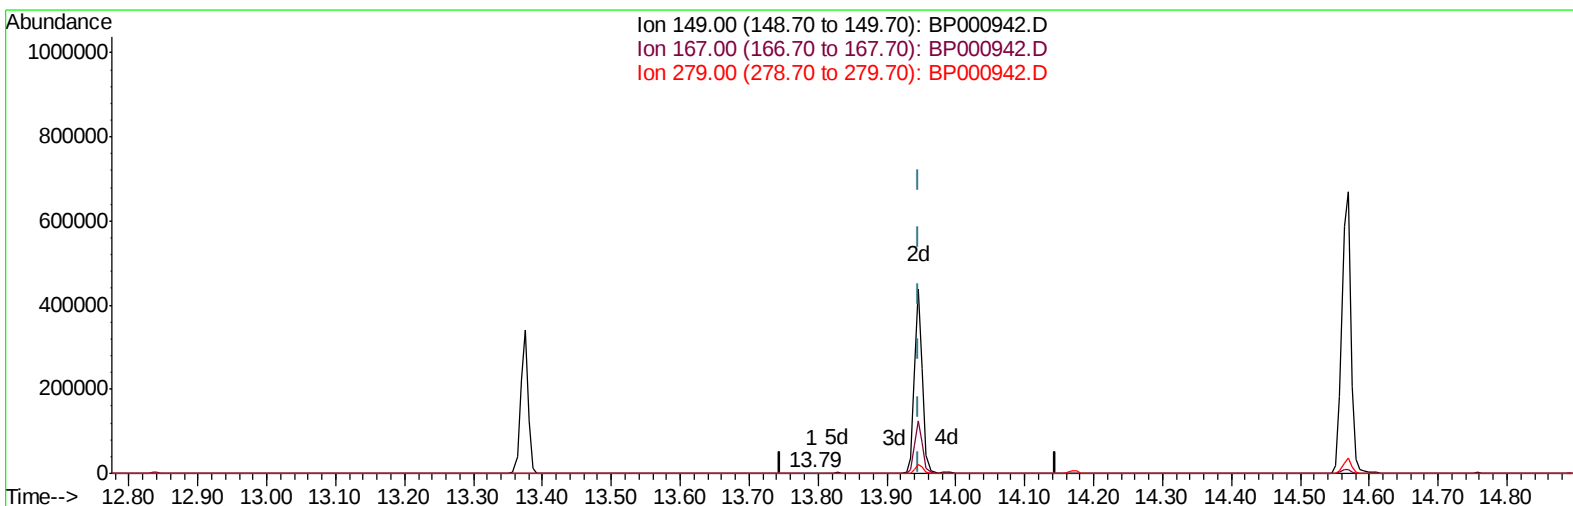

TIC: BP000942.D

(84) Bis(2-ethylhexyl)phthalate

13.793min (-0.153) 0.04ng/ul

response 824

Ion	Exp%	Act%
149.00	100	100
167.00	27.90	29.66
279.00	4.00	3.43
0.00	0.00	0.00