

Data File : BP000942.D

Acq On : 22 Oct 2019 15:10

Operator : JU

Sample : SSTDCCC020

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Oct 23 05:32:47 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Oct 19 22:14:11 2019

Response via : Initial Calibration

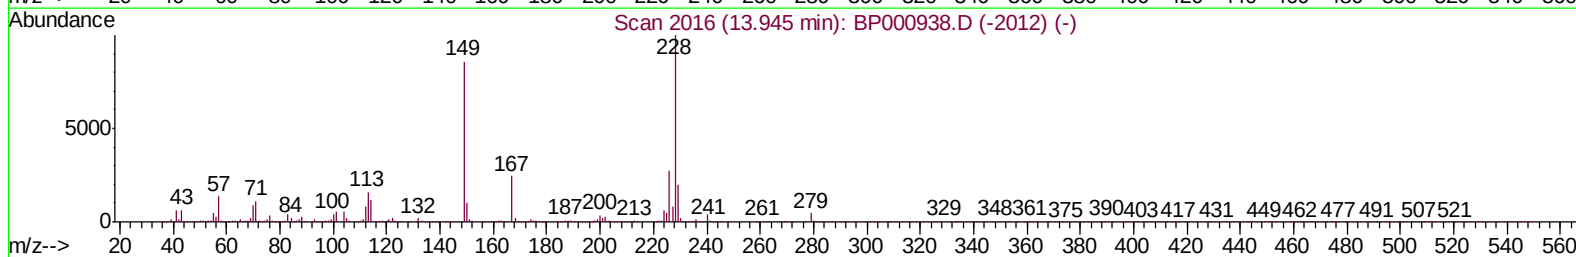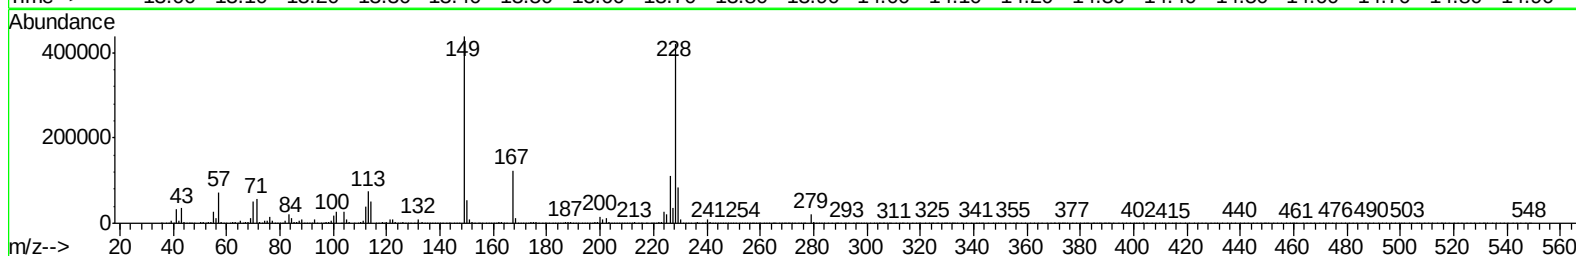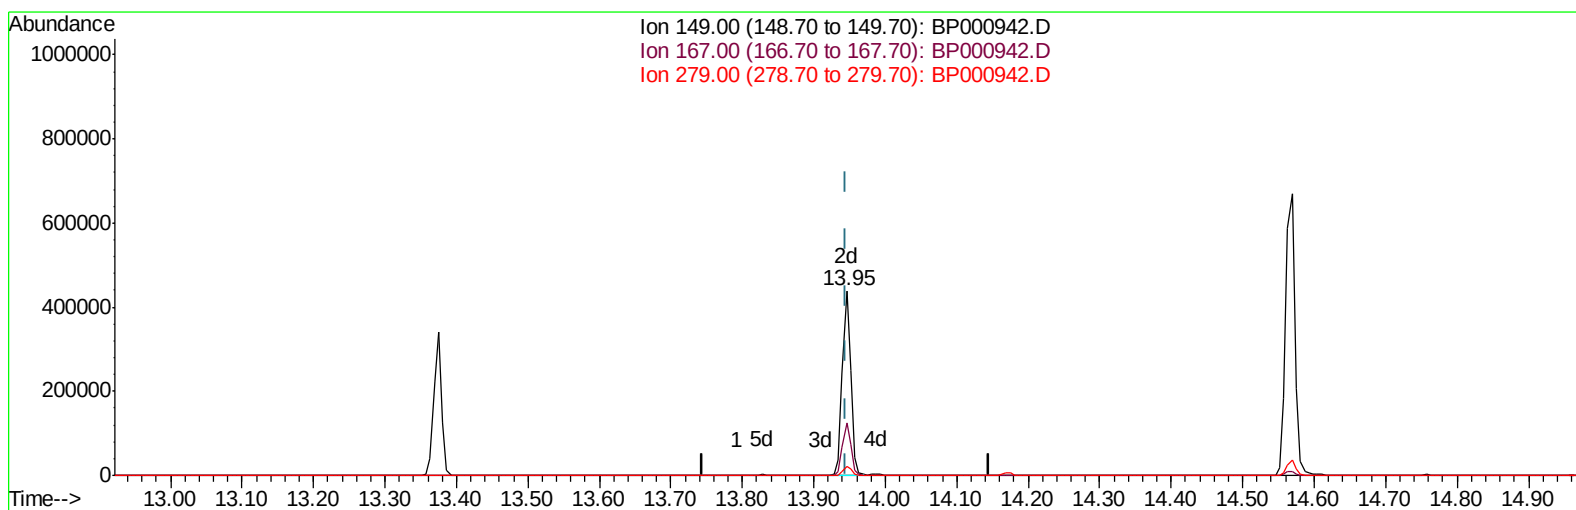

TIC: BP000942.D

(84) Bis(2-ethylhexyl)phthalate

13.946min (+0.000) 19.45ng/ul m

response 359528

Ion	Exp%	Act%
149.00	100	100
167.00	27.90	28.21
279.00	4.00	4.95#
0.00	0.00	0.00