
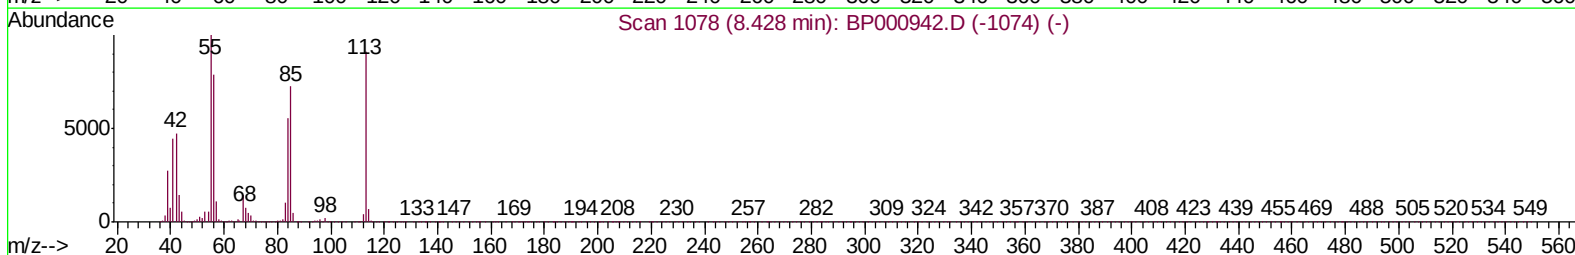
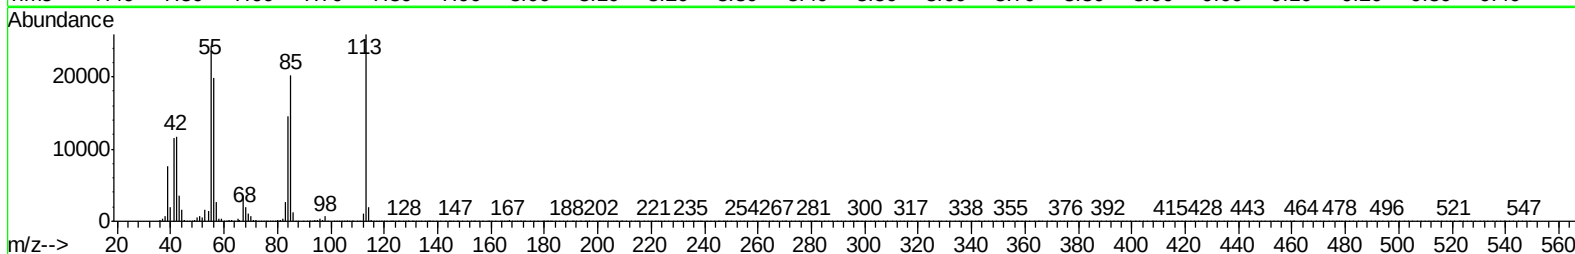


Data File : BP000967.D
Acq On : 23 Oct 2019 02:20
Operator : JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 23 05:40:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 23 05:34:10 2019
Response via : Initial Calibration

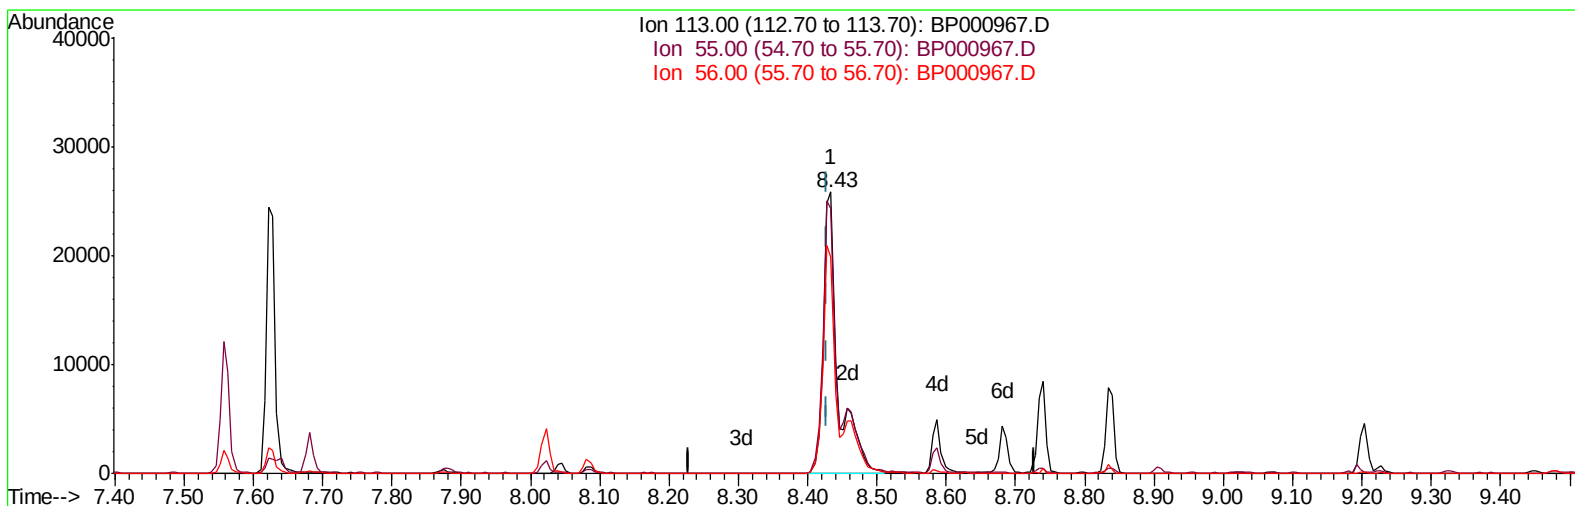

TIC: BP000967.D

(32) Caprolactam

8.434min (+0.006) 17.03ng/ul m

response 37553

Ion	Exp%	Act%
113.00	100	100
55.00	116.30	94.06
56.00	86.80	76.62
0.00	0.00	0.00