

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP102219\
 Data File : BP000966.D
 Acq On : 23 Oct 2019 01:31
 Operator : JU
 Sample : PB124178BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.346	41	44	53	rBV	22107	32285	2.79%	0.201%
2	3.740	277	281	287	rBV	3995	6650	0.58%	0.041%
3	6.375	726	729	734	rBV	558054	510309	44.14%	3.176%
4	6.422	734	737	746	rVV	436595	409411	35.41%	2.548%
5	6.511	749	752	766	rVB	827160	668725	57.85%	4.161%
6	6.740	787	791	805	rBV	671226	606484	52.46%	3.774%
7	7.122	853	856	876	rBV	839716	801419	69.32%	4.987%
8	7.299	882	886	895	rBV	699964	563310	48.73%	3.505%
9	7.622	938	941	956	rBV	463001	397972	34.43%	2.476%
10	7.781	964	968	973	rVB8	822	1454	0.13%	0.009%
11	7.875	980	984	1005	rBV	607588	656516	56.79%	4.085%
12	8.022	1005	1009	1012	rBV	975014	768669	66.49%	4.783%
13	8.093	1019	1021	1028	rVB	8192	10417	0.90%	0.065%
14	8.710	1123	1126	1137	rVB	11315	12072	1.04%	0.075%
15	8.805	1139	1142	1145	rBV3	1929	2000	0.17%	0.012%
16	9.475	1253	1256	1260	rBV	1079587	905585	78.33%	5.635%
17	9.628	1278	1282	1286	rBV	1483697	1156054	100.00%	7.194%
18	9.687	1291	1292	1299	rVB7	1431	1778	0.15%	0.011%
19	9.781	1305	1308	1312	rBV	1300222	1155873	99.98%	7.193%
20	9.905	1326	1329	1343	rBV	164930	246460	21.32%	1.534%
21	10.199	1376	1379	1385	rVB4	1280	1493	0.13%	0.009%
22	10.304	1394	1397	1401	rBV	1271315	1125420	97.35%	7.003%
23	10.387	1407	1411	1417	rBV	169856	181779	15.72%	1.131%
24	10.434	1417	1419	1423	rVB	17816	16790	1.45%	0.104%
25	10.581	1441	1444	1447	rBV	3507	2868	0.25%	0.018%
26	10.734	1467	1470	1473	rVB	4533	3907	0.34%	0.024%
27	11.099	1530	1532	1535	rVB2	1937	1622	0.14%	0.010%
28	11.163	1540	1543	1548	rBV	2258	2367	0.20%	0.015%
29	11.281	1559	1563	1567	rBV	902906	719749	62.26%	4.479%
30	11.340	1569	1573	1577	rBV	1172005	961217	83.15%	5.981%
31	12.493	1765	1769	1775	rBV	11692	10764	0.93%	0.067%
32	12.651	1793	1796	1799	rBV	8254	7991	0.69%	0.050%
33	12.722	1804	1808	1812	rBV	1245505	1067265	92.32%	6.641%
34	13.022	1856	1859	1865	rBV8	937	1456	0.13%	0.009%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP102219\
 Data File : BP000966.D
 Acq On : 23 Oct 2019 01:31
 Operator : JU
 Sample : PB124178BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	13.281	1901	1903	1906	rVB3	1635	1489	0.13%	0.009%
36	13.534	1942	1946	1949	rBV6	2059	2888	0.25%	0.018%
37	13.563	1949	1951	1956	rVB6	1190	1501	0.13%	0.009%
38	13.622	1957	1961	1962	rBV4	2160	2686	0.23%	0.017%
39	13.810	1990	1993	1999	rVV7	2912	3522	0.30%	0.022%
40	13.875	2002	2004	2009	rBV6	1834	2901	0.25%	0.018%
41	13.957	2014	2018	2025	rVV	1118510	1059514	91.65%	6.593%
42	14.128	2043	2047	2051	rBV5	5318	9292	0.80%	0.058%
43	14.440	2097	2100	2103	rBV4	4173	4225	0.37%	0.026%
44	14.745	2149	2152	2161	rVB3	8271	10982	0.95%	0.068%
45	14.957	2185	2188	2193	rVB2	12562	13361	1.16%	0.083%
46	15.087	2206	2210	2221	rVB4	6924	11667	1.01%	0.073%
47	15.339	2248	2253	2263	rBV	913393	1070634	92.61%	6.662%
48	15.428	2263	2268	2281	rVB	627600	816429	70.62%	5.080%
49	15.898	2344	2348	2356	rBV3	8351	14379	1.24%	0.089%
50	15.992	2360	2364	2370	rVB4	3962	7000	0.61%	0.044%
51	16.398	2429	2433	2439	rBV3	6749	11884	1.03%	0.074%
52	16.986	2531	2533	2541	rVB9	4208	7471	0.65%	0.046%


Sum of corrected areas: 16069956

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP102219\
Data File : BP000966.D
Acq On : 23 Oct 2019 01:31
Operator : JU
Sample : PB124178BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK78

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

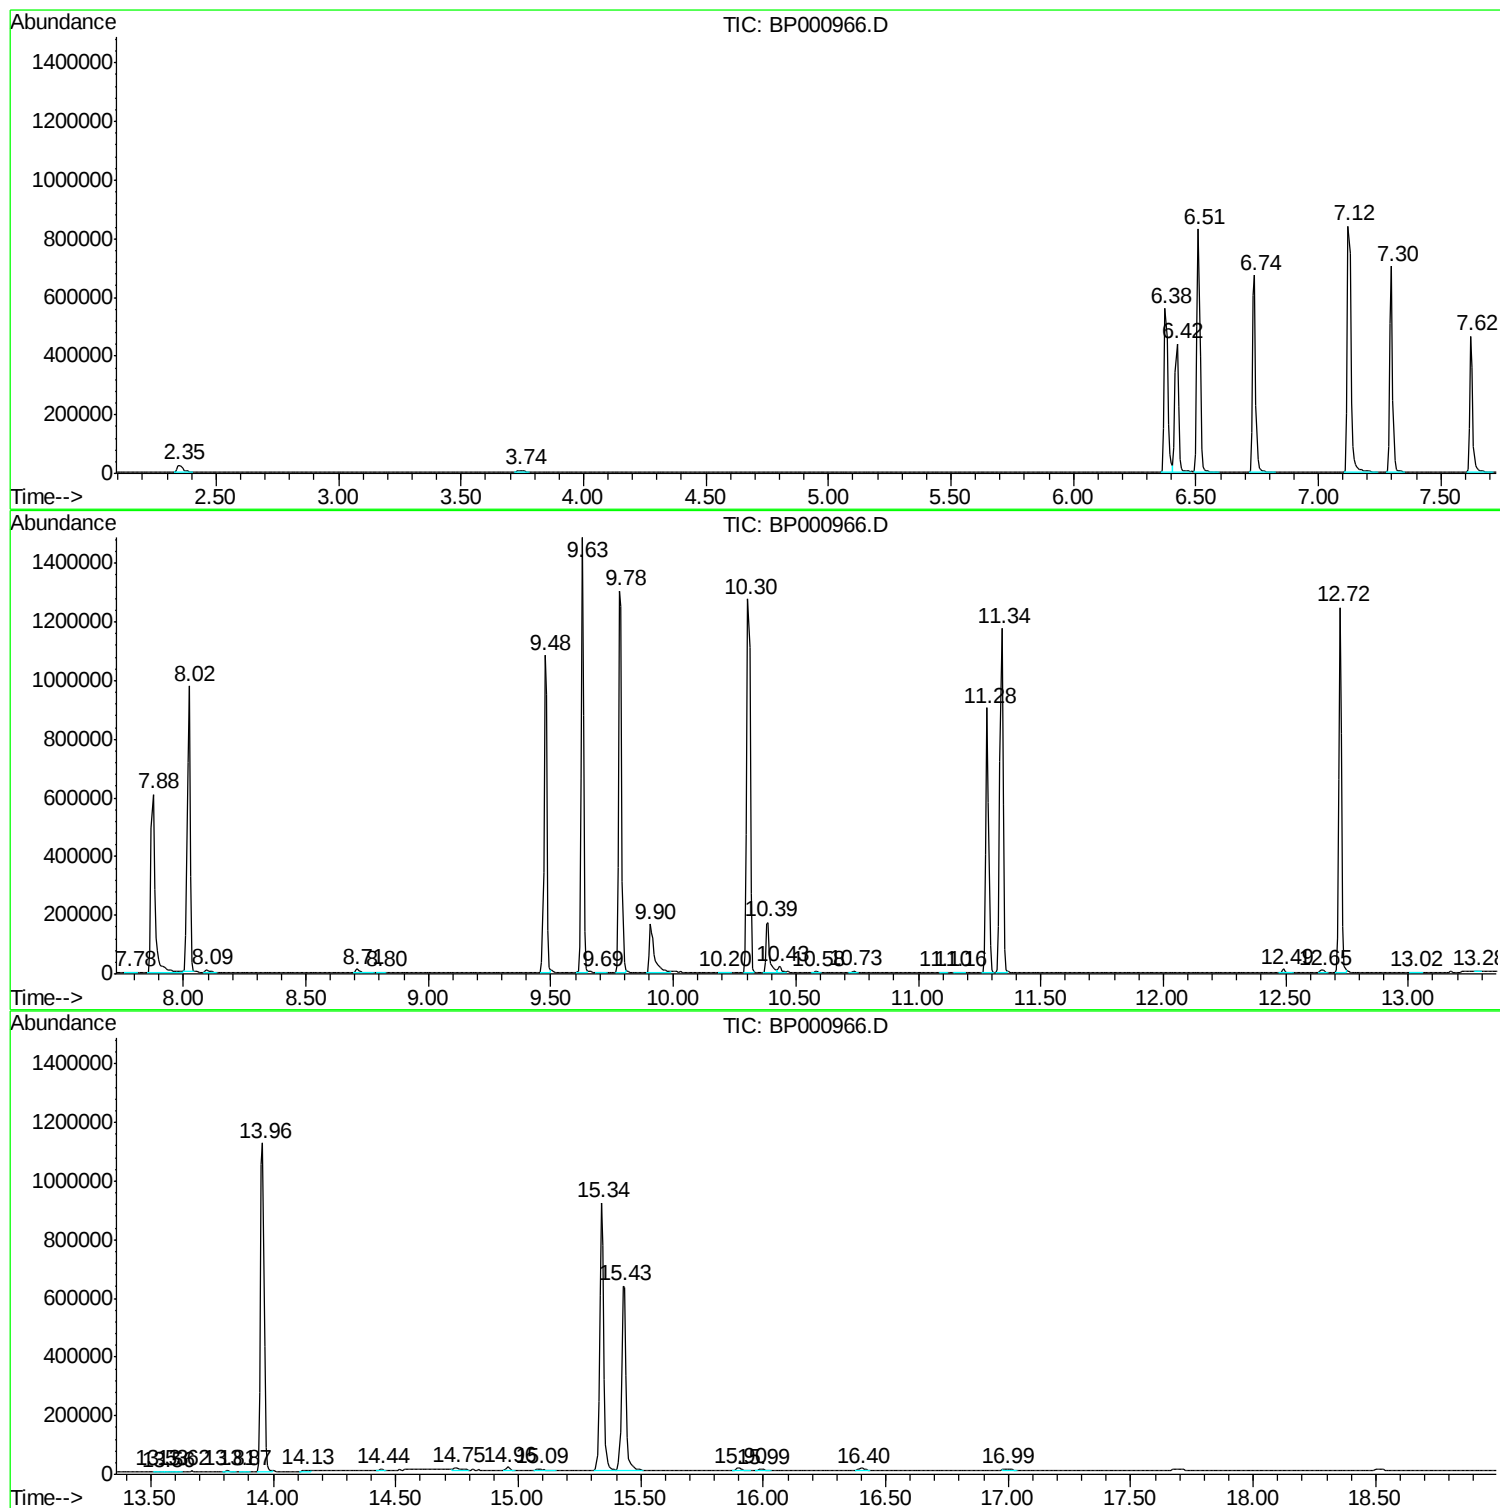

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP102219\
Data File : BP000966.D
Acq On : 23 Oct 2019 01:31
Operator : JU
Sample : PB124178BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK78

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP102219\
Data File : BP000966.D
Acq On : 23 Oct 2019 01:31
Operator : JU
Sample : PB124178BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK78

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc