
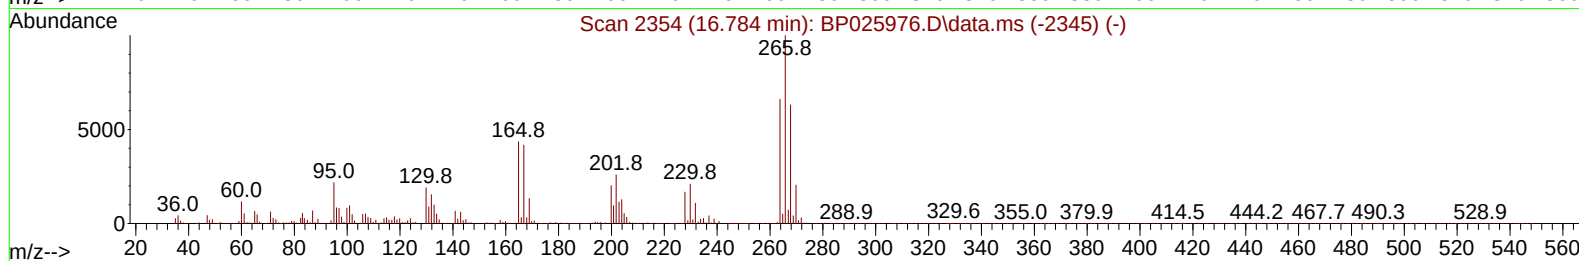
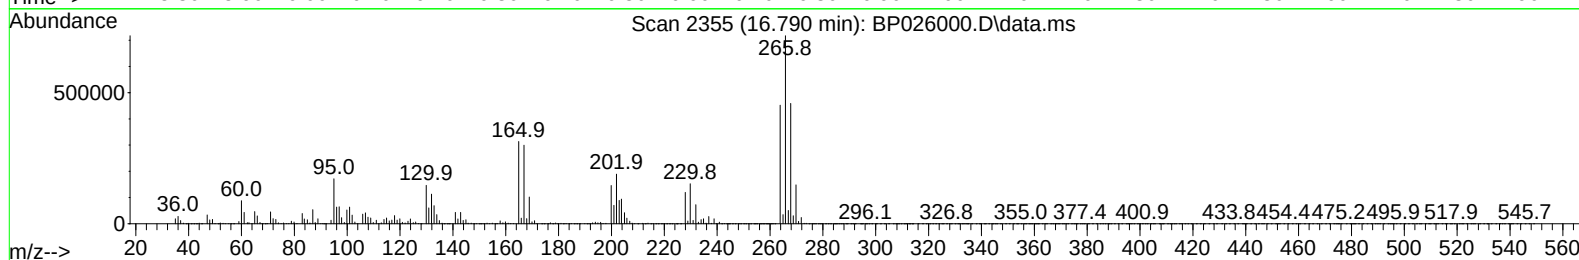


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102225\
Data File : BP026000.D
Acq On : 22 Oct 2025 15:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 16:39:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

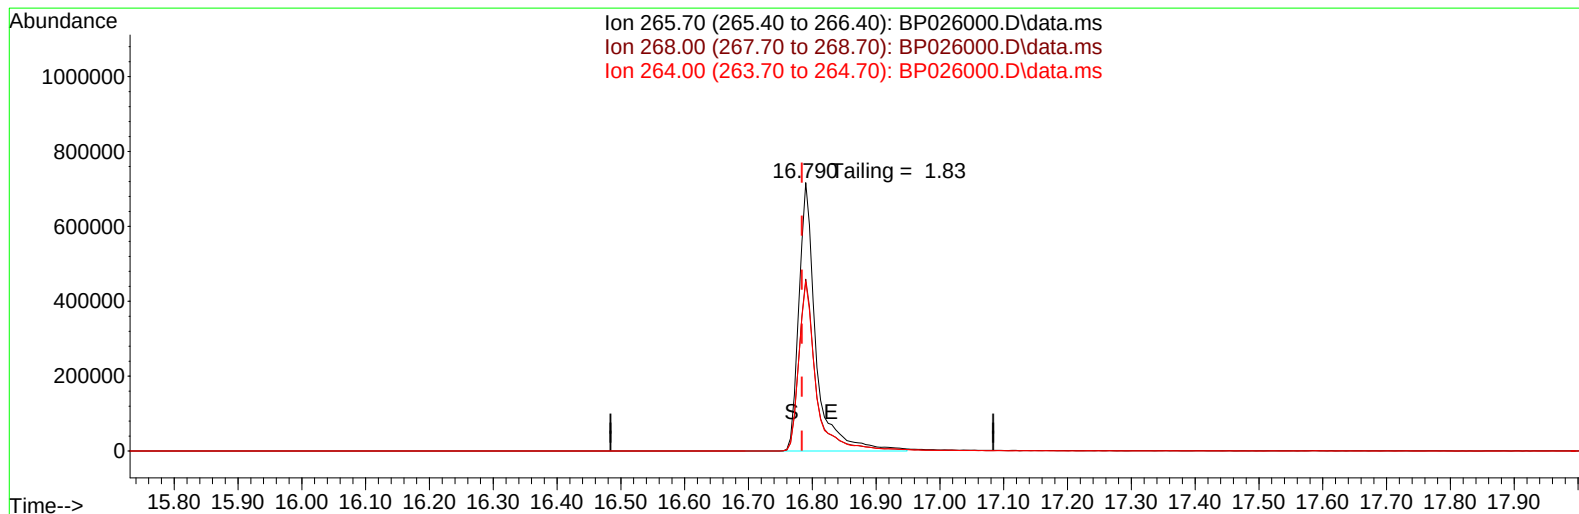

TIC: BP026000.D\data.ms

(70) Pentachlorophenol (C)




16.790min (+ 0.006) 9533301.26 ng

response 1354031

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.01
264.00	66.10	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102225\
Data File : BP026000.D
Acq On : 22 Oct 2025 15:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 16:39:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

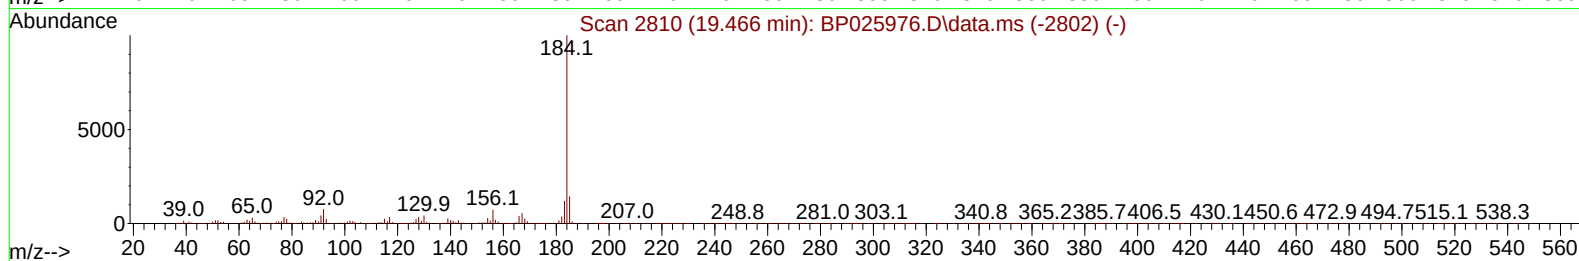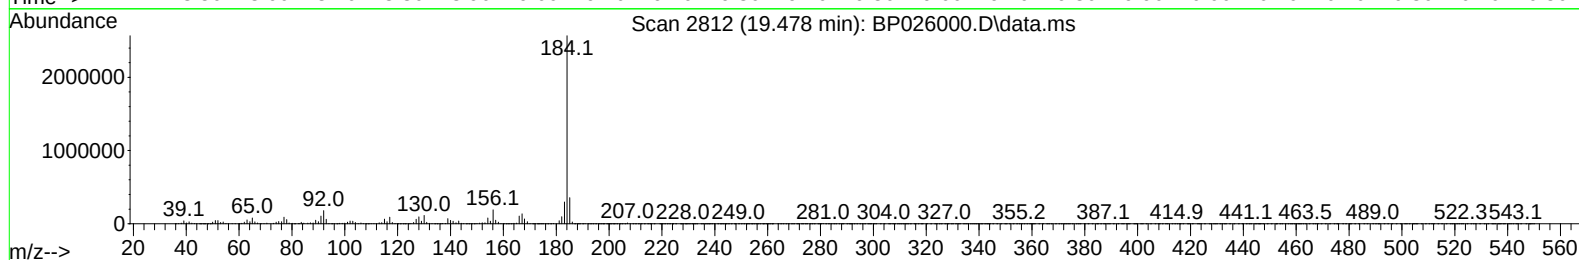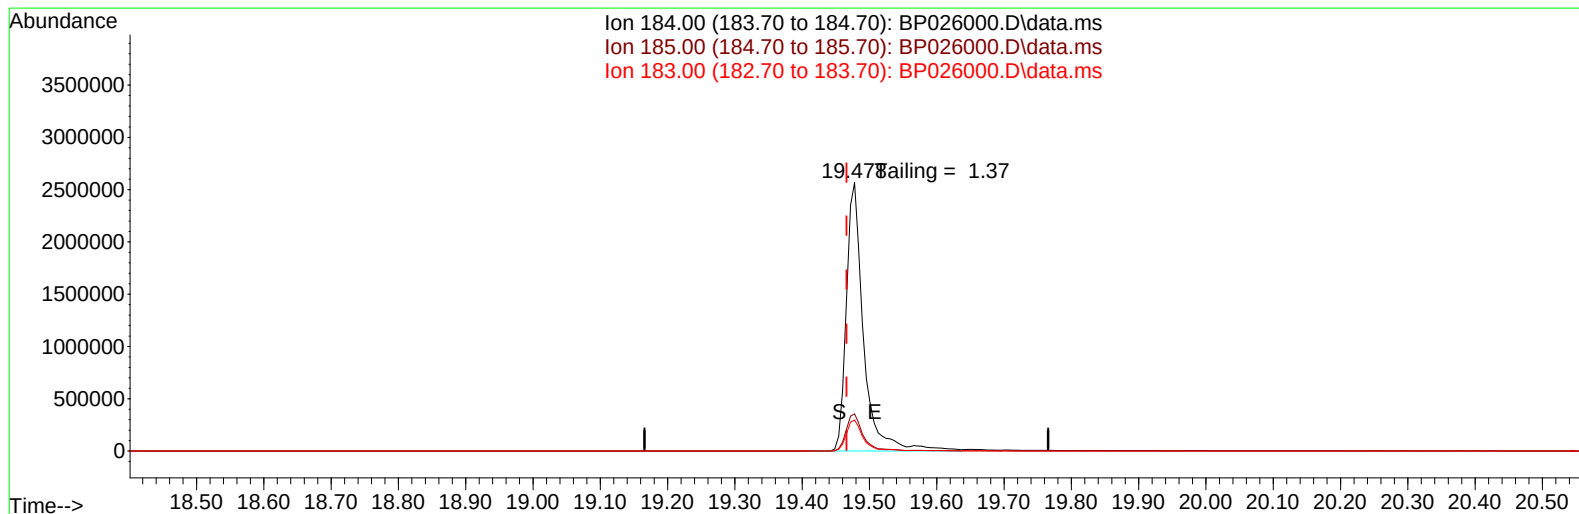

TIC: BP026000.D\data.ms

(77) Benzidine

19.478min (+ 0.012) 2937951.43 ng

response 4424447

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.86
183.00	11.80	11.60
0.00	0.00	0.00