

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017790.D
 Acq On : 24 Oct 2023 22:15
 Operator : MA/JU
 Sample : 04927-10
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD14

Quant Time: Oct 25 01:59:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	138857	20.000	ng/ul	0.00
20) Naphthalene-d8	10.716	136	573689	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	352075	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.369	188	734059	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.510	240	627950	20.000	ng/ul	0.00
88) Perylene-d12	24.063	264	653398	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	9526	2.552	ng/uL	0.00
4) Pyridine-d5	3.705	84	16529	1.691	ng/ul	0.01
7) Phenol-d5	7.040	99	164497	14.236	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	113193	15.862	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	140931	14.954	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	113089	12.463	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	65525	14.095	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.805	143	72268	14.070	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	126299	12.535	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	95066	7.210	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	417031	14.110	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	464573	14.095	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	32720	7.770	ng/ul	0.02
60) Fluorene-d10	15.581	176	351313	13.751	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.734	200	39882	8.248	ng/ul	0.00
73) Anthracene-d10	17.469	188	495521	13.210	ng/ul	0.00
81) Pyrene-d10	19.728	212	627376	15.936	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.892	264	524491	14.412	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.740	105	52936	3.711	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017790.D
Acq On : 24 Oct 2023 22:15
Operator : MA/JU
Sample : 04927-10
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD14

Quant Time: Oct 25 01:59:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

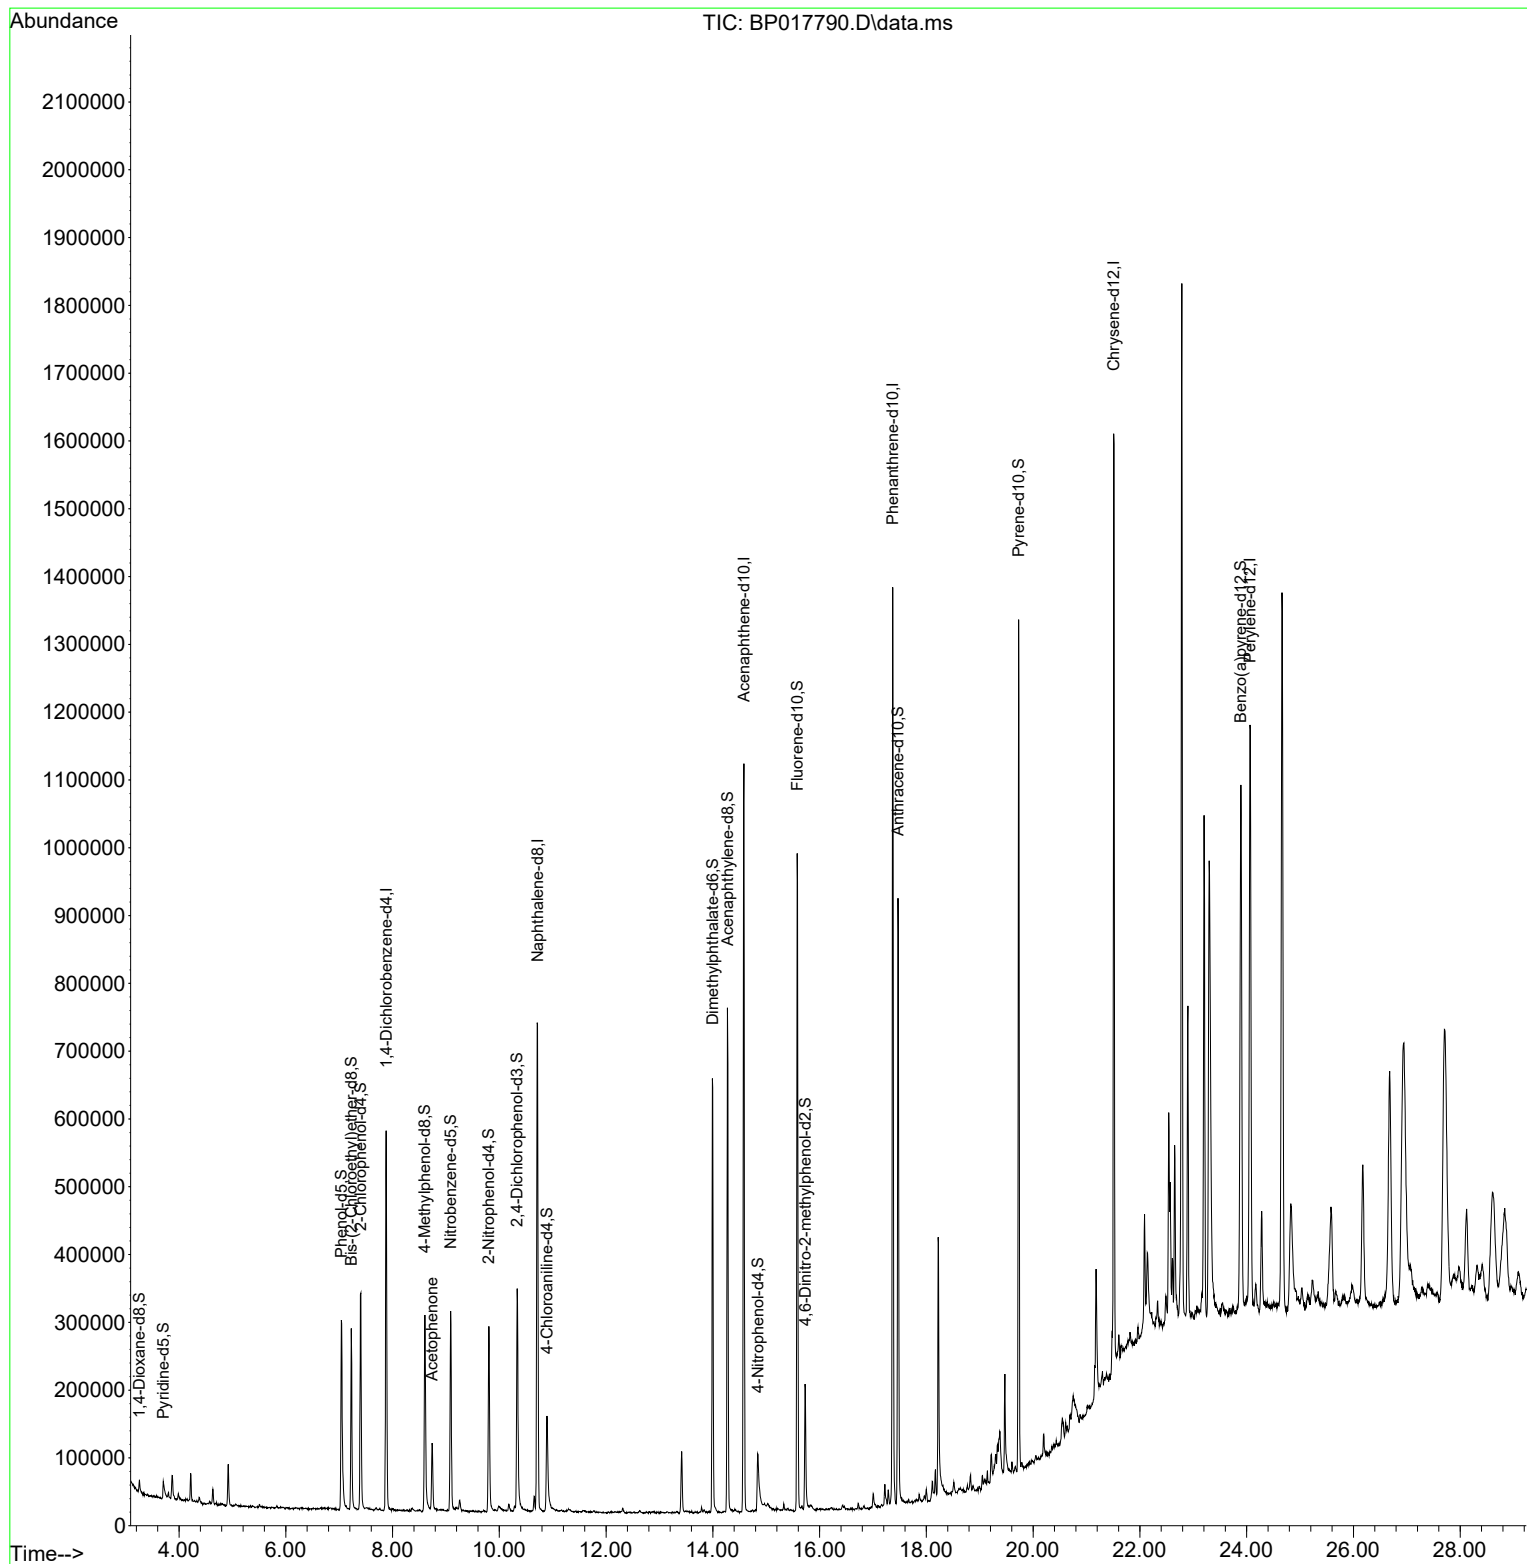

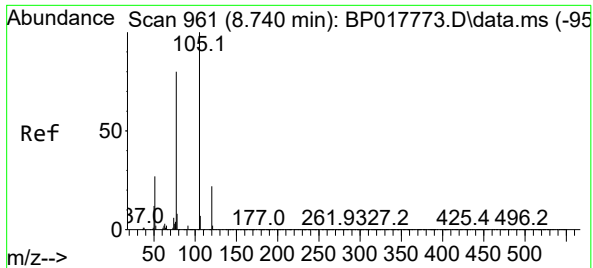

#16
 Acetophenone
 Concen: 3.711 ng/ul
 RT: 8.740 min Scan# 90
 Delta R.T. -0.006 min
 Lab File: BP017790.D
 Acq: 24 Oct 2023 22:15

Instrument :
 BNA_P
 ClientSampleId :
 GCD14

Tgt Ion:	105	Resp:	52936
Ion Ratio	Lower	Upper	
105	100		
77	82.2	64.4	96.6
51	28.2	21.2	31.8

