

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017760.D
 Acq On : 23 Oct 2023 21:09
 Operator : MA/JU
 Sample : 04926-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCCZ7

Quant Time: Oct 24 06:06:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	139749	20.000	ng/ul	0.00
20) Naphthalene-d8	10.716	136	559725	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	334897	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.369	188	691739	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.516	240	556779	20.000	ng/ul	0.00
88) Perylene-d12	24.068	264	573834	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	10929	2.909	ng/uL	0.00
4) Pyridine-d5	3.705	84	15782	1.605	ng/ul	0.01
7) Phenol-d5	7.046	99	172891	14.867	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	124054	17.273	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	145152	15.303	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	105778	11.583	ng/ul	0.00
21) Nitrobenzene-d5	9.093	128	65661	14.477	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	66792	13.328	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	125397	12.756	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	98059	7.622	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	431994	15.366	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	475557	15.168	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	27230	6.798	ng/ul	0.02
60) Fluorene-d10	15.586	176	367935	15.140	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	35662	7.827	ng/ul	0.00
73) Anthracene-d10	17.475	188	557336	15.766	ng/ul	0.00
81) Pyrene-d10	19.733	212	646950	18.533	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.898	264	500291	15.653	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.746	105	44826	3.122	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017760.D
Acq On : 23 Oct 2023 21:09
Operator : MA/JU
Sample : 04926-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCCZ7

Quant Time: Oct 24 06:06:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

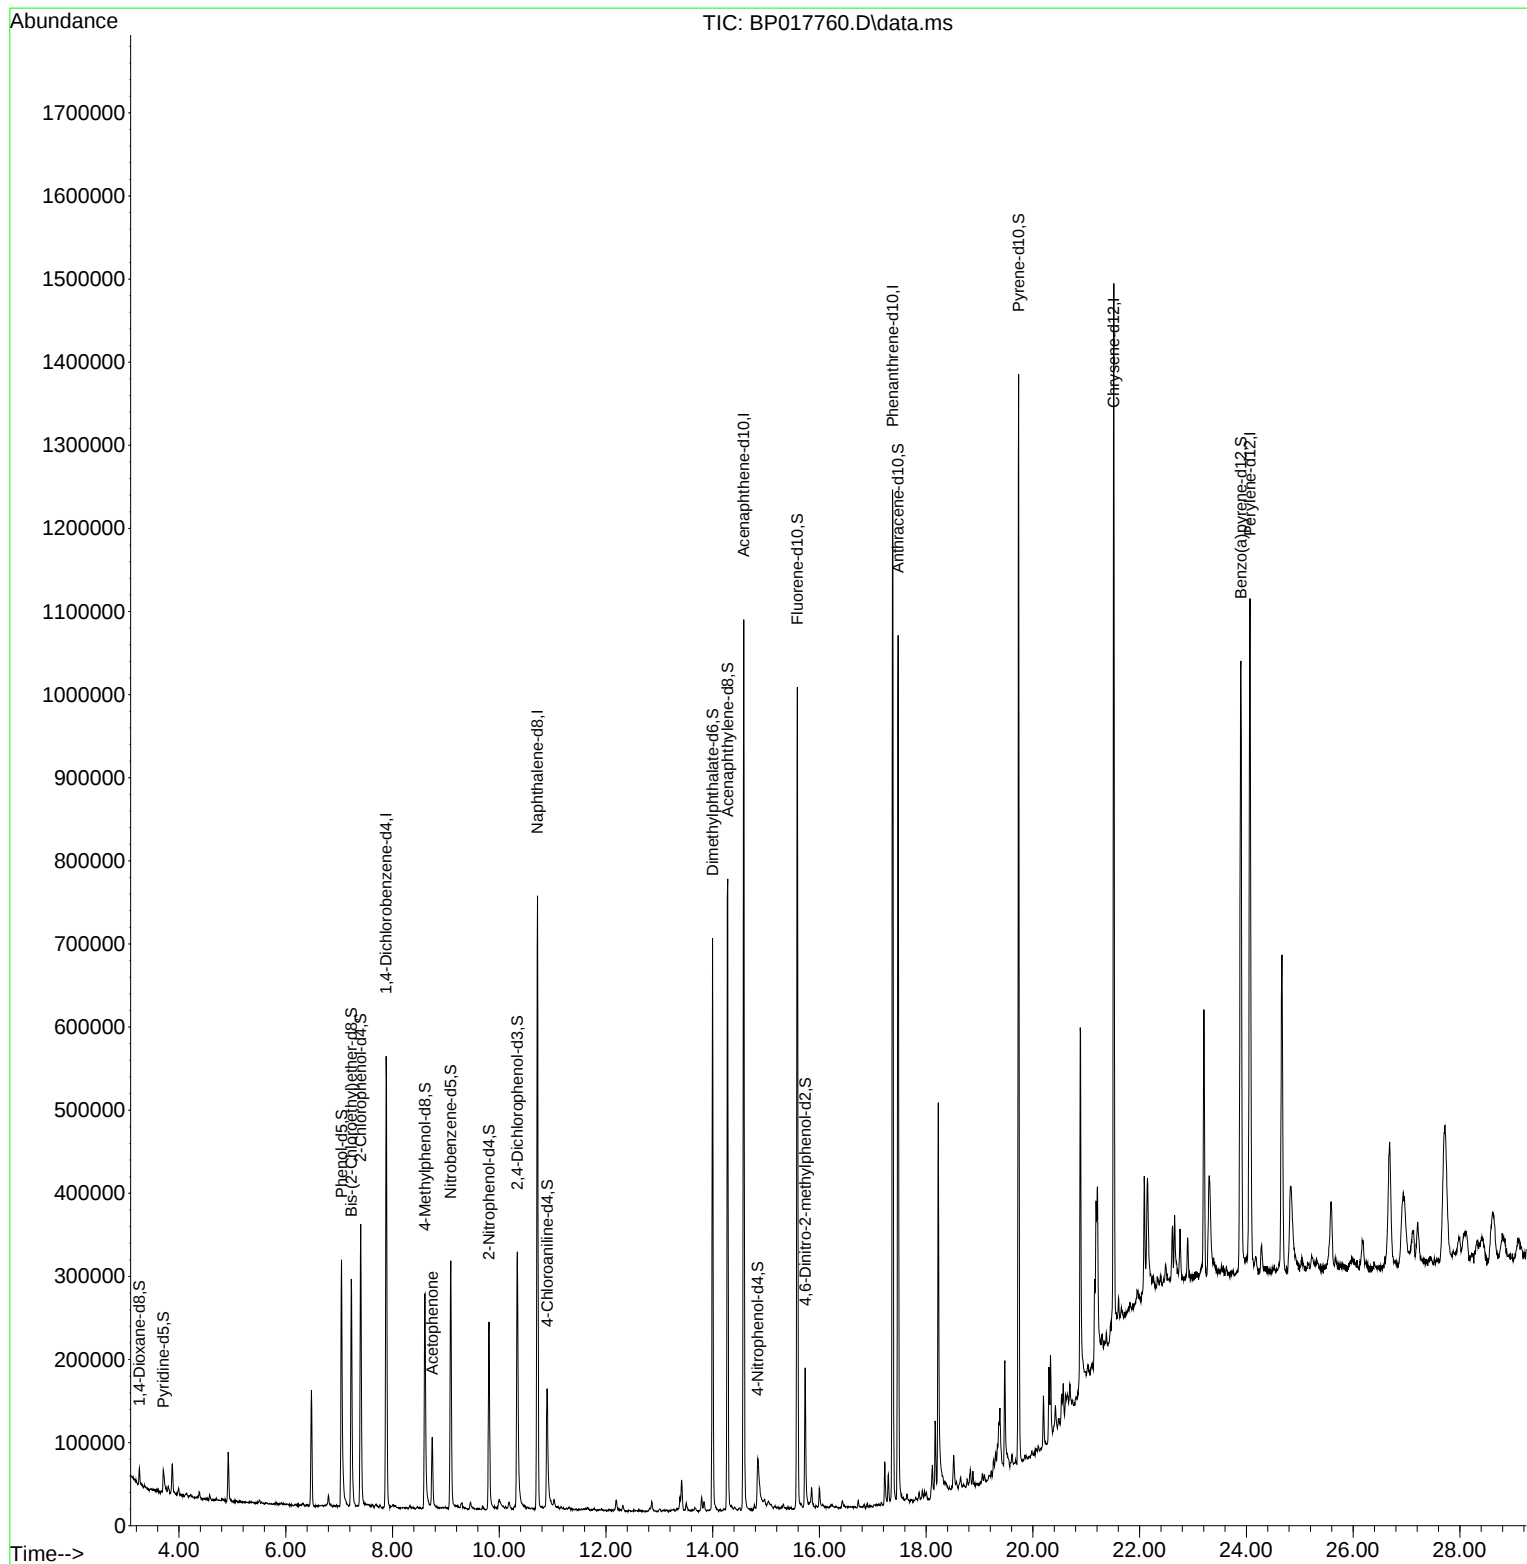

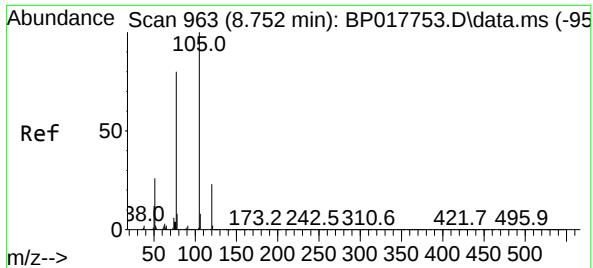

#16
 Acetophenone
 Concen: 3.122 ng/ul
 RT: 8.746 min Scan# 90
 Delta R.T. -0.000 min
 Lab File: BP017760.D
 Acq: 23 Oct 2023 21:09

Instrument :
 BNA_P
 ClientSampleId :
 GCCZ7

Tgt Ion:	105	Resp:	44826
Ion	Ratio	Lower	Upper
105	100		
77	79.4	64.4	96.6
51	29.1	21.2	31.8

