

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017761.D
 Acq On : 23 Oct 2023 21:43
 Operator : MA/JU
 Sample : 04926-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCCZ8

Quant Time: Oct 24 06:09:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	125346	20.000	ng/u1	0.00
20) Naphthalene-d8	10.716	136	502517	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	298319	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	623976	20.000	ng/u1	0.00
79) Chrysene-d12	21.516	240	498293	20.000	ng/u1	0.00
88) Perylene-d12	24.063	264	506656	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	11132	3.304	ng/uL	0.00
4) Pyridine-d5	3.699	84	25774	2.922	ng/u1	0.00
7) Phenol-d5	7.046	99	180187	17.275	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	125333	19.456	ng/u1	0.00
11) 2-Chlorophenol-d4	7.405	132	152599	17.937	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	112078	13.683	ng/u1	0.00
21) Nitrobenzene-d5	9.093	128	68030	16.707	ng/u1	0.00
24) 2-Nitrophenol-d4	9.805	143	69947	15.547	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	136139	15.426	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	106571	9.227	ng/u1	0.00
46) Dimethylphthalate-d6	13.999	166	441570	17.633	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	496695	17.785	ng/u1	0.00
54) 4-Nitrophenol-d4	14.846	143	28377	7.953	ng/u1	0.02
60) Fluorene-d10	15.587	176	382178	17.654	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	36682	8.925	ng/u1	0.00
73) Anthracene-d10	17.475	188	534779	16.771	ng/u1	0.00
81) Pyrene-d10	19.734	212	646333	20.689	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.892	264	499098	17.686	ng/u1	0.00
Target Compounds						
16) Acetophenone	8.746	105	44297	3.440	ng/u1	99
86) Bis(2-ethylhexyl)phtha...	21.375	149	38354	2.101	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017761.D
Acq On : 23 Oct 2023 21:43
Operator : MA/JU
Sample : 04926-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCCZ8

Quant Time: Oct 24 06:09:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration




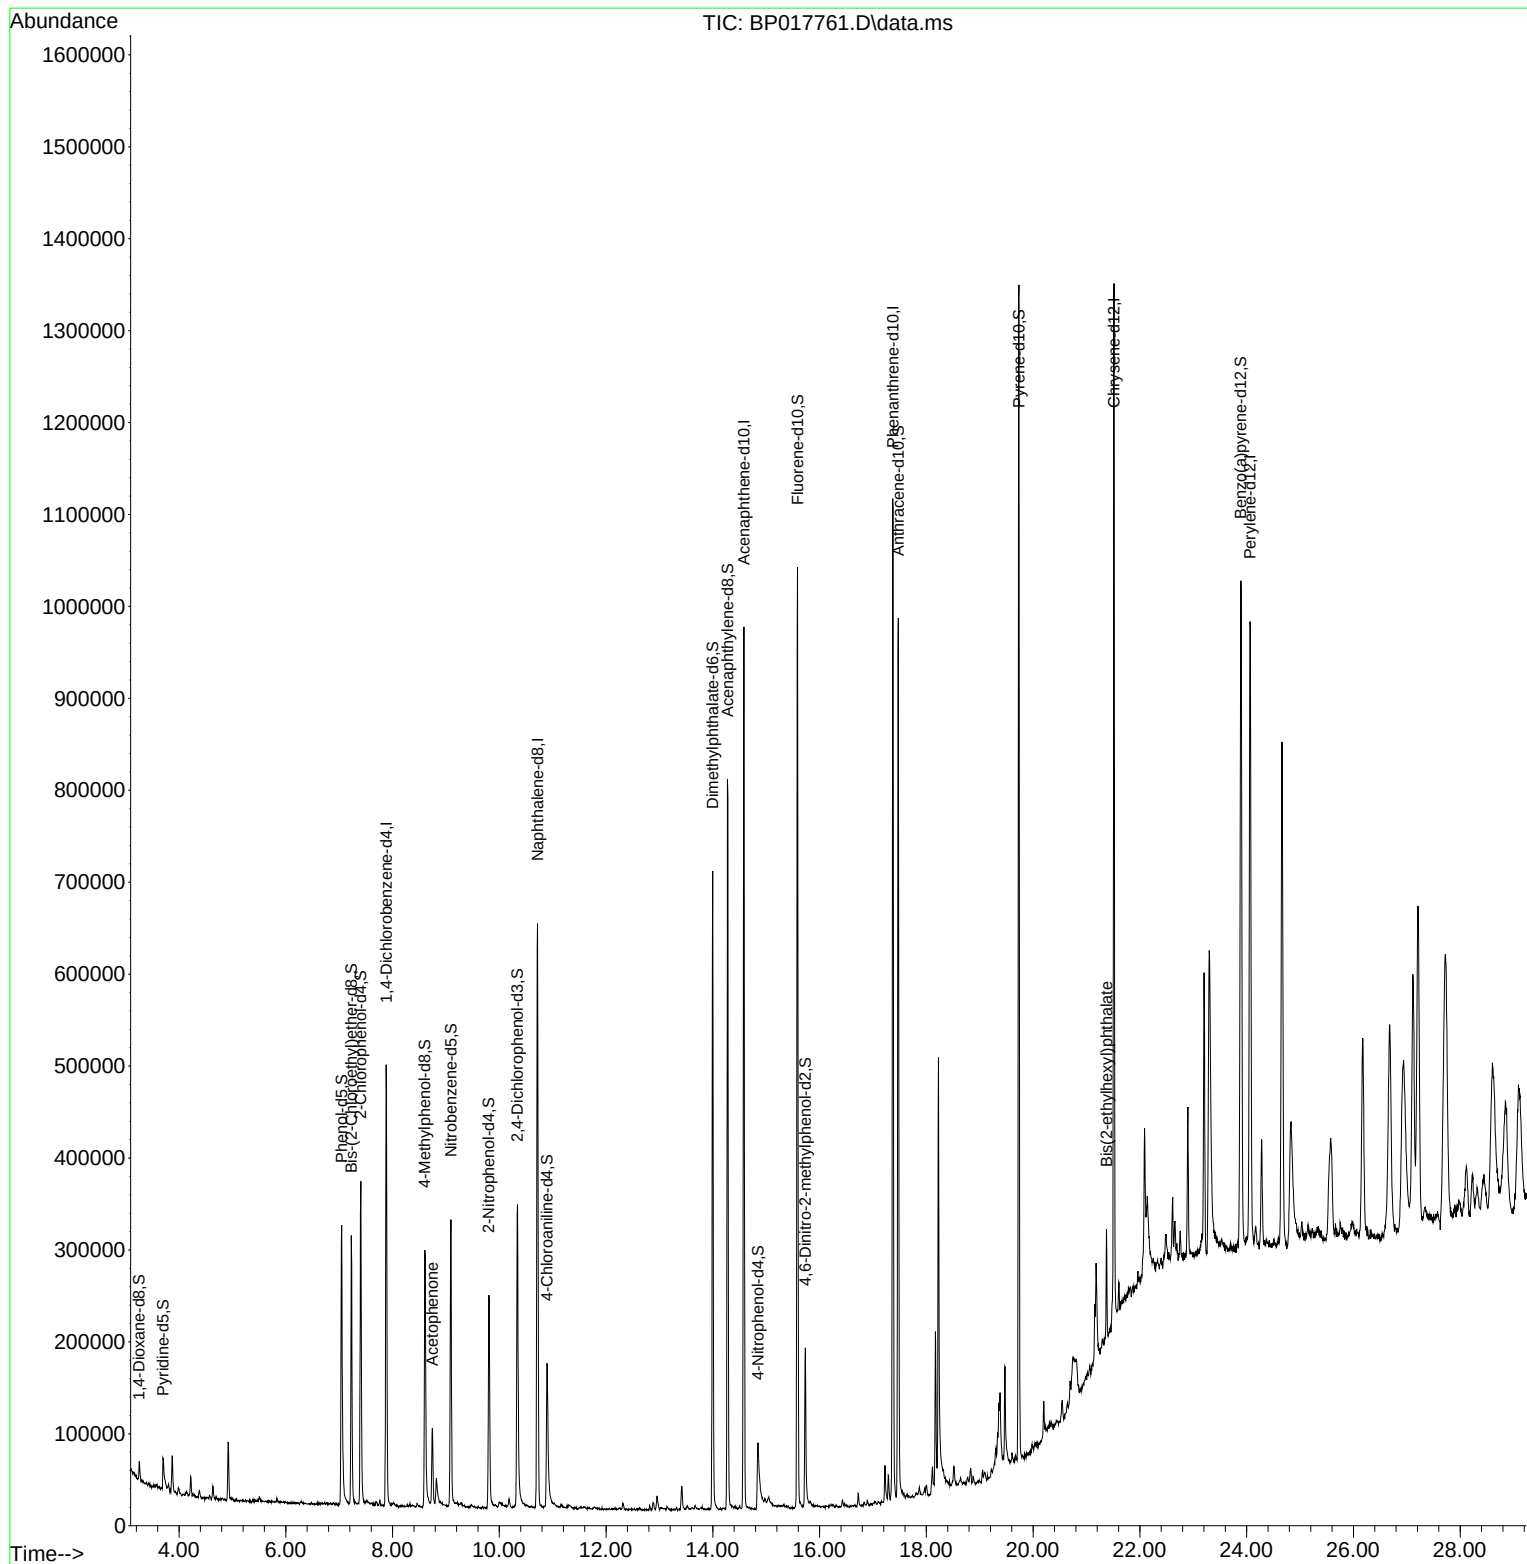


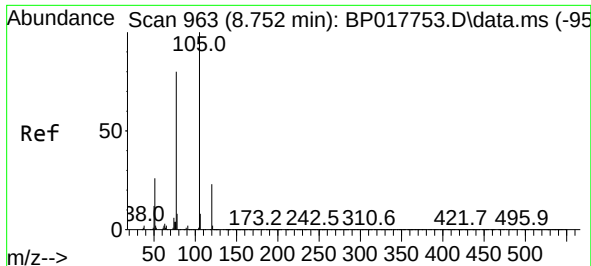

#16
Acetophenone
Concen: 3.440 ng/ul
RT: 8.746 min Scan# 90
Delta R.T. 0.000 min
Lab File: BP017761.D
Acq: 23 Oct 2023 21:43

Instrument :
BNA_P
ClientSampleId :
GCCZ8

Tgt Ion:105 Resp: 44297
Ion Ratio Lower Upper
105 100
77 80.7 64.4 96.6
51 28.3 21.2 31.8

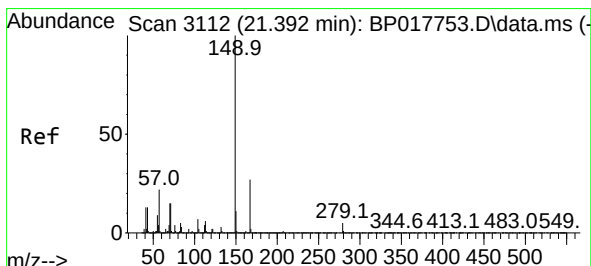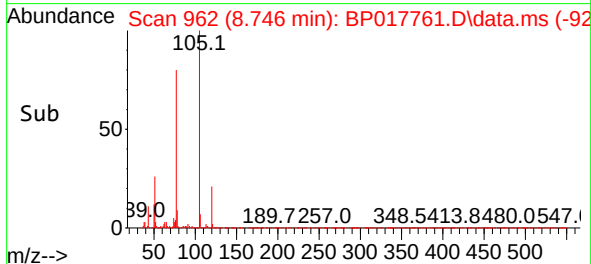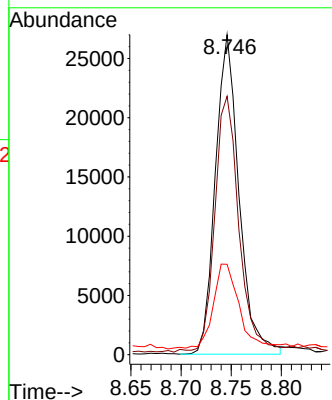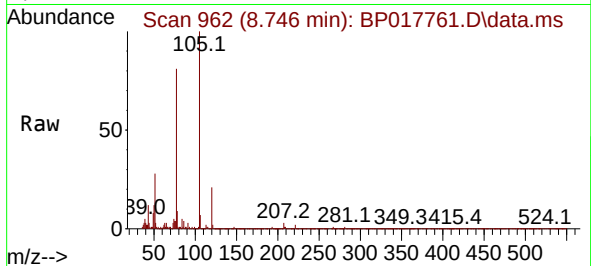

#86
Bis(2-ethylhexyl)phthalate
Concen: 2.101 ng/ul
RT: 21.375 min Scan# 3109
Delta R.T. -0.006 min
Lab File: BP017761.D
Acq: 23 Oct 2023 21:43

Tgt Ion:149 Resp: 38354
Ion Ratio Lower Upper
149 100
167 24.2 21.6 32.4
279 3.9 3.6 5.4

