

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017762.D
 Acq On : 23 Oct 2023 22:17
 Operator : MA/JU
 Sample : 04926-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCCY9

Quant Time: Oct 24 06:13:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	140152	20.000	ng/u1	0.00
20) Naphthalene-d8	10.716	136	514344	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	318074	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	684013	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.516	240	540403	20.000	ng/u1	0.00
88) Perylene-d12	24.063	264	561921	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	14743	3.913	ng/uL	0.00
4) Pyridine-d5	3.705	84	22153	2.246	ng/u1	0.01
7) Phenol-d5	7.040	99	270374	23.183	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	187400	26.018	ng/u1	0.00
11) 2-Chlorophenol-d4	7.405	132	228440	24.015	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	145561	15.893	ng/u1	0.00
21) Nitrobenzene-d5	9.093	128	106040	25.443	ng/u1	0.00
24) 2-Nitrophenol-d4	9.805	143	112182	24.361	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	200534	22.200	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	147096	12.443	ng/u1	0.00
46) Dimethylphthalate-d6	13.999	166	657001	24.606	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	744473	25.001	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	61308	16.114	ng/u1	0.00
60) Fluorene-d10	15.587	176	612751	26.547	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	70297	15.602	ng/u1	0.00
73) Anthracene-d10	17.475	188	901880	25.801	ng/u1	0.00
81) Pyrene-d10	19.734	212	1054838	31.134	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.898	264	862377	27.554	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.746	105	62194	4.319	ng/u1	98
86) Bis(2-ethylhexyl)phtha...	21.375	149	53915	2.723	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017762.D
Acq On : 23 Oct 2023 22:17
Operator : MA/JU
Sample : 04926-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCCY9

Quant Time: Oct 24 06:13:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration




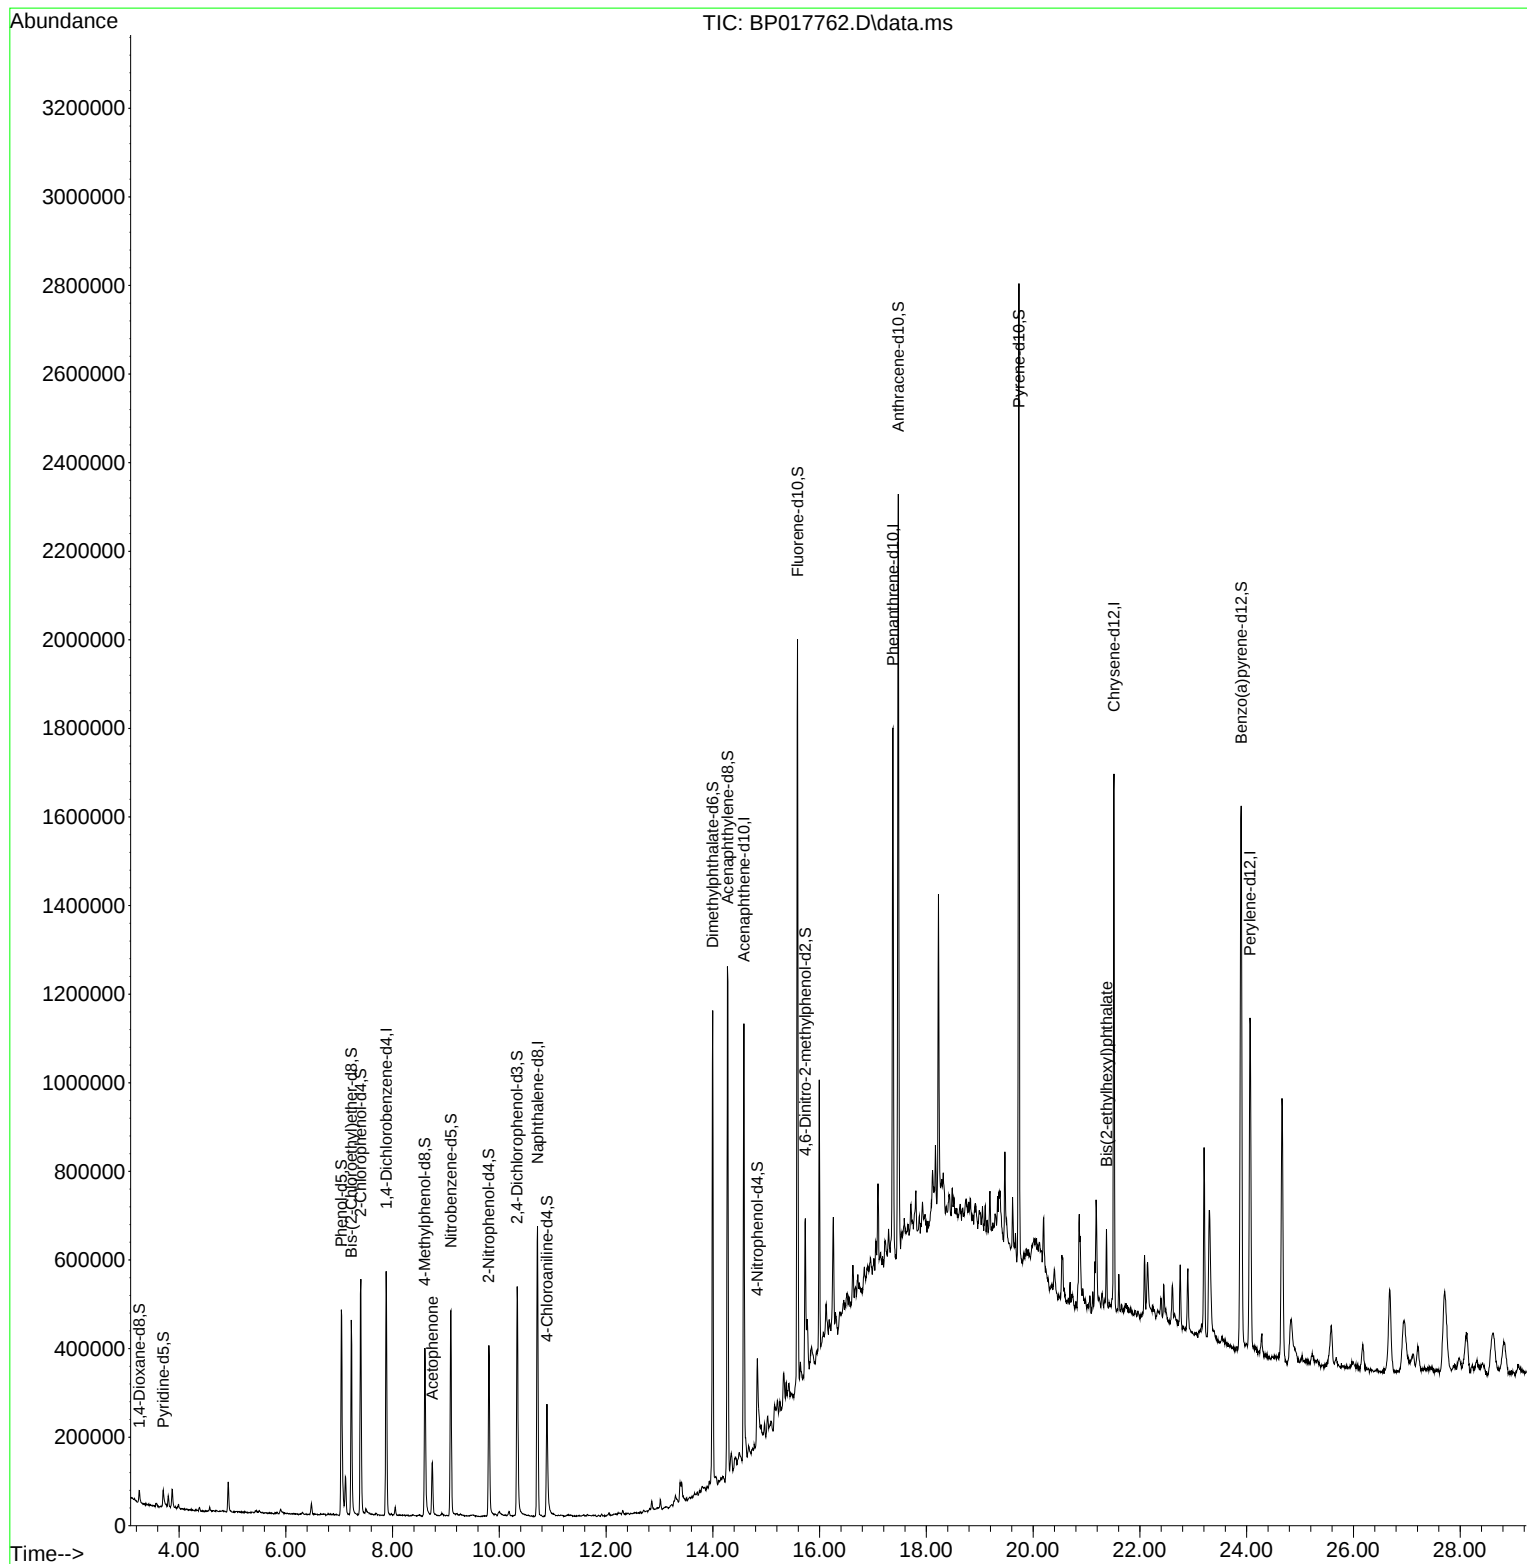


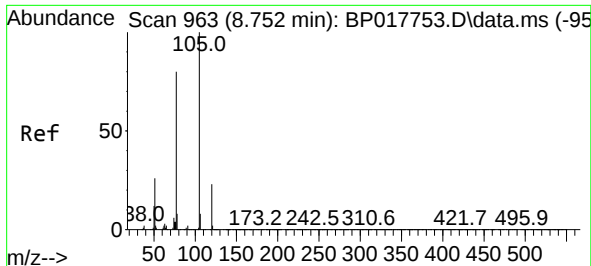

#16
Acetophenone
Concen: 4.319 ng/ul
RT: 8.746 min Scan# 90
Delta R.T. 0.000 min
Lab File: BP017762.D
Acq: 23 Oct 2023 22:17

Instrument :
BNA_P
ClientSampleId :
GCCY9

Tgt Ion:105 Resp: 62194
Ion Ratio Lower Upper
105 100
77 78.0 64.4 96.6
51 26.9 21.2 31.8

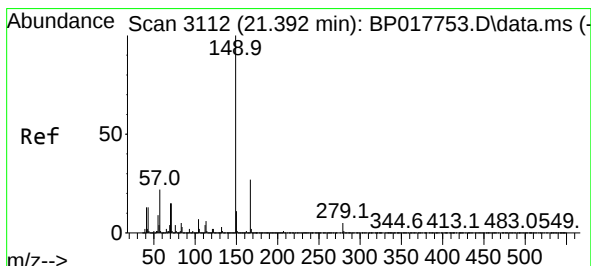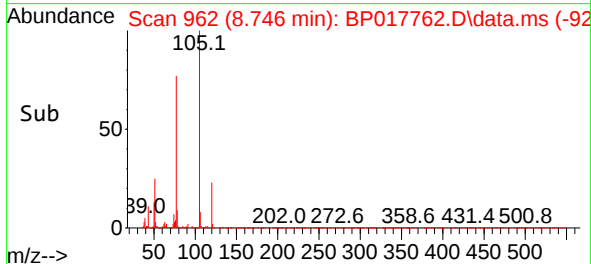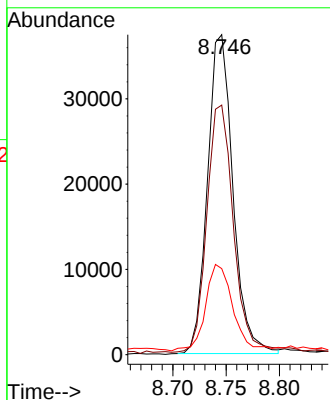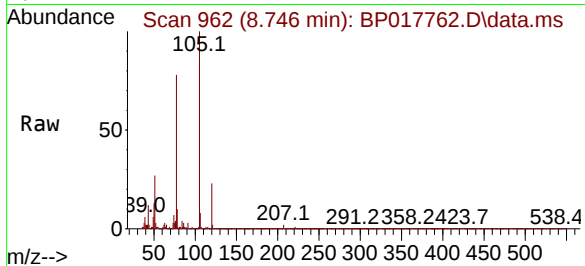

#86
Bis(2-ethylhexyl)phthalate
Concen: 2.723 ng/ul
RT: 21.375 min Scan# 3109
Delta R.T. -0.006 min
Lab File: BP017762.D
Acq: 23 Oct 2023 22:17

Tgt Ion:149 Resp: 53915
Ion Ratio Lower Upper
149 100
167 27.6 21.6 32.4
279 4.0 3.6 5.4

