

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017776.D
 Acq On : 24 Oct 2023 14:17
 Operator : MA/JU
 Sample : 04927-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD09

Quant Time: Oct 25 01:54:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	122060	20.000	ng/u1	0.00
20) Naphthalene-d8	10.722	136	480680	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.592	164	284596	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.381	188	594374	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.527	240	486442	20.000	ng/u1	0.01
88) Perylene-d12	24.086	264	506868	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	13872	4.228	ng/uL	0.00
4) Pyridine-d5	3.705	84	22149	2.578	ng/u1	0.01
7) Phenol-d5	7.052	99	227021	22.351	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	157077	25.041	ng/u1	0.00
11) 2-Chlorophenol-d4	7.410	132	190841	23.036	ng/u1	0.00
15) 4-Methylphenol-d8	8.616	113	134761	16.895	ng/u1	0.00
21) Nitrobenzene-d5	9.099	128	85757	22.017	ng/u1	0.00
24) 2-Nitrophenol-d4	9.816	143	94964	22.066	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	168816	19.997	ng/u1	0.00
31) 4-Chloroaniline-d4	10.904	131	127259	11.519	ng/u1	0.01
46) Dimethylphthalate-d6	14.010	166	538399	22.536	ng/u1	0.00
49) Acenaphthylene-d8	14.287	160	600833	22.551	ng/u1	0.00
54) 4-Nitrophenol-d4	14.851	143	39173	11.507	ng/u1	0.02
60) Fluorene-d10	15.598	176	463603	22.448	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	54283	13.865	ng/u1	0.01
73) Anthracene-d10	17.481	188	657510	21.647	ng/u1	0.00
81) Pyrene-d10	19.739	212	804574	26.382	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.915	264	646568	22.903	ng/u1	0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.752	105	41185	3.284	ng/u1	97
71) Pentachlorophenol	17.016	266	18216	3.795	ng/u1	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017776.D
Acq On : 24 Oct 2023 14:17
Operator : MA/JU
Sample : 04927-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD09

Quant Time: Oct 25 01:54:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration




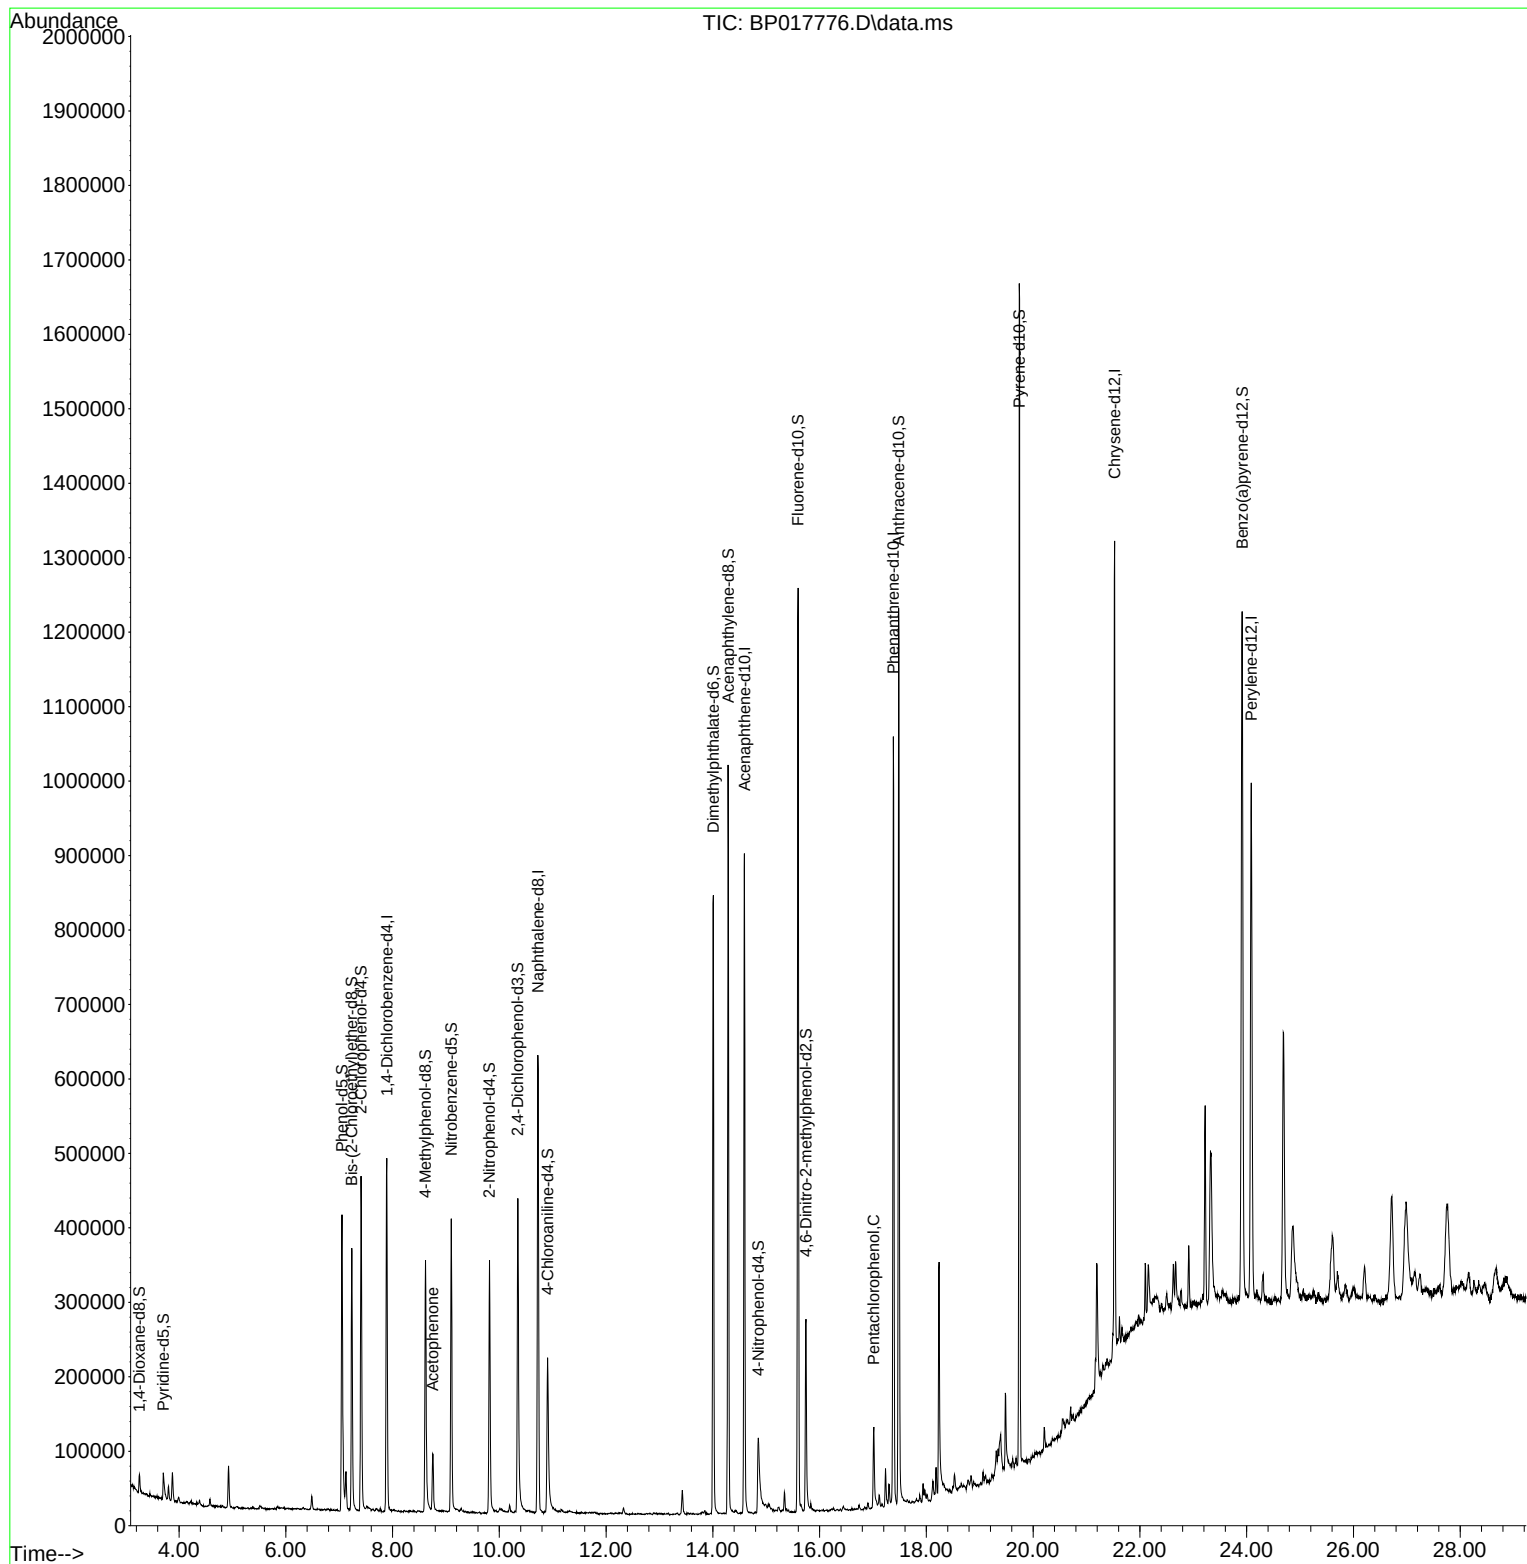


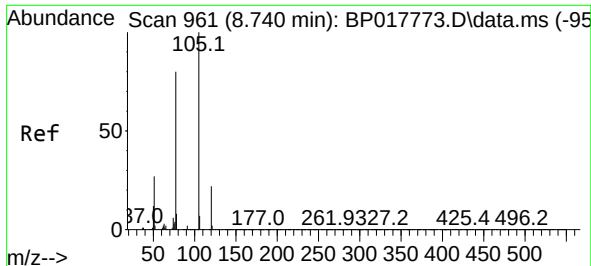

#16
Acetophenone
Concen: 3.284 ng/ul
RT: 8.752 min Scan# 961
Delta R.T. 0.006 min
Lab File: BP017776.D
Acq: 24 Oct 2023 14:17

Instrument :
BNA_P
ClientSampleId :
GCD09

Tgt Ion:105 Resp: 41185
Ion Ratio Lower Upper
105 100
77 82.4 64.4 96.6
51 29.2 21.2 31.8

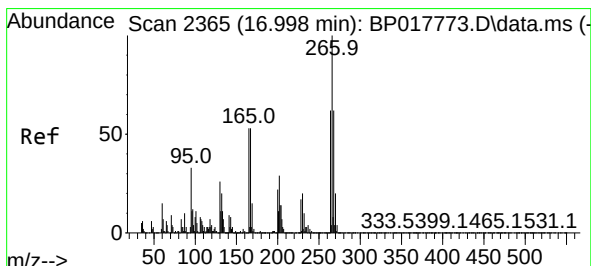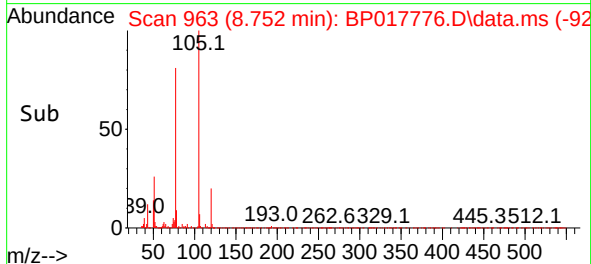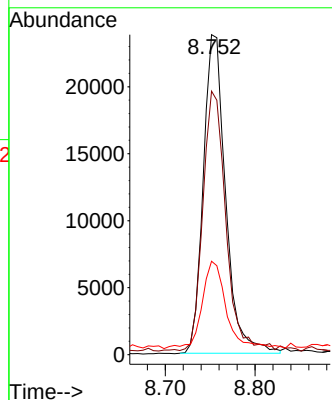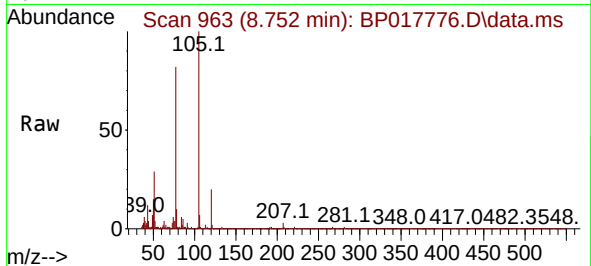

#71
Pentachlorophenol
Concen: 3.795 ng/ul
RT: 17.016 min Scan# 2368
Delta R.T. 0.012 min
Lab File: BP017776.D
Acq: 24 Oct 2023 14:17

Tgt Ion:266 Resp: 18216
Ion Ratio Lower Upper
266 100
264 69.6 49.4 74.2
268 71.4 50.3 75.5

