

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017786.D
 Acq On : 24 Oct 2023 19:59
 Operator : MA/JU
 Sample : 04926-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD02

Quant Time: Oct 25 01:58:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	123277	20.000	ng/u1	0.00
20) Naphthalene-d8	10.716	136	497334	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	300007	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.369	188	624001	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.516	240	521910	20.000	ng/u1	0.00
88) Perylene-d12	24.063	264	539622	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	11424	3.447	ng/uL	0.00
4) Pyridine-d5	3.705	84	20175	2.325	ng/u1	0.01
7) Phenol-d5	7.040	99	203412	19.829	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	139246	21.979	ng/u1	0.00
11) 2-Chlorophenol-d4	7.405	132	173785	20.770	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	147121	18.262	ng/u1	0.00
21) Nitrobenzene-d5	9.093	128	81259	20.164	ng/u1	0.00
24) 2-Nitrophenol-d4	9.805	143	88012	19.766	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	152146	17.419	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	106986	9.360	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	490218	19.465	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	542519	19.316	ng/u1	0.00
54) 4-Nitrophenol-d4	14.840	143	40085	11.170	ng/u1	0.01
60) Fluorene-d10	15.587	176	415214	19.073	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	48990	11.919	ng/u1	0.00
73) Anthracene-d10	17.475	188	538710	16.894	ng/u1	0.00
81) Pyrene-d10	19.727	212	710586	21.716	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.898	264	582188	19.371	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.746	105	46043	3.635	ng/u1	97
71) Pentachlorophenol	17.004	266	15150	3.006	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017786.D
Acq On : 24 Oct 2023 19:59
Operator : MA/JU
Sample : 04926-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD02

Quant Time: Oct 25 01:58:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration




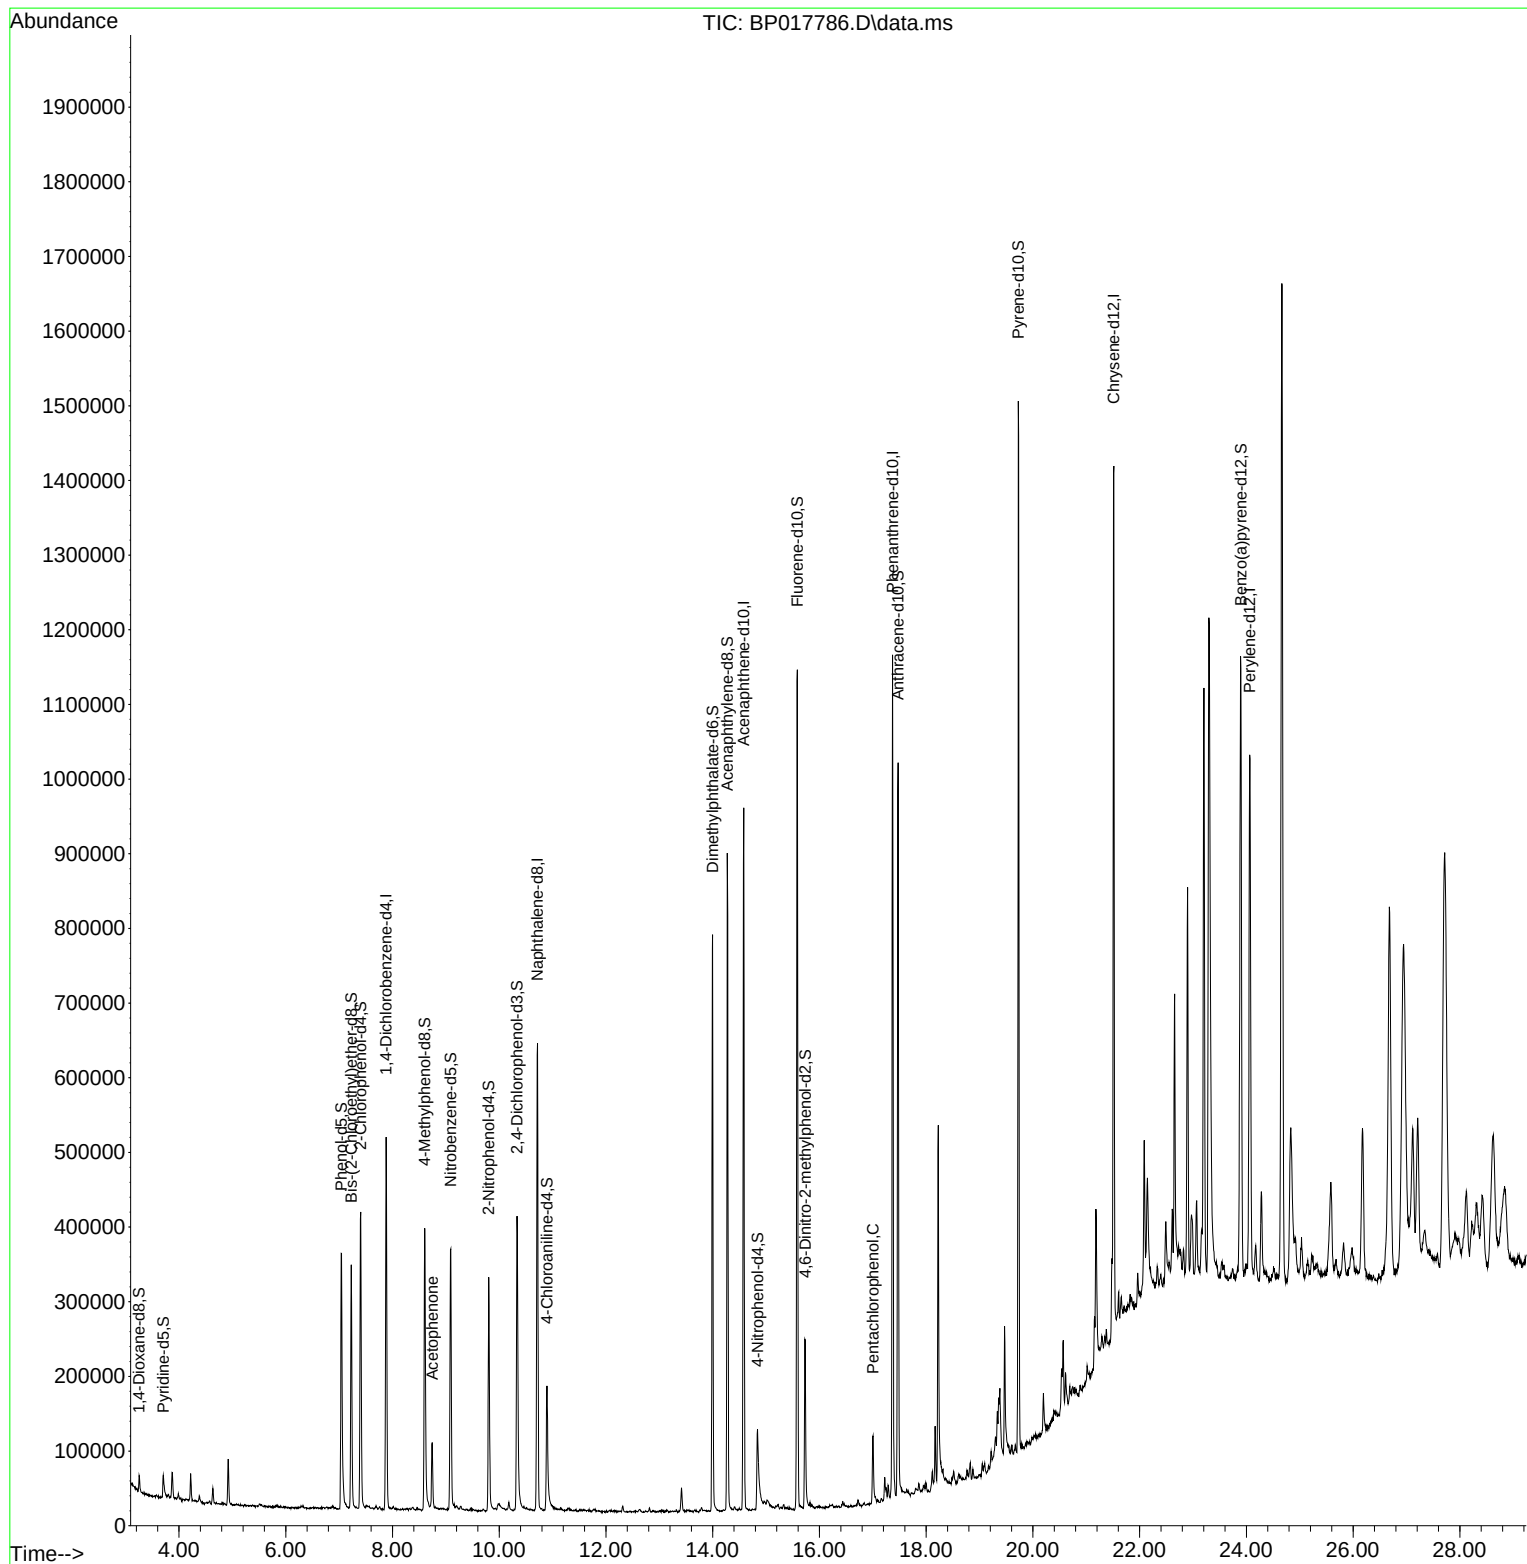


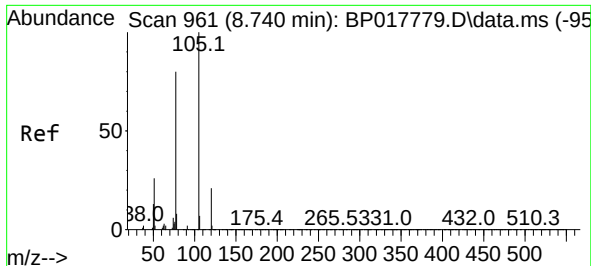

#16
Acetophenone
Concen: 3.635 ng/ul
RT: 8.746 min Scan# 961
Delta R.T. -0.000 min
Lab File: BP017786.D
Acq: 24 Oct 2023 19:59

Instrument :
BNA_P
ClientSampleId :
GCD02

Tgt Ion:	105	Resp:	46043
Ion	Ratio	Lower	Upper
105	100		
77	82.1	64.4	96.6
51	30.2	21.2	31.8

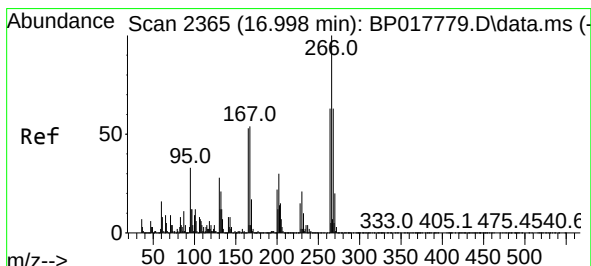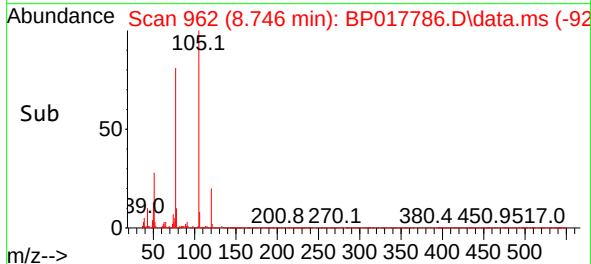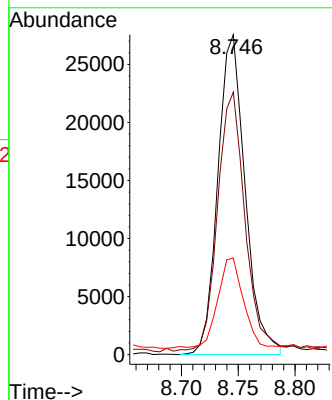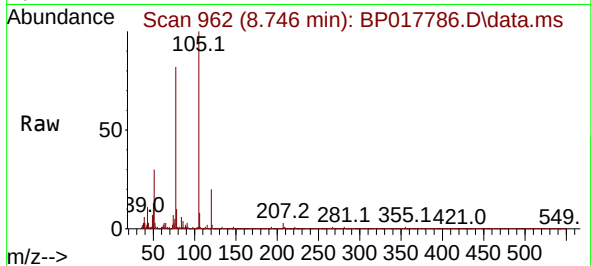

#71
Pentachlorophenol
Concen: 3.006 ng/ul
RT: 17.004 min Scan# 2366
Delta R.T. -0.000 min
Lab File: BP017786.D
Acq: 24 Oct 2023 19:59

Tgt Ion:	266	Resp:	15150
Ion	Ratio	Lower	Upper
266	100		
264	62.5	49.4	74.2
268	66.2	50.3	75.5

