

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017791.D
 Acq On : 24 Oct 2023 22:49
 Operator : MA/JU
 Sample : 04927-12
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD16

Quant Time: Oct 25 01:59:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	124620	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	509310	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.581	164	305563	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.369	188	647098	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.516	240	524773	20.000	ng/ul	0.00
88) Perylene-d12	24.063	264	554252	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	13772	4.111	ng/uL	0.00
4) Pyridine-d5	3.693	84	69826	7.961	ng/ul	0.00
7) Phenol-d5	7.040	99	240041	23.147	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	164964	25.758	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	209424	24.760	ng/ul	-0.01
15) 4-Methylphenol-d8	8.605	113	168392	20.678	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	98899	23.964	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.805	143	107337	23.539	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	188373	21.059	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	161607	13.805	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	608628	23.727	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	678545	23.720	ng/ul	0.00
54) 4-Nitrophenol-d4	14.840	143	55448	15.171	ng/ul	0.01
60) Fluorene-d10	15.587	176	512944	23.133	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.728	200	64443	15.119	ng/ul	0.00
73) Anthracene-d10	17.469	188	711489	21.516	ng/ul	0.00
81) Pyrene-d10	19.733	212	880500	26.762	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.898	264	727956	23.581	ng/ul	0.00
Target Compounds						
71) Pentachlorophenol	17.004	266	7996	1.530	ng/ul	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017791.D
 Acq On : 24 Oct 2023 22:49
 Operator : MA/JU
 Sample : 04927-12
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD16

Quant Time: Oct 25 01:59:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

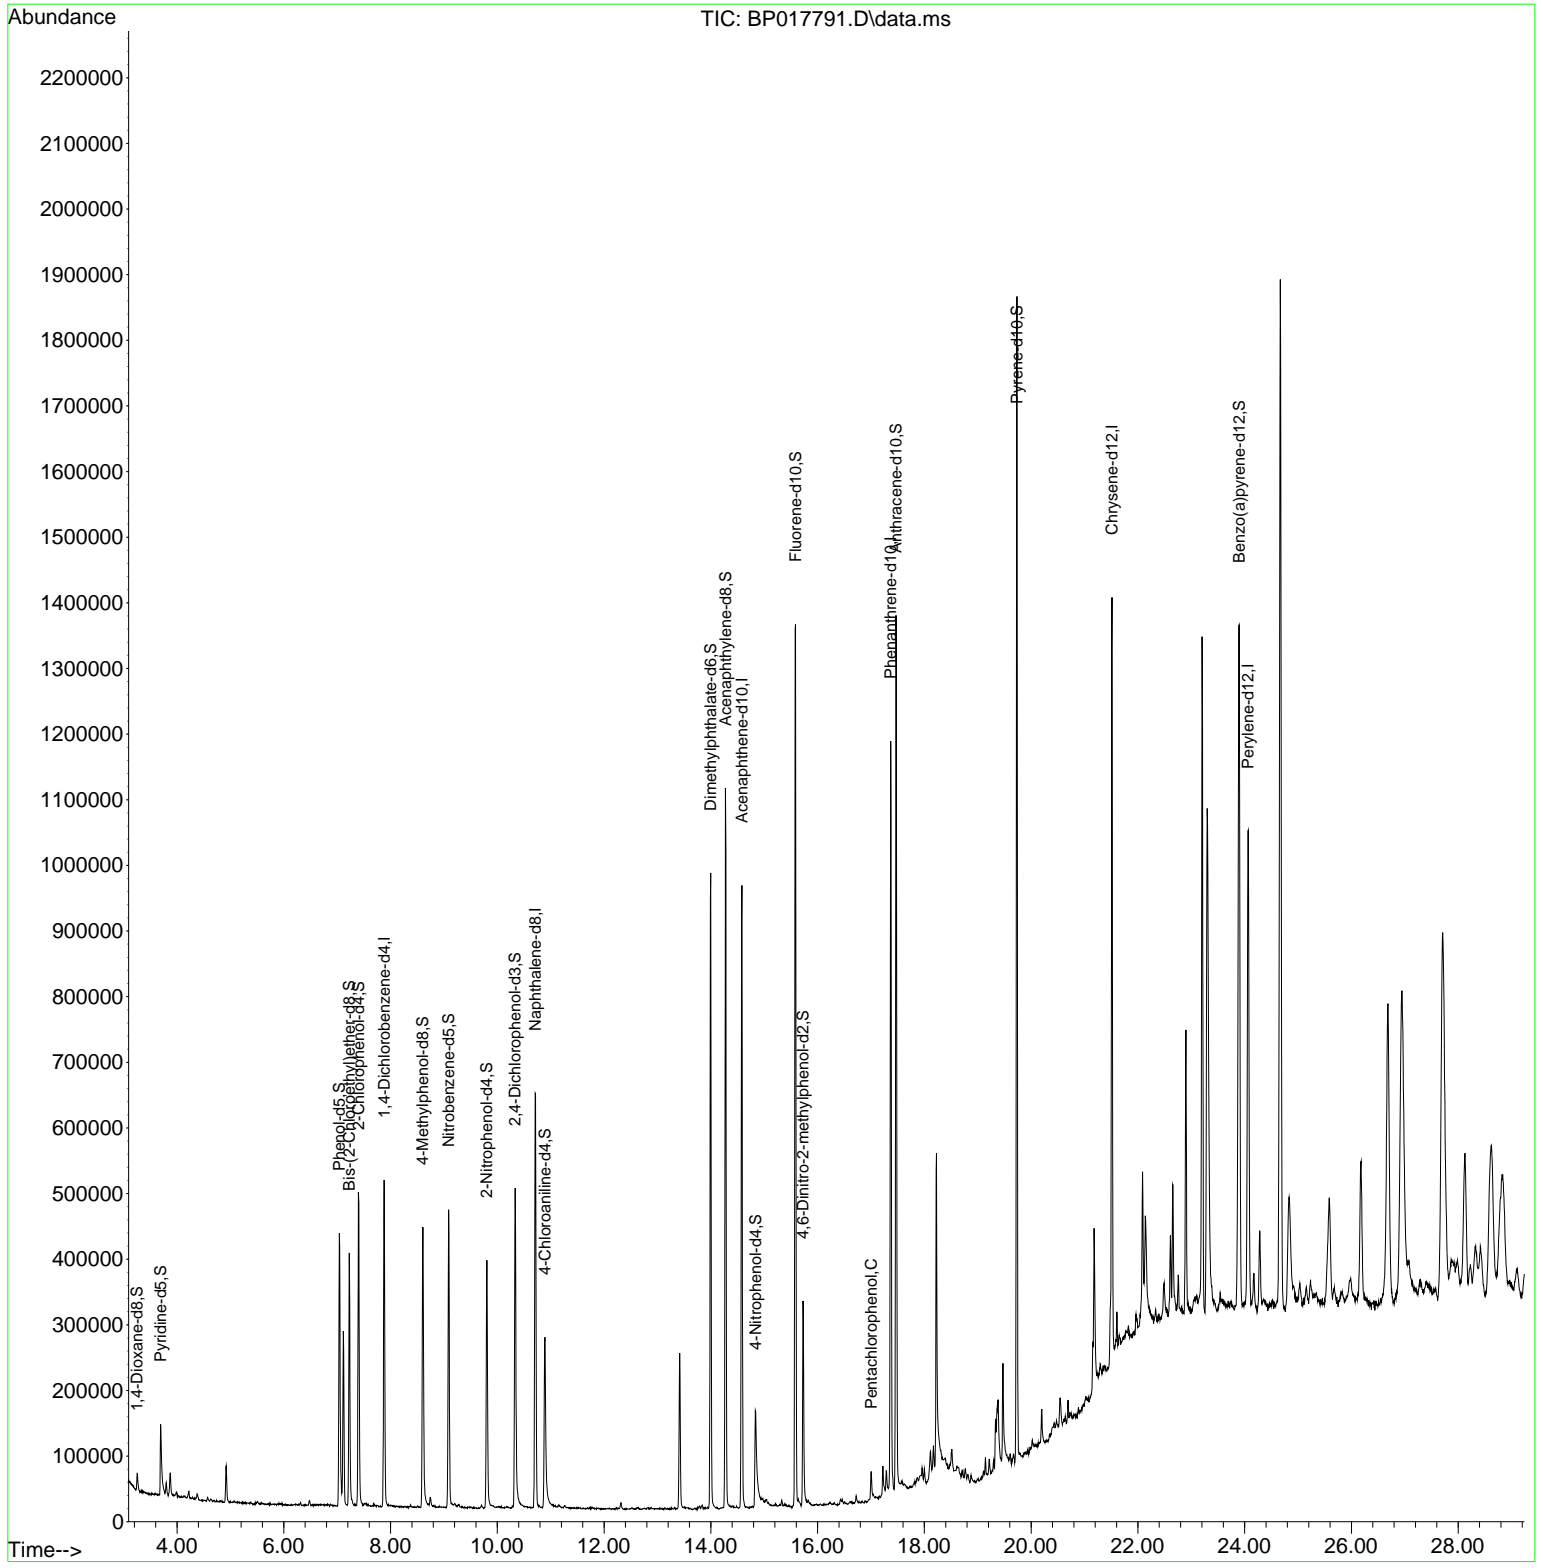

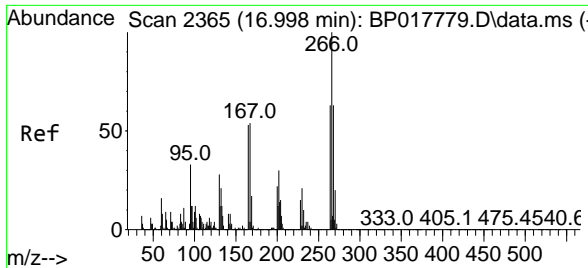

#71
 Pentachlorophenol
 Concen: 1.530 ng/ul
 RT: 17.004 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP017791.D
 Acq: 24 Oct 2023 22:49

Instrument :
 BNA_P
 ClientSampleId :
 GCD16

Tgt Ion	Resp	Lower	Upper
266	7996		
264	56.9	49.4	74.2
268	50.6	50.3	75.5

