

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017800.D
 Acq On : 25 Oct 2023 04:27
 Operator : MA/JU
 Sample : 04927-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD17

Quant Time: Oct 25 05:26:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	113017	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	460022	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.575	164	274363	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.369	188	578304	20.000	ng/u1	0.00
79) Chrysene-d12	21.510	240	478350	20.000	ng/u1	0.00
88) Perylene-d12	24.063	264	502453	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	14200	4.674	ng/uL	0.00
4) Pyridine-d5	3.693	84	115981	14.582	ng/u1	0.00
7) Phenol-d5	7.040	99	250231	26.607	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	164852	28.383	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.399	132	206722	26.950	ng/u1	-0.01
15) 4-Methylphenol-d8	8.604	113	160356	21.712	ng/u1	0.00
21) Nitrobenzene-d5	9.087	128	100329	26.915	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.804	143	115608	28.070	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	198533	24.573	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	166049	15.705	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	636653	27.642	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	717383	27.930	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	69837	21.280	ng/u1	0.00
60) Fluorene-d10	15.581	176	535495	26.897	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.728	200	74137	19.462	ng/u1	0.00
73) Anthracene-d10	17.469	188	749777	25.371	ng/u1	0.00
81) Pyrene-d10	19.727	212	920083	30.679	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.898	264	766537	27.391	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	16.998	266	31593	6.765	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017800.D
Acq On : 25 Oct 2023 04:27
Operator : MA/JU
Sample : 04927-13
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD17

Quant Time: Oct 25 05:26:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

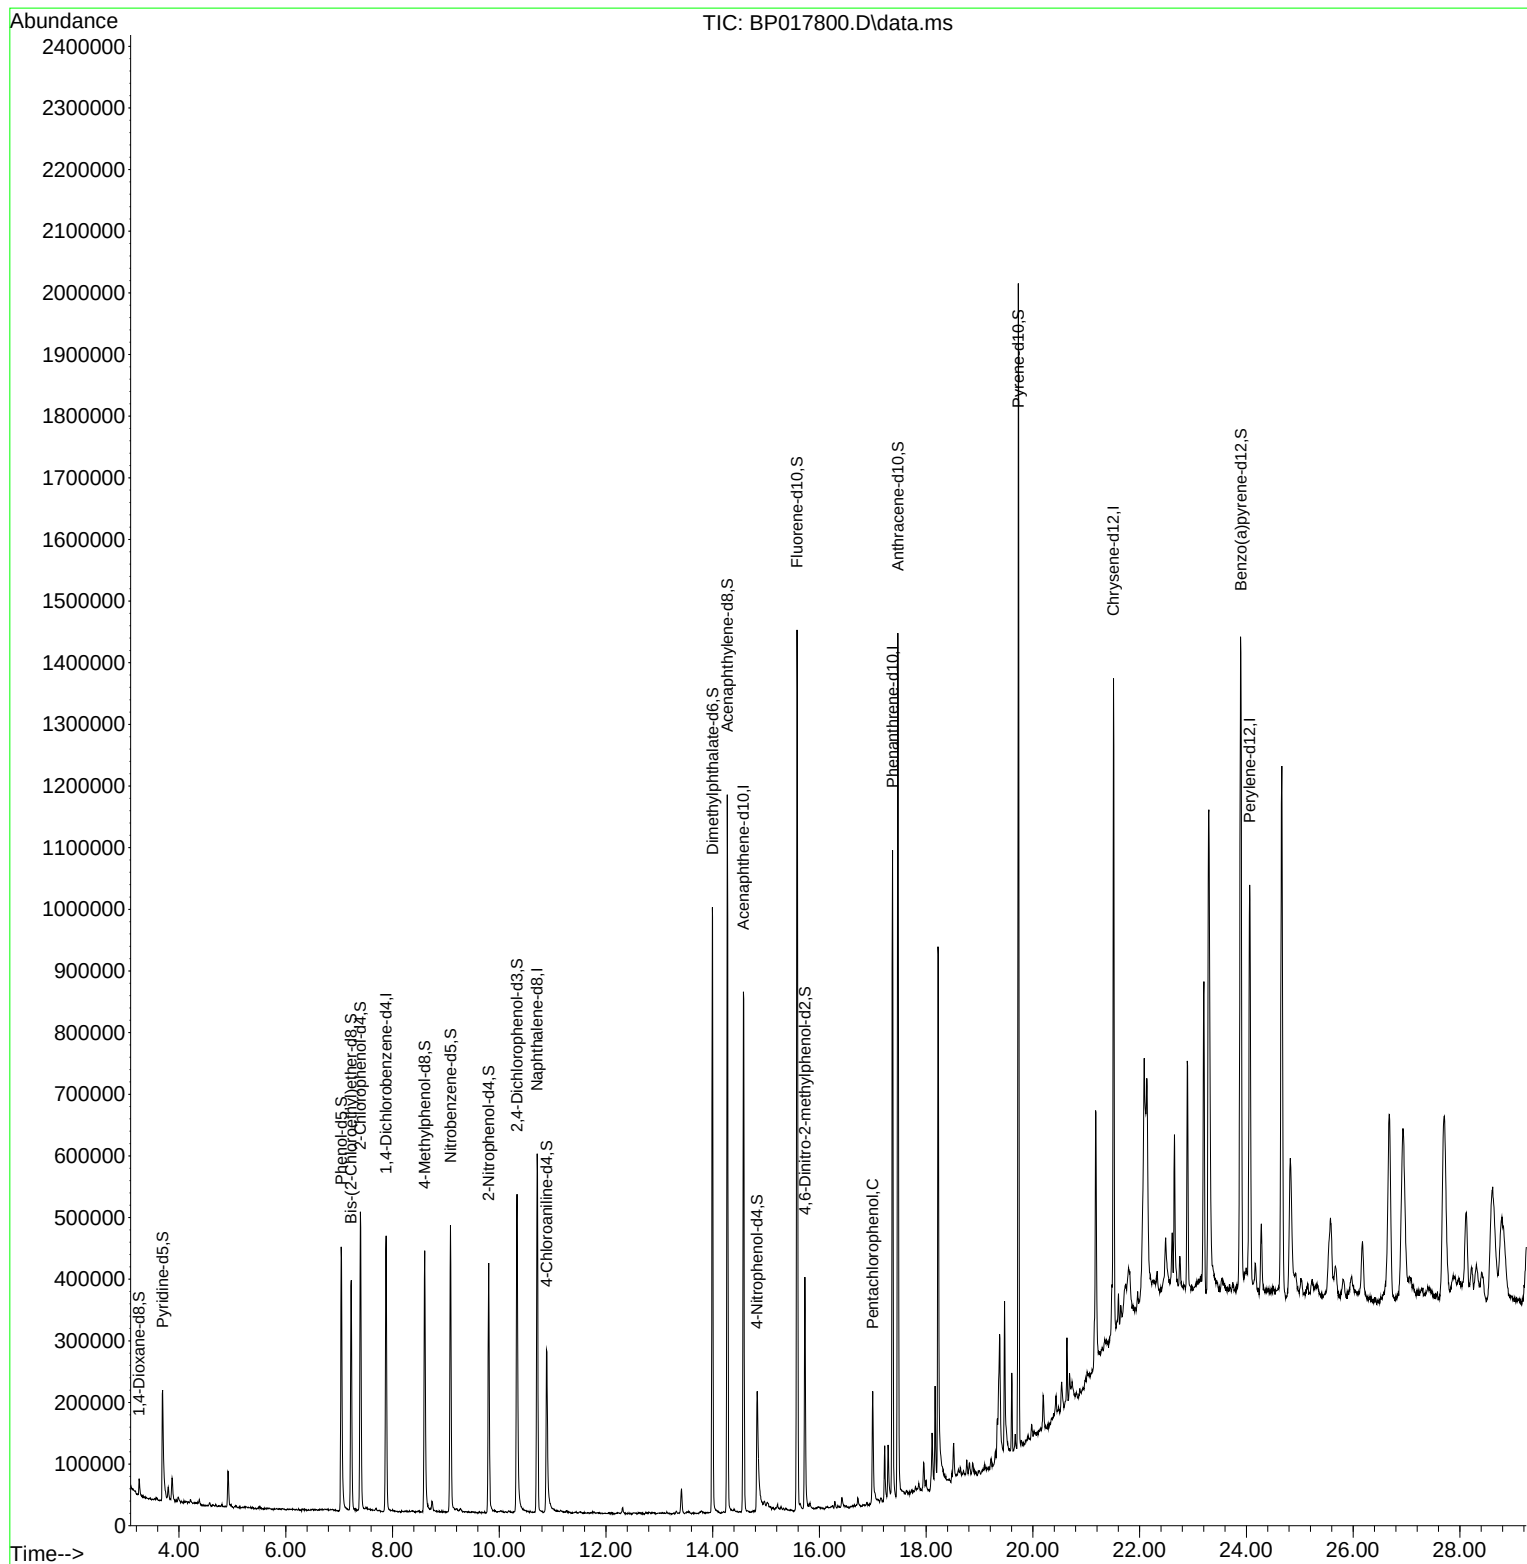

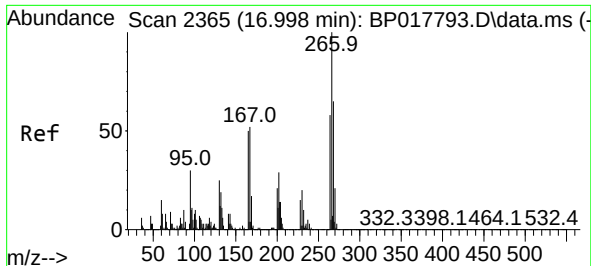

#71
 Pentachlorophenol
 Concen: 6.765 ng/ul
 RT: 16.998 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP017800.D
 Acq: 25 Oct 2023 04:27

Instrument :
 BNA_P
 ClientSampleId :
 GCD17

Tgt Ion:266 Resp: 31593
 Ion Ratio Lower Upper
 266 100
 264 58.4 49.4 74.2
 268 60.0 50.3 75.5

