

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017803.D
 Acq On : 25 Oct 2023 06:09
 Operator : MA/JU
 Sample : 04927-06
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD10

Quant Time: Oct 25 06:38:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	122657	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	495686	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.575	164	302439	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.369	188	637583	20.000	ng/u1	0.00
79) Chrysene-d12	21.516	240	517751	20.000	ng/u1	0.00
88) Perylene-d12	24.068	264	552507	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	18633	5.651	ng/uL	0.00
4) Pyridine-d5	3.687	84	161768	18.740	ng/u1	0.00
7) Phenol-d5	7.040	99	316667	31.025	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	215281	34.152	ng/u1	0.00
11) 2-Chlorophenol-d4	7.399	132	272868	32.777	ng/u1	-0.01
15) 4-Methylphenol-d8	8.605	113	217068	27.081	ng/u1	0.00
21) Nitrobenzene-d5	9.087	128	133351	33.200	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.804	143	154107	34.725	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	251812	28.925	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	245887	21.583	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	792026	31.196	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	904170	31.934	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	73335	20.272	ng/u1	0.00
60) Fluorene-d10	15.581	176	673225	30.675	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.728	200	92189	21.951	ng/u1	0.00
73) Anthracene-d10	17.469	188	987032	30.294	ng/u1	0.00
81) Pyrene-d10	19.727	212	1162802	35.822	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.898	264	987568	32.092	ng/u1	0.00


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.380	149	3161013	166.624 ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017803.D
Acq On : 25 Oct 2023 06:09
Operator : MA/JU
Sample : 04927-06
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD10

Quant Time: Oct 25 06:38:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

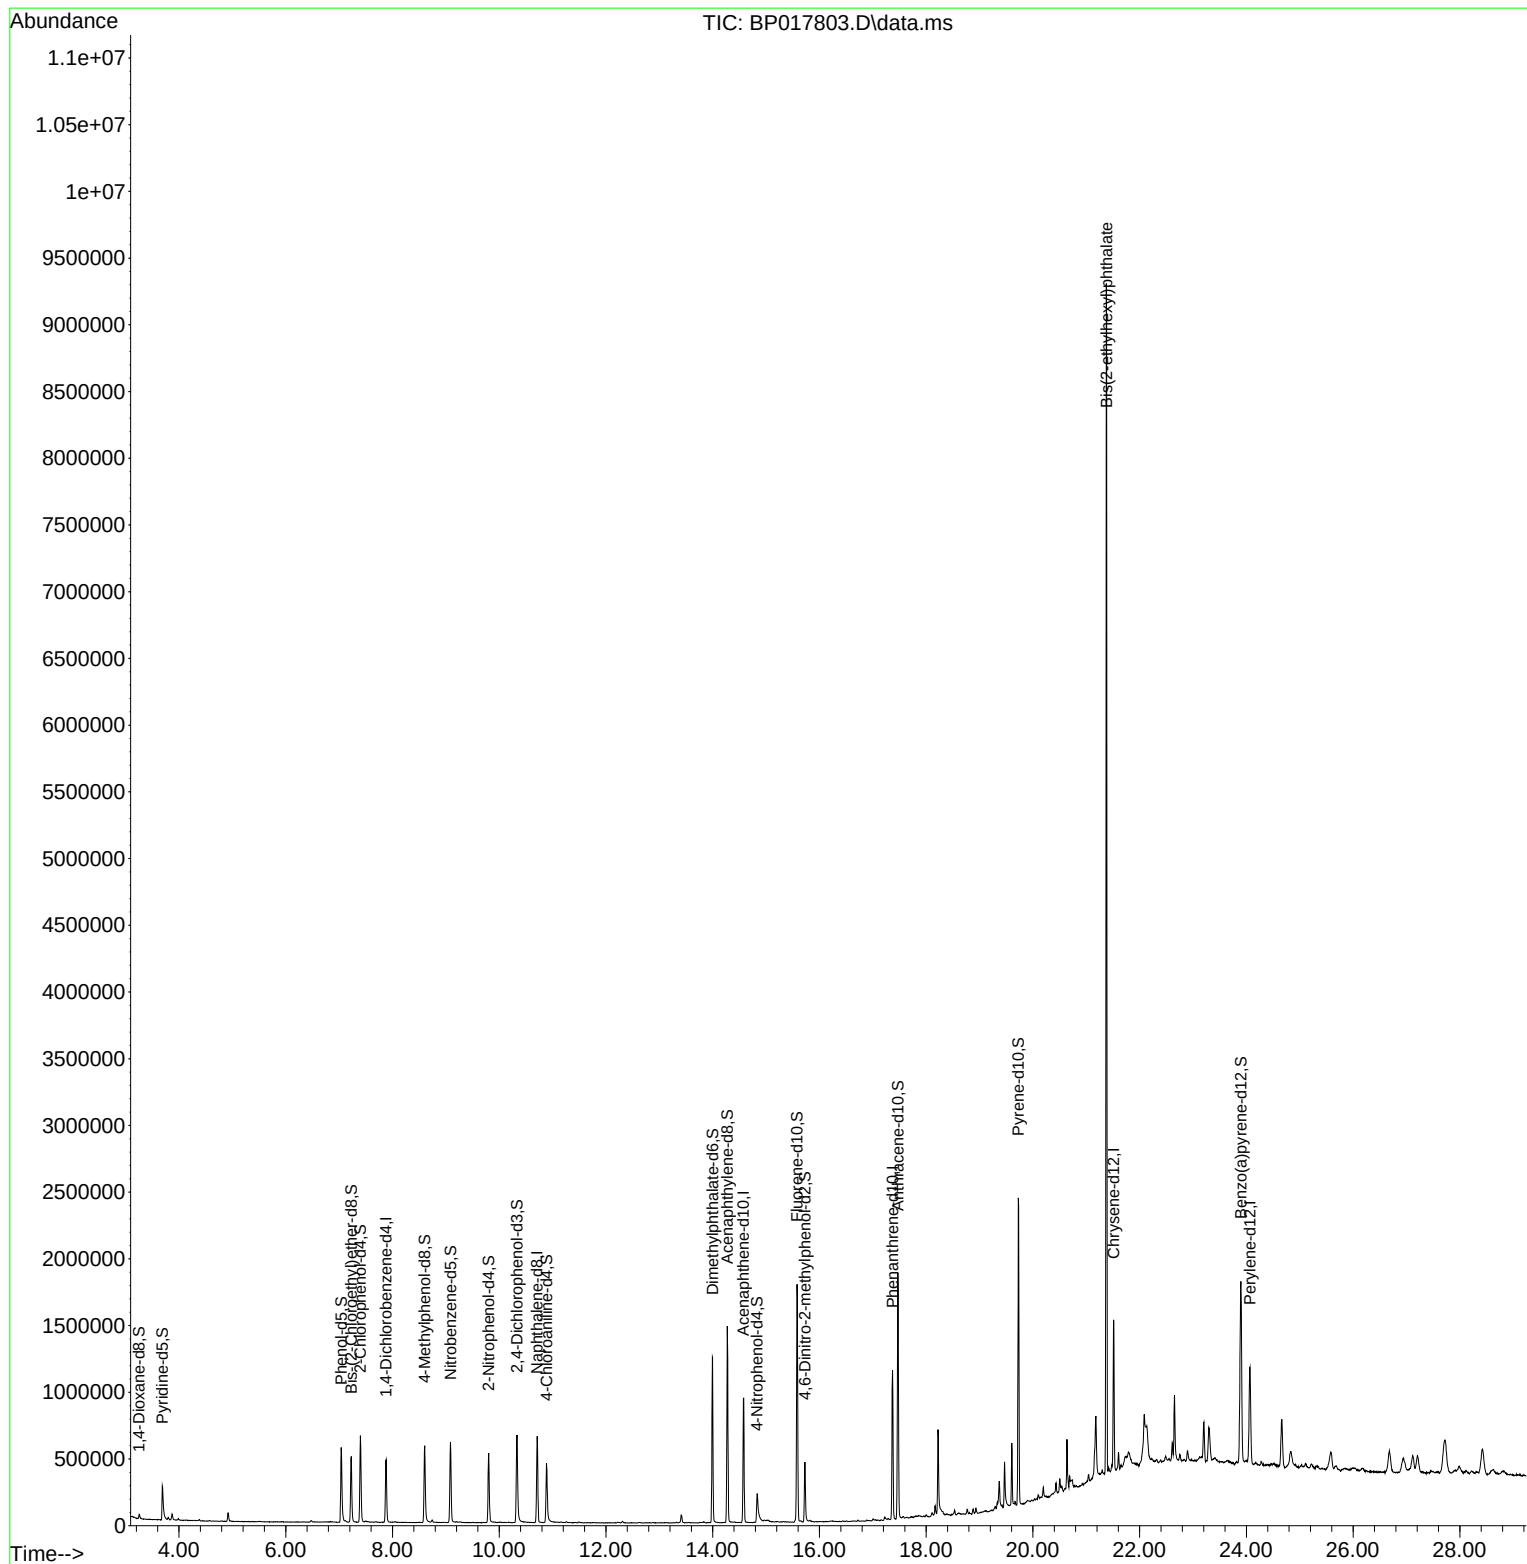

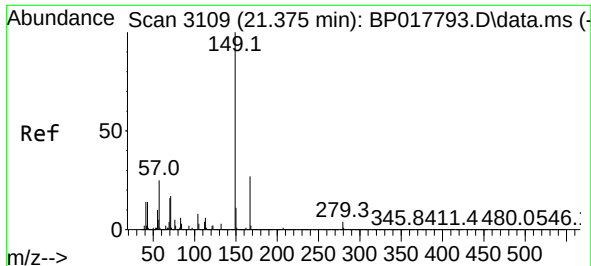

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 166.624 ng/ul
 RT: 21.380 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BP017803.D
 Acq: 25 Oct 2023 06:09

Instrument :
 BNA_P
 ClientSampleId :
 GCD10

Tgt Ion:149 Resp: 3161013

Ion	Ratio	Lower	Upper
149	100		
167	27.3	21.6	32.4
279	4.7	3.6	5.4

