

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017805.D
 Acq On : 25 Oct 2023 07:16
 Operator : MA/JU
 Sample : 04927-14
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD18

Quant Time: Oct 25 07:45:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	132215	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	525953	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.581	164	320027	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.369	188	659412	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	541515	20.000	ng/ul	0.00
88) Perylene-d12	24.069	264	566398	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	16660	4.688	ng/uL	0.00
4) Pyridine-d5	3.687	84	155717	16.735	ng/ul	0.00
7) Phenol-d5	7.040	99	297193	27.012	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	199919	29.423	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.399	132	250754	27.943	ng/ul	-0.01
15) 4-Methylphenol-d8	8.605	113	172295	19.941	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	123349	28.943	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.805	143	137430	29.185	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	237855	25.750	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	163483	13.524	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	730104	27.176	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	823813	27.497	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	78581	20.528	ng/ul	0.00
60) Fluorene-d10	15.581	176	615722	26.513	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.728	200	84520	19.459	ng/ul	0.00
73) Anthracene-d10	17.469	188	835178	24.785	ng/ul	0.00
81) Pyrene-d10	19.728	212	1042469	30.706	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.898	264	859249	27.237	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.998	266	21052	3.953	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017805.D
Acq On : 25 Oct 2023 07:16
Operator : MA/JU
Sample : 04927-14
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD18

Quant Time: Oct 25 07:45:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

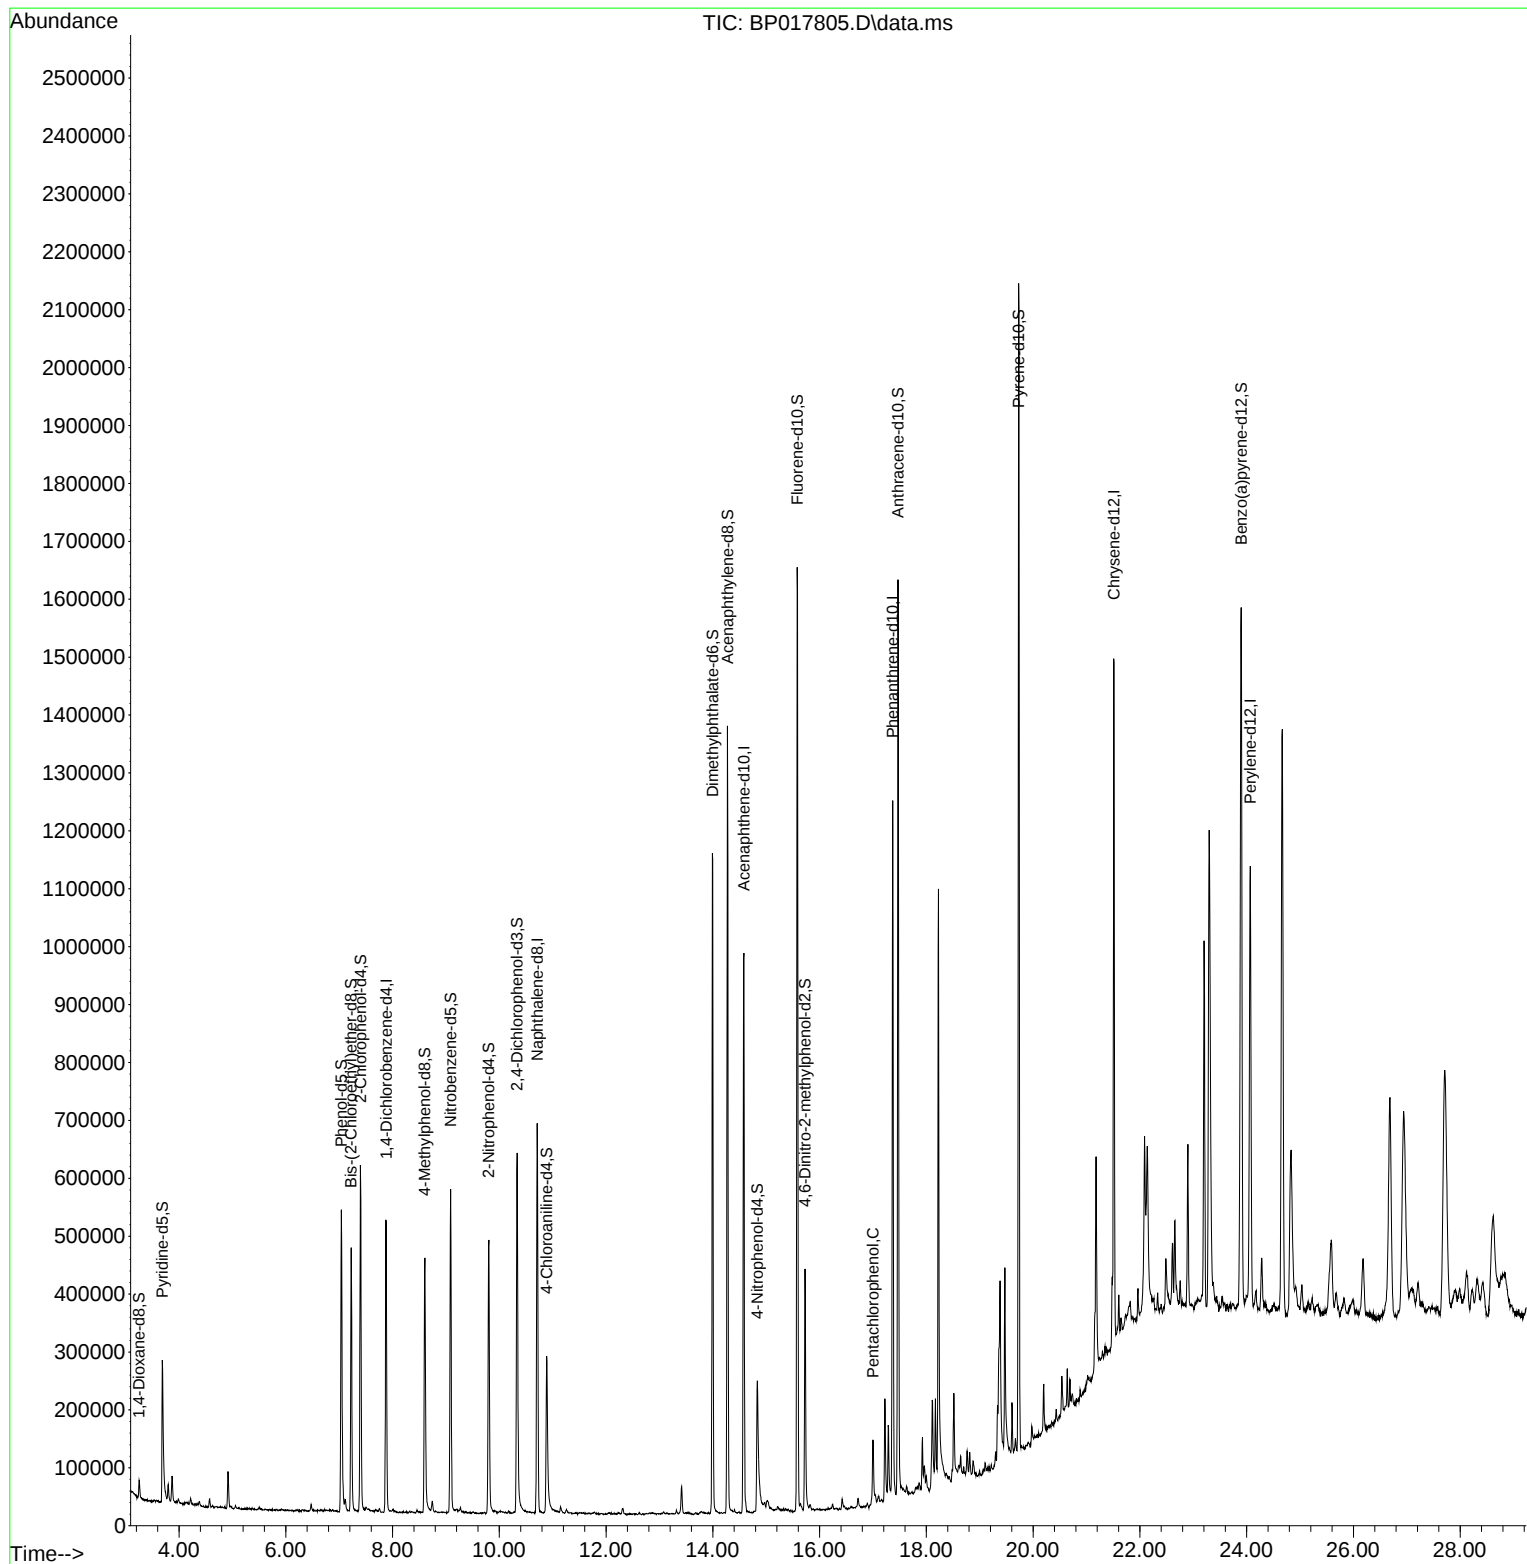

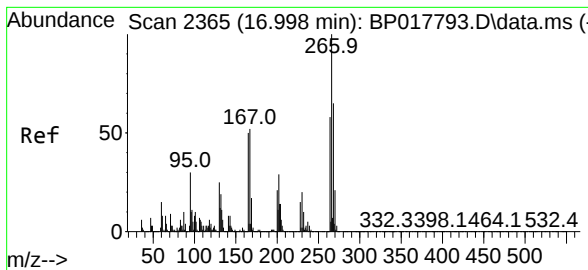

#71
 Pentachlorophenol
 Concen: 3.953 ng/ul
 RT: 16.998 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP017805.D
 Acq: 25 Oct 2023 07:16

Instrument :
 BNA_P
 ClientSampleId :
 GCD18

Tgt Ion:	266	Resp:	21052
Ion Ratio	Lower	Upper	
266	100		
264	62.1	49.4	74.2
268	58.3	50.3	75.5

