

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017772.D
 Acq On : 24 Oct 2023 03:55
 Operator : MA/JU
 Sample : PB156465BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK465

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017772.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	35	rVB	46548	66212	1.93%	0.170%
2	3.687	98	102	117	rBV	478145	816712	23.76%	2.101%
3	3.987	150	153	159	rBV	16414	23001	0.67%	0.059%
4	7.040	665	672	689	rBV	685213	1155177	33.60%	2.971%
5	7.228	698	704	715	rVB	605939	916412	26.66%	2.357%
6	7.405	726	734	746	rBV	735335	1223077	35.58%	3.146%
7	7.881	808	815	827	rBV	641153	1003330	29.19%	2.581%
8	8.604	931	938	960	rBV	805261	1403761	40.84%	3.611%
9	9.087	1013	1020	1034	rBV	677333	1127347	32.79%	2.900%
10	9.804	1134	1142	1157	rBV	577939	971327	28.26%	2.498%
11	10.334	1224	1232	1251	rBV	759936	1433776	41.71%	3.688%
12	10.716	1288	1297	1304	rBV	835021	1393448	40.54%	3.584%
13	10.769	1304	1306	1310	rVB5	3058	3594	0.10%	0.009%
14	10.887	1319	1326	1344	rBV	682323	1270515	36.96%	3.268%
15	12.316	1559	1569	1576	rBV2	13158	27130	0.79%	0.070%
16	13.416	1749	1756	1761	rBV2	18436	31694	0.92%	0.082%
17	13.540	1773	1777	1780	rVB6	2481	3711	0.11%	0.010%
18	13.998	1848	1855	1868	rBV	1382982	1932586	56.22%	4.971%
19	14.275	1895	1902	1916	rBV	1580087	2310922	67.22%	5.944%
20	14.392	1921	1922	1929	rVB7	2313	4737	0.14%	0.012%
21	14.581	1947	1954	1962	rBV	1178099	1699807	49.45%	4.372%
22	14.828	1990	1996	2015	rBV	262398	686938	19.98%	1.767%
23	15.586	2117	2125	2137	rBV	1941527	2826061	82.21%	7.269%
24	15.728	2143	2149	2162	rBV	485341	741062	21.56%	1.906%
25	15.828	2162	2166	2170	rVB4	11612	18275	0.53%	0.047%
26	16.381	2256	2260	2264	rBV7	2931	5183	0.15%	0.013%
27	17.157	2390	2392	2396	rVB4	3707	4653	0.14%	0.012%
28	17.369	2421	2428	2439	rBV	1502788	2080239	60.51%	5.350%
29	17.469	2439	2445	2461	rVV2	2155223	3106271	90.36%	7.989%
30	18.239	2570	2576	2579	rBV6	5578	12271	0.36%	0.032%
31	19.298	2751	2756	2762	rBV4	28766	44637	1.30%	0.115%
32	19.369	2764	2768	2772	rVB	25225	34085	0.99%	0.088%
33	19.610	2806	2809	2812	rBV4	10029	12985	0.38%	0.033%
34	19.727	2824	2829	2839	rBV	2670008	3437631	100.00%	8.842%
35	21.510	3127	3132	3141	rBV	1465334	1960887	57.04%	5.043%
36	23.892	3530	3537	3549	rVB2	1541379	3199610	93.08%	8.229%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017772.D
Acq On : 24 Oct 2023 03:55
Operator : MA/JU
Sample : PB156465BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK465

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	24.063	3559	3566	3577	rVB	882675	1890894	55.01%	4.863%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 38879958

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017772.D
Acq On : 24 Oct 2023 03:55
Operator : MA/JU
Sample : PB156465BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK465

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

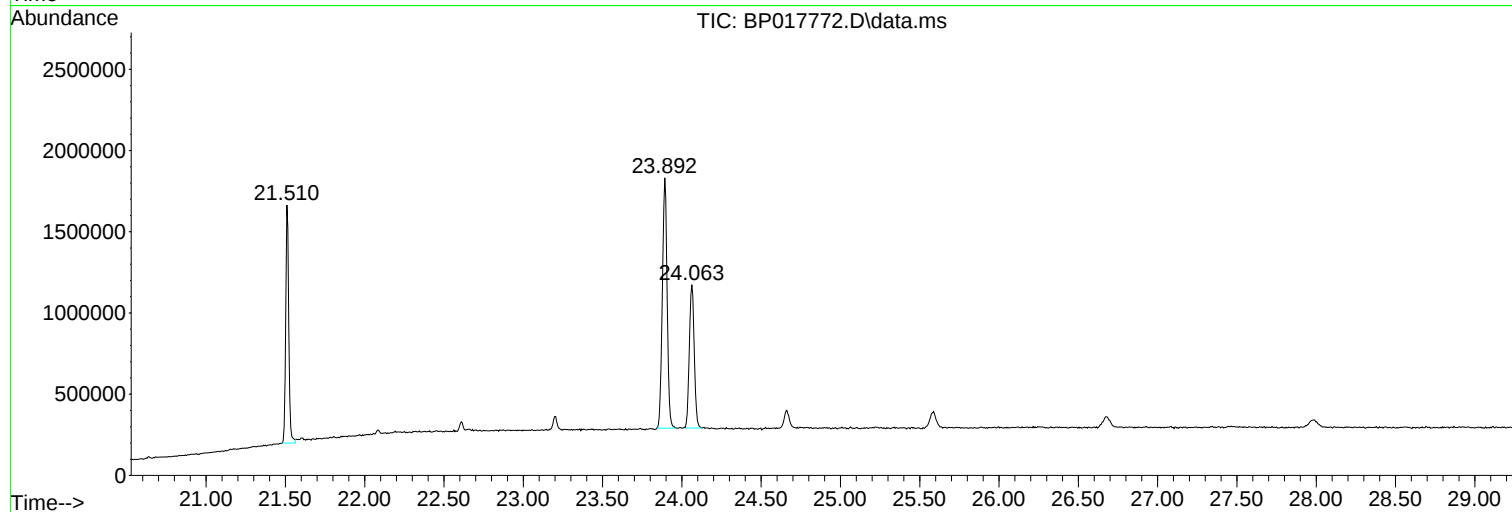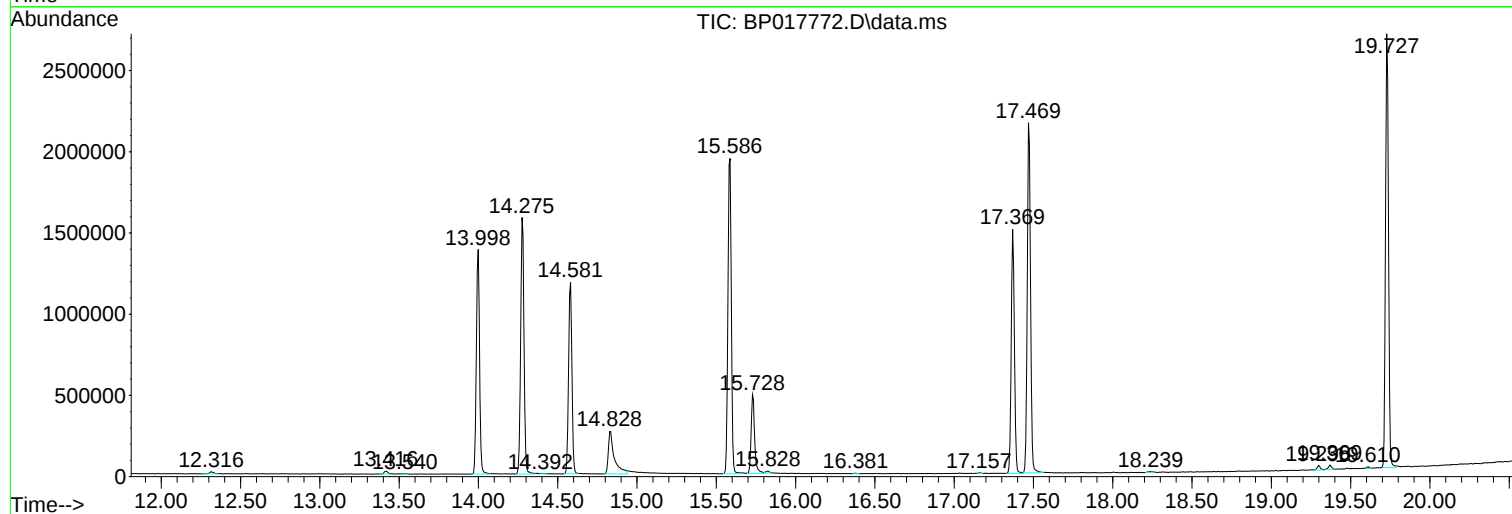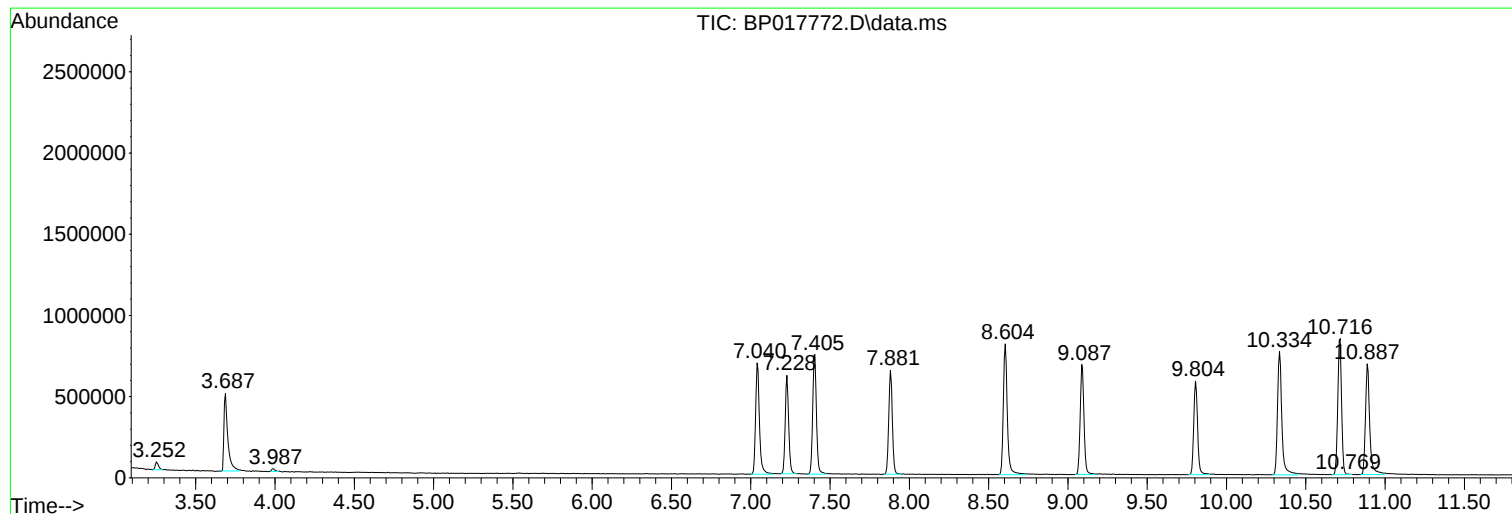

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017772.D
Acq On : 24 Oct 2023 03:55
Operator : MA/JU
Sample : PB156465BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK465

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017772.D
Acq On : 24 Oct 2023 03:55
Operator : MA/JU
Sample : PB156465BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK465

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------