

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017794.D
 Acq On : 25 Oct 2023 01:04
 Operator : MA/JU
 Sample : PB156501BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK501

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017794.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	39	rVB	47810	72070	2.04%	0.180%
2	3.687	98	102	119	rBV	484706	840640	23.81%	2.099%
3	3.987	150	153	159	rVB2	18447	25271	0.72%	0.063%
4	5.240	361	366	368	rBV6	3077	4551	0.13%	0.011%
5	5.999	492	495	497	rBV4	3169	3733	0.11%	0.009%
6	7.040	666	672	689	rBV	701065	1180670	33.43%	2.948%
7	7.228	697	704	716	rBV	602629	943149	26.71%	2.355%
8	7.399	727	733	745	rBV	782904	1234122	34.95%	3.082%
9	7.881	807	815	824	rBV	607066	954489	27.03%	2.384%
10	8.605	931	938	958	rBV	839976	1461339	41.38%	3.649%
11	9.087	1012	1020	1036	rBV	725466	1177127	33.33%	2.940%
12	9.804	1134	1142	1156	rBV	603362	1021303	28.92%	2.550%
13	10.328	1224	1231	1246	rBV	790223	1474862	41.77%	3.683%
14	10.710	1288	1296	1305	rBV	803638	1332467	37.73%	3.327%
15	10.887	1316	1326	1347	rBV	704357	1348188	38.18%	3.367%
16	12.316	1563	1569	1573	rBV3	13070	23273	0.66%	0.058%
17	13.363	1742	1747	1750	rBV7	2414	3921	0.11%	0.010%
18	13.416	1750	1756	1762	rVV4	18567	30830	0.87%	0.077%
19	13.534	1772	1776	1783	rVB10	3760	8341	0.24%	0.021%
20	13.998	1848	1855	1866	rBV	1472258	2096393	59.37%	5.235%
21	14.275	1895	1902	1912	rBV	1810283	2506308	70.97%	6.259%
22	14.575	1947	1953	1965	rBV	1150277	1706369	48.32%	4.261%
23	14.828	1988	1996	2015	rBV2	306702	774627	21.94%	1.934%
24	15.581	2118	2124	2135	rBV	2209401	3041883	86.14%	7.596%
25	15.728	2143	2149	2162	rBV	540272	783600	22.19%	1.957%
26	15.822	2162	2165	2170	rVB4	11244	16674	0.47%	0.042%
27	17.039	2367	2372	2377	rVB8	3265	5744	0.16%	0.014%
28	17.163	2389	2393	2397	rBV4	2541	4538	0.13%	0.011%
29	17.369	2421	2428	2438	rBV	1427584	1957680	55.44%	4.889%
30	17.469	2438	2445	2466	rVV2	2237610	3168879	89.74%	7.913%
31	18.010	2532	2537	2539	rBV6	2980	4052	0.11%	0.010%
32	18.228	2569	2574	2581	rBV10	10667	20779	0.59%	0.052%
33	19.298	2752	2756	2760	rBV2	22708	28712	0.81%	0.072%
34	19.369	2764	2768	2774	rVB	26384	35212	1.00%	0.088%
35	19.475	2782	2786	2791	rBV7	11264	16471	0.47%	0.041%
36	19.604	2806	2808	2812	rVB5	10763	11591	0.33%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017794.D
Acq On : 25 Oct 2023 01:04
Operator : MA/JU
Sample : PB156501BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK501

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	19.727	2823	2829	2838	rBV	2770378	3531273	100.00%	8.818%
38	21.510	3127	3132	3141	rBV	1414495	1886363	53.42%	4.711%
39	23.198	3416	3419	3425	rVB2	108638	160860	4.56%	0.402%
40	23.892	3529	3537	3546	rBV2	1610765	3310860	93.76%	8.268%
41	24.063	3559	3566	3577	rVB	865508	1835609	51.98%	4.584%




Sum of corrected areas: 40044823

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017794.D
Acq On : 25 Oct 2023 01:04
Operator : MA/JU
Sample : PB156501BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK501

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

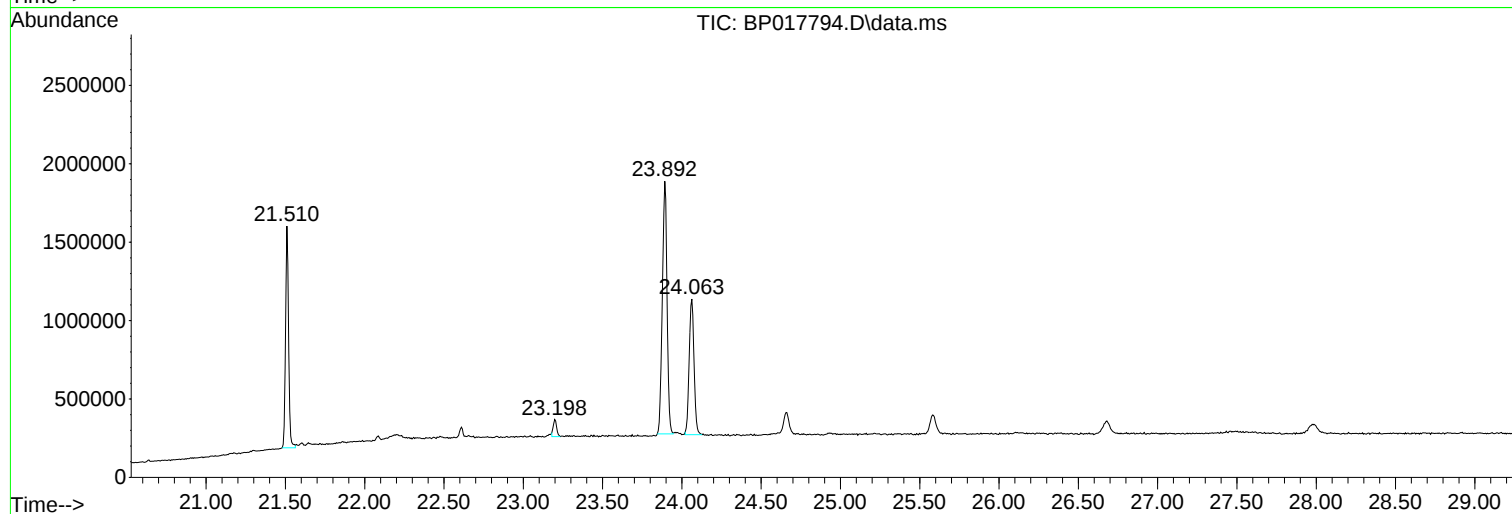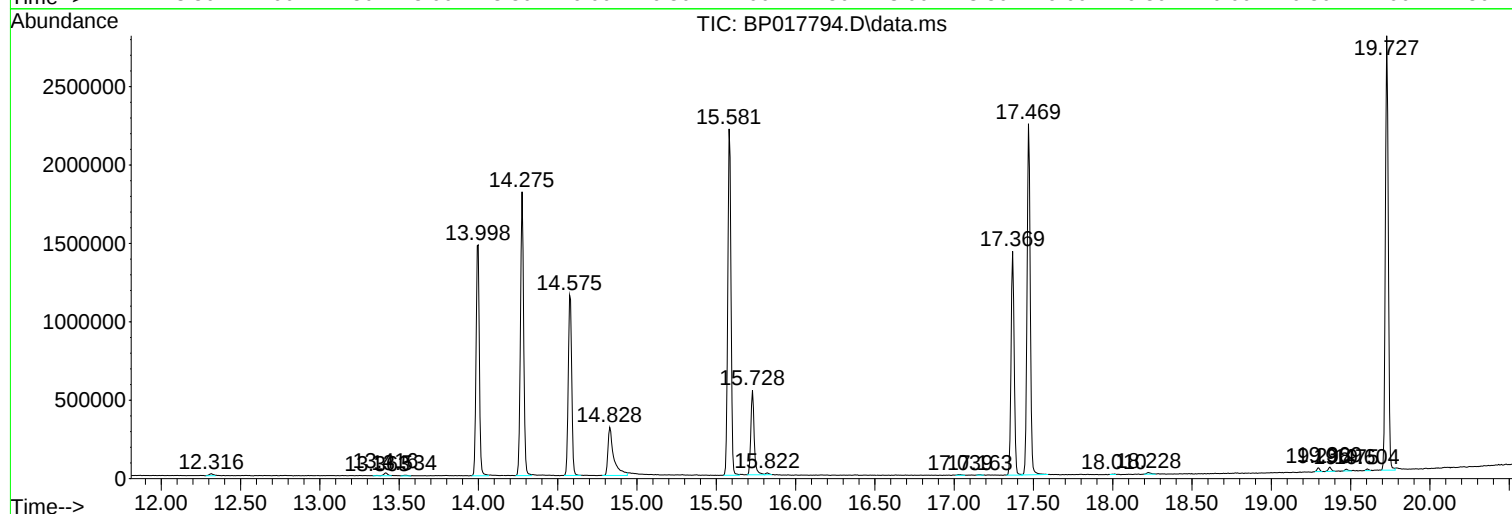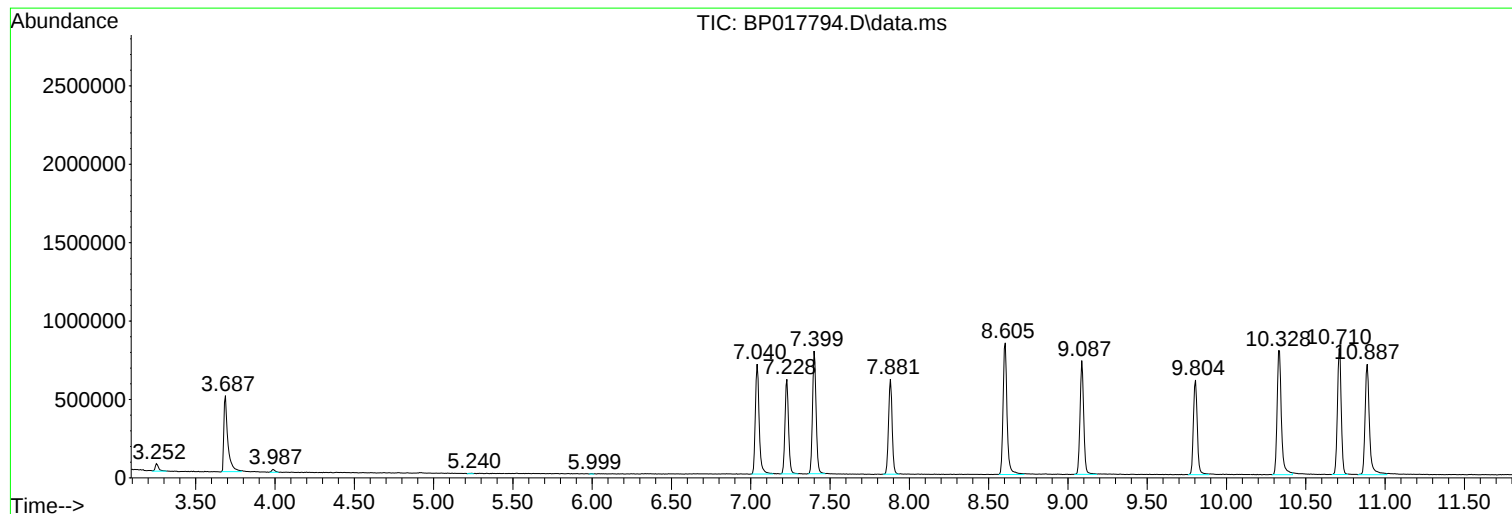

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017794.D
Acq On : 25 Oct 2023 01:04
Operator : MA/JU
Sample : PB156501BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK501

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017794.D
Acq On : 25 Oct 2023 01:04
Operator : MA/JU
Sample : PB156501BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK501

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc