

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017795.D
 Acq On : 25 Oct 2023 01:38
 Operator : MA/JU
 Sample : 04987-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.987	150	153	155	rBV4	5914	6703	0.40%	0.081%
2	4.387	219	221	224	rVB3	3547	2622	0.16%	0.032%
3	5.446	399	401	403	rBV3	2083	1754	0.11%	0.021%
4	5.552	417	419	422	rBV4	3081	2919	0.17%	0.035%
5	5.681	439	441	443	rBV2	1980	1993	0.12%	0.024%
6	6.434	567	569	572	rVB4	2362	2230	0.13%	0.027%
7	6.493	578	579	582	rVV3	1866	1752	0.10%	0.021%
8	6.528	582	585	587	rVB4	1796	2068	0.12%	0.025%
9	7.016	665	668	670	rBV4	1538	2097	0.13%	0.025%
10	7.205	698	700	702	rBV3	2328	1804	0.11%	0.022%
11	7.787	795	799	800	rBV4	1954	2318	0.14%	0.028%
12	7.881	808	815	826	rBV	494583	800913	47.99%	9.714%
13	8.069	845	847	850	rVB4	2322	1966	0.12%	0.024%
14	8.434	905	909	910	rBV4	1391	2001	0.12%	0.024%
15	8.540	924	927	928	rVV3	2117	2261	0.14%	0.027%
16	8.552	928	929	933	rVB4	2270	2408	0.14%	0.029%
17	8.581	933	934	938	rVB4	2293	2005	0.12%	0.024%
18	8.799	967	971	972	rBV4	2585	2242	0.13%	0.027%
19	9.099	1018	1022	1024	rBV5	1487	2266	0.14%	0.027%
20	9.205	1035	1040	1041	rBV5	2116	3022	0.18%	0.037%
21	9.593	1104	1106	1110	rBV5	2266	2508	0.15%	0.030%
22	9.799	1135	1141	1143	rVB7	1720	3070	0.18%	0.037%
23	9.852	1146	1150	1153	rVV4	2323	2826	0.17%	0.034%
24	10.005	1170	1176	1177	rBV5	1172	2156	0.13%	0.026%
25	10.157	1199	1202	1205	rBV5	1490	1997	0.12%	0.024%
26	10.205	1208	1210	1214	rVB5	1653	2160	0.13%	0.026%
27	10.410	1244	1245	1250	rBV4	1509	1699	0.10%	0.021%
28	10.710	1288	1296	1310	rBV	618337	1086030	65.08%	13.172%
29	11.252	1384	1388	1390	rVV5	1929	2216	0.13%	0.027%
30	11.310	1394	1398	1400	rBV5	1652	2046	0.12%	0.025%
31	11.493	1426	1429	1430	rBV2	1829	1877	0.11%	0.023%
32	11.569	1437	1442	1443	rVB5	1850	2408	0.14%	0.029%
33	12.122	1535	1536	1539	rVB3	2184	1768	0.11%	0.021%
34	12.193	1544	1548	1549	rBV3	2052	1989	0.12%	0.024%
35	12.210	1549	1551	1554	rVB4	2301	1863	0.11%	0.023%
36	12.257	1554	1559	1560	rBV5	1469	1787	0.11%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017795.D
 Acq On : 25 Oct 2023 01:38
 Operator : MA/JU
 Sample : 04987-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	12.340	1568	1573	1575	rVB6	1667	2160	0.13%	0.026%
38	12.710	1631	1636	1640	rBV8	1691	2919	0.17%	0.035%
39	12.746	1640	1642	1645	rVV4	1610	1833	0.11%	0.022%
40	12.810	1649	1653	1655	rVB5	1350	1972	0.12%	0.024%

41	12.887	1662	1666	1668	rVB5	2082	2783	0.17%	0.034%
42	12.951	1674	1677	1678	rBV3	2745	2325	0.14%	0.028%
43	13.034	1689	1691	1694	rVB4	1834	2157	0.13%	0.026%
44	13.416	1751	1756	1761	rBV9	4814	8757	0.52%	0.106%
45	13.451	1761	1762	1766	rVB4	2015	1775	0.11%	0.022%

46	13.569	1779	1782	1784	rBV4	1492	1699	0.10%	0.021%
47	13.793	1816	1820	1822	rBV5	1029	1720	0.10%	0.021%
48	13.940	1844	1845	1848	rBV3	2023	1851	0.11%	0.022%
49	14.040	1860	1862	1864	rBV3	2247	2865	0.17%	0.035%
50	14.140	1876	1879	1882	rBV5	1918	2829	0.17%	0.034%

51	14.575	1946	1953	1969	rBV	944658	1460557	87.52%	17.715%
52	14.793	1987	1990	1993	rVB4	2062	2605	0.16%	0.032%
53	14.963	2017	2019	2022	rVB4	1828	1845	0.11%	0.022%
54	15.075	2036	2038	2040	rVV3	1952	2177	0.13%	0.026%
55	15.122	2043	2046	2051	rVV7	1235	1982	0.12%	0.024%

56	15.310	2076	2078	2080	rBV3	2666	2249	0.13%	0.027%
57	15.363	2083	2087	2088	rBV3	1944	2479	0.15%	0.030%
58	15.528	2110	2115	2116	rVB5	1400	1792	0.11%	0.022%
59	15.604	2124	2128	2131	rVV6	2203	3248	0.19%	0.039%
60	15.675	2134	2140	2142	rBV7	1937	3092	0.19%	0.038%

61	16.375	2256	2259	2261	rBV4	1477	1734	0.10%	0.021%
62	16.445	2268	2271	2274	rVB5	1772	1890	0.11%	0.023%
63	16.634	2300	2303	2306	rVB5	2071	1922	0.12%	0.023%
64	16.657	2306	2307	2310	rVB3	2459	1731	0.10%	0.021%
65	16.687	2310	2312	2314	rBV3	1455	1745	0.10%	0.021%

66	16.787	2326	2329	2330	rVB3	2391	2157	0.13%	0.026%
67	16.798	2330	2331	2334	rBV3	1659	1899	0.11%	0.023%
68	16.963	2358	2359	2361	rBV2	1756	1671	0.10%	0.020%
69	17.145	2388	2390	2392	rBV3	2076	2295	0.14%	0.028%
70	17.222	2399	2403	2406	rVB6	2202	2688	0.16%	0.033%

71	17.257	2406	2409	2411	rBV3	2177	2765	0.17%	0.034%
72	17.369	2422	2428	2450	rBV	1101608	1668845	100.00%	20.241%
73	17.528	2454	2455	2458	rVB3	2387	1914	0.11%	0.023%
74	18.239	2574	2576	2578	rBV3	2329	2010	0.12%	0.024%
75	19.604	2806	2808	2811	rBV4	9725	11608	0.70%	0.141%

76	21.510	3127	3132	3142	rBV	1132565	1565528	93.81%	18.988%
----	--------	------	------	------	-----	---------	---------	--------	---------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017795.D
Acq On : 25 Oct 2023 01:38
Operator : MA/JU
Sample : 04987-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

77	24.063	3559	3566	3578	rVB	699922	1486927	89.10%	18.035%
----	--------	------	------	------	-----	--------	---------	--------	---------




Sum of corrected areas: 8244744

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017795.D
Acq On : 25 Oct 2023 01:38
Operator : MA/JU
Sample : 04987-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

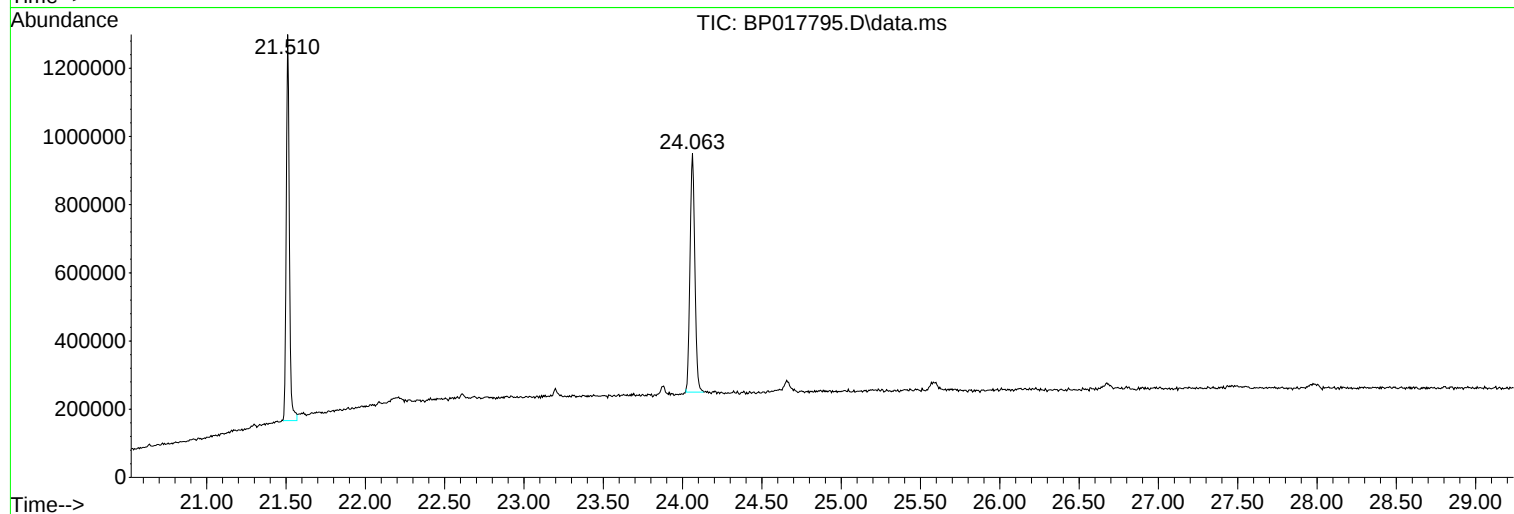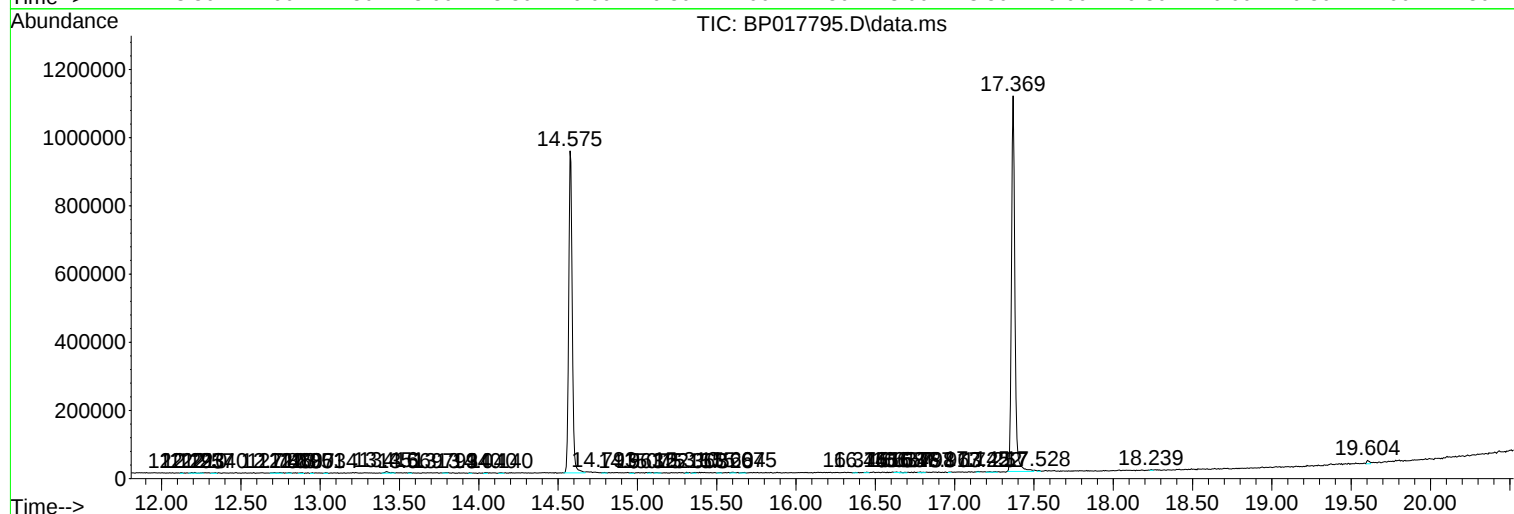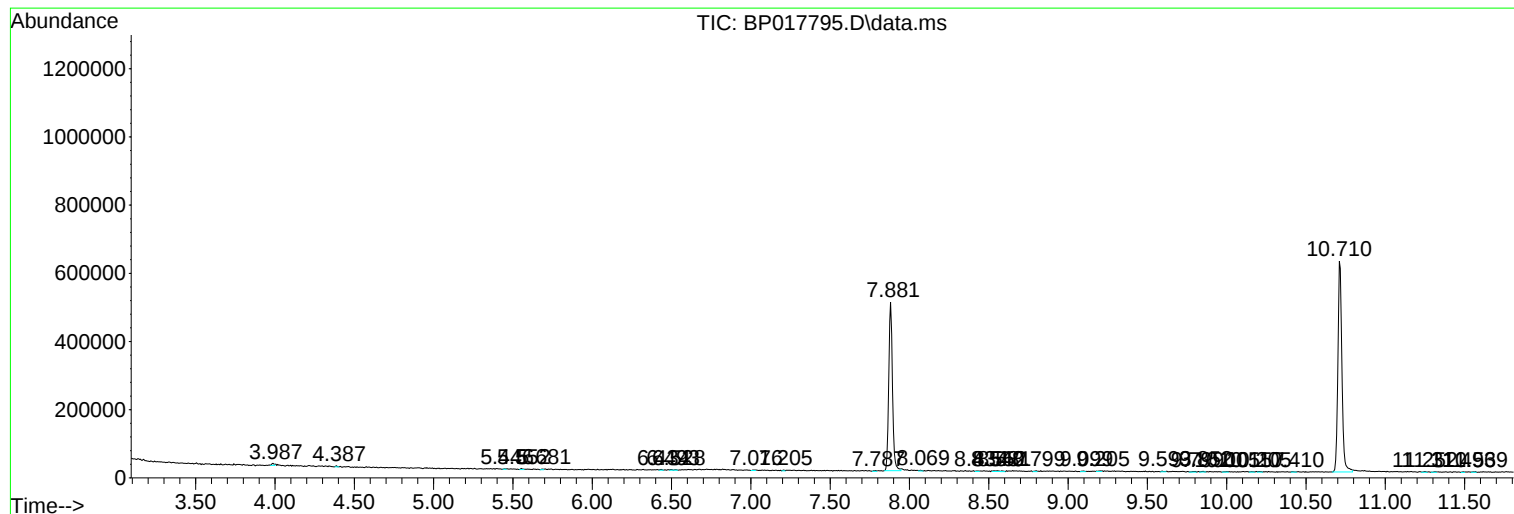

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017795.D
Acq On : 25 Oct 2023 01:38
Operator : MA/JU
Sample : 04987-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017795.D
Acq On : 25 Oct 2023 01:38
Operator : MA/JU
Sample : 04987-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc