

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017796.D
 Acq On : 25 Oct 2023 02:12
 Operator : MA/JU
 Sample : 04987-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.905	137	139	142	rBV4	3115	2946	0.19%	0.037%
2	3.987	150	153	157	rBV4	6095	7833	0.49%	0.097%
3	4.793	288	290	294	rVB5	3059	3101	0.19%	0.039%
4	5.040	330	332	333	rBV2	2383	2034	0.13%	0.025%
5	5.258	365	369	371	rBV5	2288	3308	0.21%	0.041%
6	5.275	371	372	375	rVB3	2570	1616	0.10%	0.020%
7	5.299	375	376	379	rBV2	1763	2122	0.13%	0.026%
8	5.722	446	448	450	rBV3	1613	1597	0.10%	0.020%
9	5.840	466	468	469	rVB2	2563	1740	0.11%	0.022%
10	5.934	482	484	486	rBV3	2229	1755	0.11%	0.022%
11	6.522	583	584	587	rBV3	2312	2349	0.15%	0.029%
12	6.605	593	598	602	rVB8	2354	4040	0.25%	0.050%
13	6.646	602	605	608	rBV5	2346	2499	0.16%	0.031%
14	6.693	610	613	616	rBV5	1664	1901	0.12%	0.024%
15	7.293	714	715	717	rBV2	2020	1602	0.10%	0.020%
16	7.346	723	724	729	rVV5	1584	2159	0.14%	0.027%
17	7.881	808	815	824	rBV	485176	794229	49.93%	9.862%
18	8.275	879	882	883	rBV3	1657	1852	0.12%	0.023%
19	8.481	916	917	922	rBV5	1069	1684	0.11%	0.021%
20	8.604	936	938	940	rVB2	2167	1824	0.11%	0.023%
21	8.652	942	946	949	rBV5	2193	4026	0.25%	0.050%
22	8.810	969	973	975	rBV5	1569	2384	0.15%	0.030%
23	9.057	1013	1015	1017	rVB2	2145	1860	0.12%	0.023%
24	9.104	1019	1023	1026	rVB5	1570	2944	0.19%	0.037%
25	9.222	1041	1043	1045	rBV3	1635	1860	0.12%	0.023%
26	9.340	1061	1063	1066	rBV4	1703	1979	0.12%	0.025%
27	9.369	1066	1068	1071	rVV4	1129	1724	0.11%	0.021%
28	9.422	1073	1077	1081	rBV7	1720	2491	0.16%	0.031%
29	9.534	1094	1096	1099	rVB4	1578	1769	0.11%	0.022%
30	9.916	1158	1161	1164	rBV5	1819	2187	0.14%	0.027%
31	9.951	1164	1167	1170	rVB5	2618	2827	0.18%	0.035%
32	10.075	1185	1188	1191	rVB5	1894	2464	0.15%	0.031%
33	10.122	1191	1196	1197	rBV5	1979	1887	0.12%	0.023%
34	10.334	1230	1232	1234	rBV2	2214	1824	0.11%	0.023%
35	10.551	1268	1269	1272	rBV3	1405	1615	0.10%	0.020%
36	10.628	1277	1282	1283	rVB5	1673	2206	0.14%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017796.D
 Acq On : 25 Oct 2023 02:12
 Operator : MA/JU
 Sample : 04987-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	10.710	1289	1296	1307	rBV	613210	1068714	67.18%	13.270%
38	10.781	1307	1308	1314	rVV4	5911	7792	0.49%	0.097%
39	11.581	1441	1444	1447	rVB3	2221	3002	0.19%	0.037%
40	11.604	1447	1448	1451	rBV2	1941	2218	0.14%	0.028%
41	11.875	1491	1494	1497	rBV5	1737	2574	0.16%	0.032%
42	11.940	1504	1505	1510	rBV5	1317	1607	0.10%	0.020%
43	11.998	1513	1515	1519	rVV5	1354	1753	0.11%	0.022%
44	12.051	1521	1524	1526	rVV4	1760	1592	0.10%	0.020%
45	12.257	1557	1559	1562	rVB4	2069	2496	0.16%	0.031%
46	12.351	1572	1575	1579	rBV6	1583	2867	0.18%	0.036%
47	12.622	1616	1621	1622	rVB5	2079	2646	0.17%	0.033%
48	12.645	1622	1625	1626	rBV3	2074	2025	0.13%	0.025%
49	12.775	1645	1647	1649	rVB3	1793	1664	0.10%	0.021%
50	12.981	1678	1682	1685	rBV6	1154	1622	0.10%	0.020%
51	13.134	1704	1708	1710	rBV4	1628	1857	0.12%	0.023%
52	13.204	1718	1720	1725	rVB5	1599	2364	0.15%	0.029%
53	13.334	1739	1742	1745	rVB5	1522	1688	0.11%	0.021%
54	13.381	1745	1750	1751	rBV5	1742	2773	0.17%	0.034%
55	13.416	1751	1756	1765	rVB6	9217	18972	1.19%	0.236%
56	13.540	1774	1777	1781	rBV6	1611	2849	0.18%	0.035%
57	13.675	1796	1800	1802	rBV5	1286	1967	0.12%	0.024%
58	13.763	1810	1815	1817	rBV6	2294	3185	0.20%	0.040%
59	13.792	1817	1820	1822	rBV4	1717	1747	0.11%	0.022%
60	14.181	1880	1886	1889	rBV7	1429	2258	0.14%	0.028%
61	14.216	1889	1892	1894	rBV4	1456	1696	0.11%	0.021%
62	14.439	1927	1930	1932	rVB4	2012	2034	0.13%	0.025%
63	14.581	1946	1954	1970	rBV	932195	1423219	89.46%	17.672%
64	15.092	2040	2041	2045	rVB4	2099	2079	0.13%	0.026%
65	15.128	2045	2047	2049	rBV3	2550	2376	0.15%	0.030%
66	15.657	2133	2137	2138	rBV4	1809	2266	0.14%	0.028%
67	15.834	2164	2167	2169	rBV4	2025	1994	0.13%	0.025%
68	15.981	2190	2192	2195	rBV4	1422	1758	0.11%	0.022%
69	16.086	2206	2210	2212	rBV5	2235	2314	0.15%	0.029%
70	16.145	2215	2220	2222	rBV6	1244	1770	0.11%	0.022%
71	16.228	2232	2234	2236	rVB2	2476	1654	0.10%	0.021%
72	16.281	2239	2243	2246	rBV6	2233	3196	0.20%	0.040%
73	16.328	2249	2251	2254	rBV4	1398	2113	0.13%	0.026%
74	16.475	2274	2276	2278	rVV3	2090	2055	0.13%	0.026%
75	16.692	2310	2313	2316	rVB5	2275	2780	0.17%	0.035%
76	16.739	2318	2321	2324	rVB5	1140	1807	0.11%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
 Data File : BP017796.D
 Acq On : 25 Oct 2023 02:12
 Operator : MA/JU
 Sample : 04987-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

77	17.028	2367	2370	2372	rBV3	3482	2889	0.18%	0.036%
78	17.163	2389	2393	2395	rBV4	2242	2840	0.18%	0.035%
79	17.369	2421	2428	2442	rBV	1086880	1590813	100.00%	19.753%
80	17.457	2442	2443	2445	rBV2	1974	1622	0.10%	0.020%
81	17.651	2473	2476	2479	rBV5	1780	2138	0.13%	0.027%
82	17.757	2492	2494	2496	rVB3	2234	1890	0.12%	0.023%
83	17.775	2496	2497	2499	rBV2	2637	1766	0.11%	0.022%
84	18.228	2570	2574	2579	rBV8	7128	12186	0.77%	0.151%
85	18.451	2608	2612	2613	rBV3	2552	2775	0.17%	0.034%
86	18.492	2616	2619	2621	rVB3	2457	2601	0.16%	0.032%
87	19.463	2782	2784	2785	rBV2	6363	5114	0.32%	0.063%
88	19.604	2806	2808	2813	rVB6	6162	7410	0.47%	0.092%
89	21.510	3127	3132	3141	rBV	1133497	1520795	95.60%	18.883%
90	24.063	3559	3566	3577	rVB	689381	1423206	89.46%	17.672%




Sum of corrected areas: 8053626

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017796.D
Acq On : 25 Oct 2023 02:12
Operator : MA/JU
Sample : 04987-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

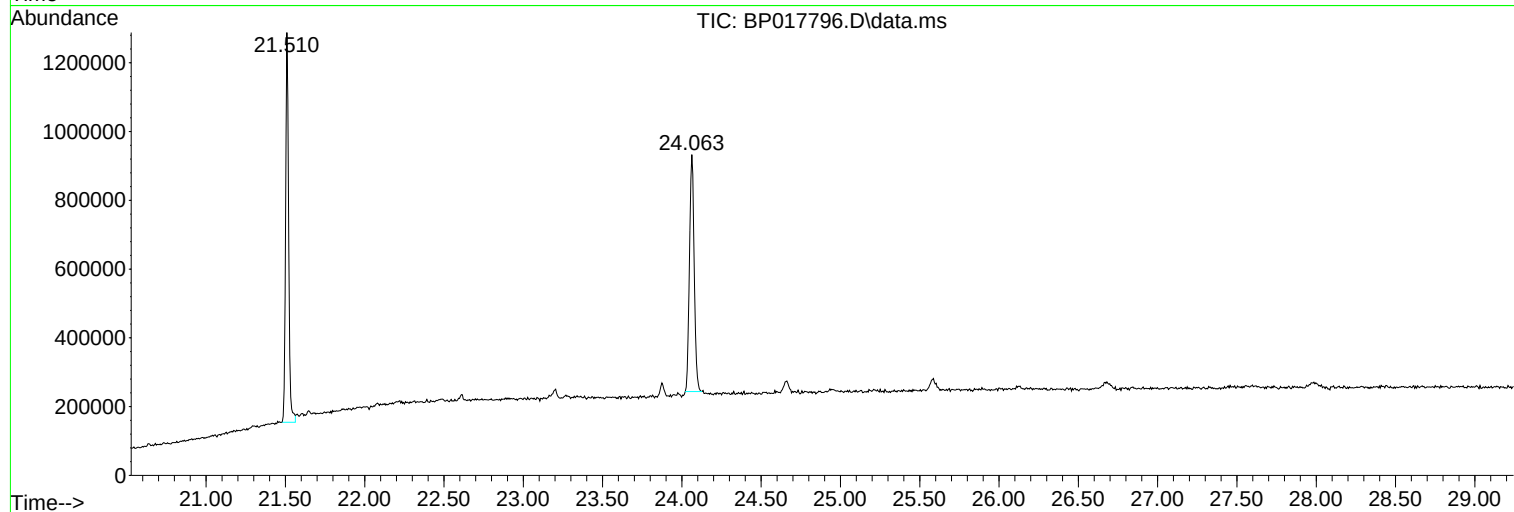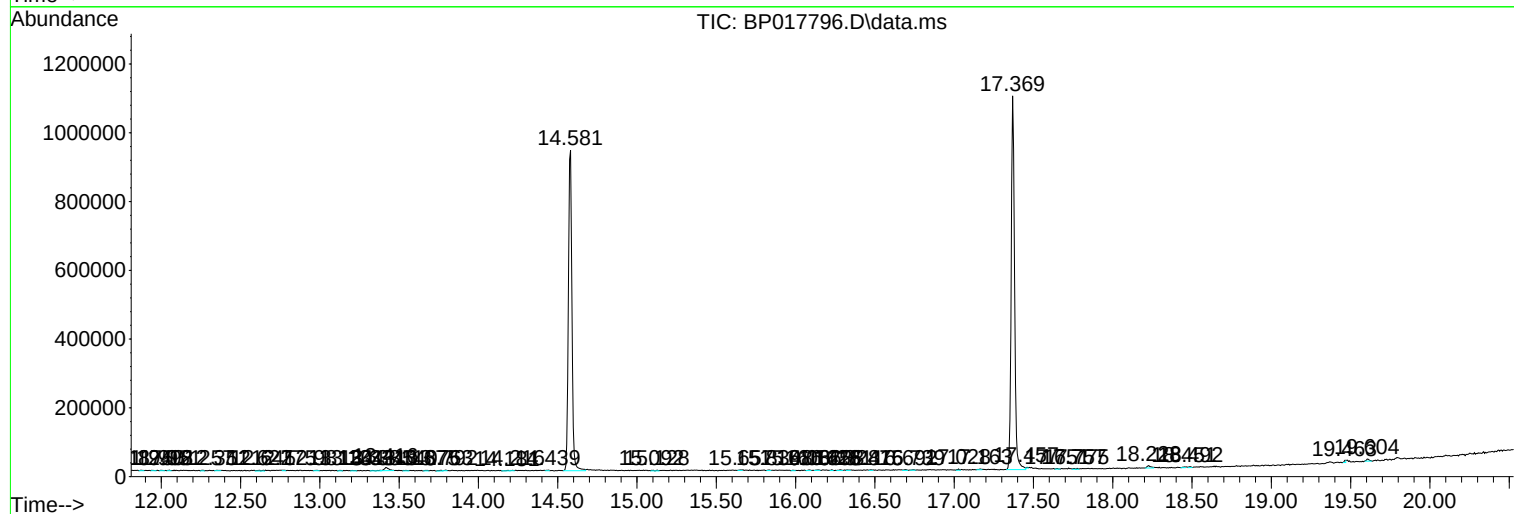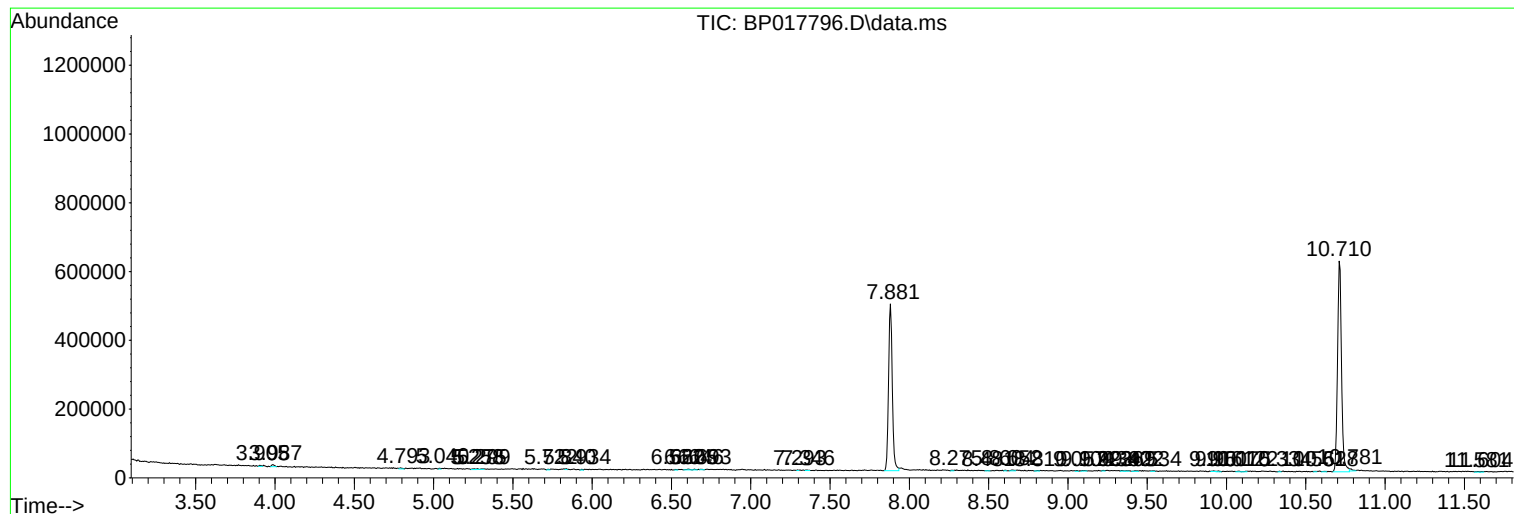

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017796.D
Acq On : 25 Oct 2023 02:12
Operator : MA/JU
Sample : 04987-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102323\
Data File : BP017796.D
Acq On : 25 Oct 2023 02:12
Operator : MA/JU
Sample : 04987-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc