

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
 Data File : BP017808.D
 Acq On : 25 Oct 2023 18:07
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020795

Quant Time: Oct 26 04:56:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	106391	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	419538	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.575	164	246231	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.369	188	501444	20.000	ng/u1	0.00
79) Chrysene-d12	21.510	240	454399	20.000	ng/u1	0.00
88) Perylene-d12	24.063	264	450703	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	25370	8.871	ng/uL	0.01
4) Pyridine-d5	3.699	84	161351	21.549	ng/u1	0.00
7) Phenol-d5	7.046	99	192553	21.749	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	121759	22.269	ng/u1	0.00
11) 2-Chlorophenol-d4	7.405	132	159645	22.109	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	151252	21.755	ng/u1	0.00
21) Nitrobenzene-d5	9.087	128	73668	21.670	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.805	143	82008	21.833	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	147931	20.077	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	194534	20.174	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	410243	19.847	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	474385	20.579	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	53871	18.291	ng/u1	0.00
60) Fluorene-d10	15.581	176	346132	19.372	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.734	200	62378	18.885	ng/u1	0.00
73) Anthracene-d10	17.469	188	521637	20.357	ng/u1	0.00
81) Pyrene-d10	19.728	212	579556	20.343	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.892	264	509752	20.307	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.305	88	28448	9.378	ng/uL	92
5) Pyridine	3.723	79	166876	21.753	ng/u1	99
6) Benzaldehyde	7.046	77	121441	25.499	ng/u1	93
8) Phenol	7.069	94	192640	22.068	ng/u1	96
10) Bis(2-Chloroethyl)ether	7.322	93	158874	21.815	ng/u1	98
12) 2-Chlorophenol	7.434	128	159760	22.028	ng/u1	97
13) 2-Methylphenol	8.334	108	141625	21.498	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.393	45	128387	14.322	ng/u1	99
16) Acetophenone	8.740	105	236532	21.640	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.705	70	111484	21.503	ng/u1	98
18) 4-Methylphenol	8.669	108	149389	21.353	ng/u1	98
19) Hexachloroethane	8.940	117	75977	22.800	ng/u1	87
22) Nitrobenzene	9.134	77	193014	22.802	ng/u1	99
23) Isophorone	9.646	82	330099	21.808	ng/u1	99
25) 2-Nitrophenol	9.840	139	86355	21.538	ng/u1	91
26) 2,4-Dimethylphenol	9.881	107	172278	21.893	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.134	93	198063	21.156	ng/u1	96
29) 2,4-Dichlorophenol	10.357	162	142870	20.277	ng/u1	95
30) Naphthalene	10.763	128	490441	20.313	ng/u1	99
32) 4-Chloroaniline	10.910	127	184763	20.010	ng/u1	97
33) Hexachlorobutadiene	10.987	225	106033	18.535	ng/u1	100
34) Caprolactam	11.751	113	34494	19.013	ng/u1	88
35) 4-Chloro-3-methylphenol	12.022	107	145181	21.887	ng/u1	89
36) 2-Methylnaphthalene	12.381	142	322805	19.793	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
 Data File : BP017808.D
 Acq On : 25 Oct 2023 18:07
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020795


Quant Time: Oct 26 04:56:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.604	142	322747	19.351	ng/ul	93
39) 1,2,4,5-Tetrachloroben...	12.734	216	175527	19.265	ng/ul#	98
40) Hexachlorocyclopentadiene	12.675	237	90290	17.248	ng/ul	99
41) 2,4,6-Trichlorophenol	12.998	196	110463	20.201	ng/ul	97
42) 2,4,5-Trichlorophenol	13.075	196	114365	20.230	ng/ul	99
43) 1,1'-Biphenyl	13.404	154	417467	20.579	ng/ul	98
44) 2-Chloronaphthalene	13.451	162	333309	20.325	ng/ul	96
45) 2-Nitroaniline	13.698	65	91982	24.683	ng/ul	93
47) Dimethylphthalate	14.045	163	406190	19.939	ng/ul	99
48) 2,6-Dinitrotoluene	14.198	165	77305	20.616	ng/ul	91
50) Acenaphthylene	14.304	152	533015	20.642	ng/ul	99
51) 3-Nitroaniline	14.540	138	73586	20.634	ng/ul	95
52) Acenaphthene	14.645	153	348446	19.962	ng/ul	98
53) 2,4-Dinitrophenol	14.751	184	33226	15.785	ng/ul	88
55) 4-Nitrophenol	14.840	109	67061	21.509	ng/ul	94
56) Dibenzofuran	14.981	168	480675	19.613	ng/ul	93
57) 2,4-Dinitrotoluene	14.987	165	113396	20.490	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.204	232	91442	18.227	ng/ul#	83
59) Diethylphthalate	15.404	149	407674	20.726	ng/ul	98
61) Fluorene	15.640	166	389726	19.359	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.634	204	196820	18.394	ng/ul	93
63) 4-Nitroaniline	15.716	138	68226	21.211	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.745	198	66167	18.703	ng/ul#	90
67) N-Nitrosodiphenylamine	15.863	169	323744	21.311	ng/ul	100
68) 4-Bromophenyl-phenylether	16.539	248	111365	18.981	ng/ul#	87
69) Hexachlorobenzene	16.622	284	120405	17.876	ng/ul#	87
70) Atrazine	16.828	200	110735	19.833	ng/ul	98
71) Pentachlorophenol	16.998	266	67748	16.730	ng/ul	93
72) Phenanthrene	17.410	178	599460	20.408	ng/ul	100
74) Anthracene	17.504	178	606104	20.372	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.357	216	172119	20.457	ng/ul	95
76) Pentachlorobenzene	14.875	250	157370	19.299	ng/ul	98
77) Carbazole	17.804	167	517393	20.577	ng/ul	99
78) Di-n-butylphthalate	18.310	149	664311	22.756	ng/ul	99
80) Fluoranthene	19.398	202	682914	20.864	ng/ul	98
82) Pyrene	19.757	202	712581	20.549	ng/ul	97
83) Butylbenzylphthalate	20.627	149	293717	24.626	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.439	252	190420	18.548	ng/ul#	98
85) Benzo(a)anthracene	21.492	228	687298	19.896	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.375	149	411255	24.701	ng/ul#	99
87) Chrysene	21.551	228	652352	19.970	ng/ul	99
89) Di-n-octyl phthalate	22.351	149	694622	24.331	ng/ul	100
90) Benzo(b)fluoranthene	23.269	252	640696	20.887	ng/ul	98
91) Benzo(k)fluoranthene	23.321	252	621195	19.982	ng/ul	99
93) Benzo(a)pyrene	23.945	252	580918	20.173	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.774	276	666798	19.429	ng/ul	98
95) Dibenzo(a,h)anthracene	26.798	278	551345	19.254	ng/ul	98
96) Benzo(g,h,i)perylene	27.615	276	536732	19.410	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 26 04:56:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration







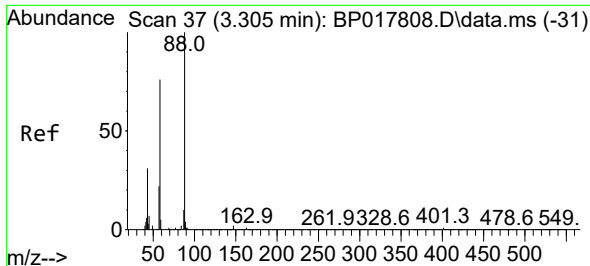

#2
1,4-Dioxane
Concen: 9.378 ng/uL
RT: 3.305 min Scan# 31
Delta R.T. 0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion: 88 Resp: 28448
Ion Ratio Lower Upper
88 100
43 32.6 24.4 36.6
58 74.4 53.0 79.6

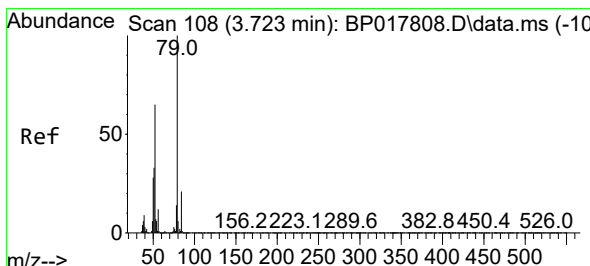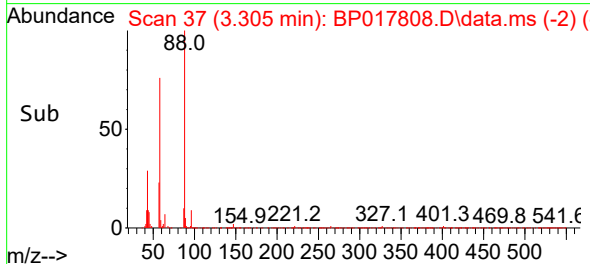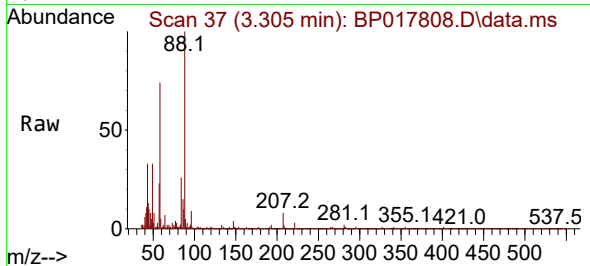

#5
Pyridine
Concen: 21.753 ng/uL
RT: 3.723 min Scan# 108
Delta R.T. 0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion: 79 Resp: 166876
Ion Ratio Lower Upper
79 100
52 71.5 57.2 85.8
51 34.5 28.6 42.8


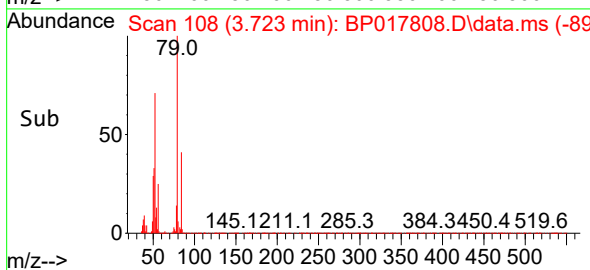

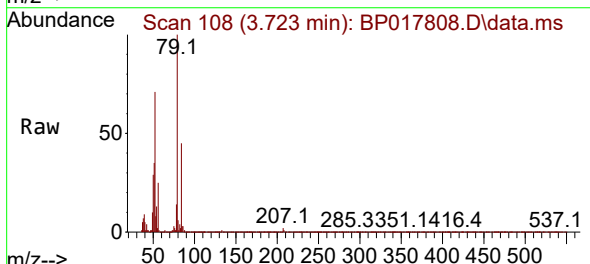




#6
Benzaldehyde
Concen: 25.499 ng/ul
RT: 7.046 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion: 77 Resp: 121441
Ion Ratio Lower Upper
77 100
105 88.0 75.4 113.2
106 84.1 72.3 108.5



#8
Phenol
Concen: 22.068 ng/ul
RT: 7.069 min Scan# 677
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion: 94 Resp: 192640
Ion Ratio Lower Upper
94 100
65 31.4 25.0 37.4
66 46.0 33.0 49.6









#10
Bis(2-Chloroethyl)ether
Concen: 21.815 ng/ul
RT: 7.322 min Scan# 720
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion: 93 Resp: 158874
Ion Ratio Lower Upper
93 100
63 75.4 60.7 91.1
95 31.4 27.8 41.6

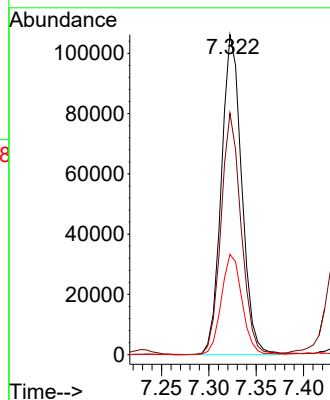

#12
2-Chlorophenol
Concen: 22.028 ng/ul
RT: 7.434 min Scan# 739
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:128 Resp: 159760
Ion Ratio Lower Upper
128 100
64 48.8 36.7 55.1
130 33.4 26.2 39.2

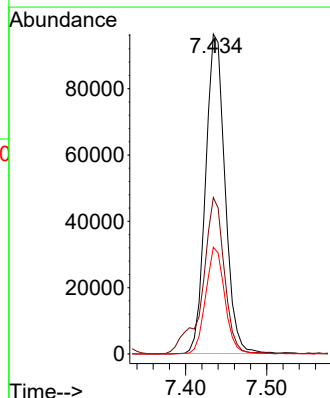



#13

2-Methylphenol

Concen: 21.498 ng/ul

RT: 8.334 min Scan# 892

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :





SSTD020795

Tgt Ion:108 Resp: 141625

Ion Ratio Lower Upper

108 100

107 92.5 73.4 110.2

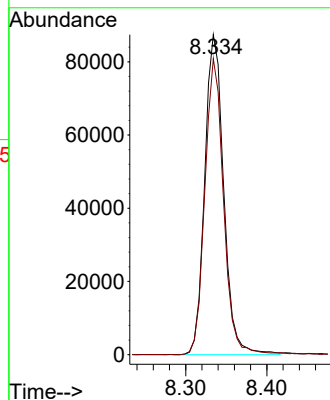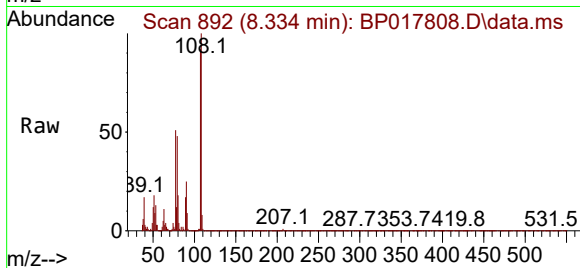

#14

2,2'-oxybis(1-Chloropropane)

Concen: 14.322 ng/ul

RT: 8.393 min Scan# 902

Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion: 45 Resp: 128387


Ion Ratio Lower Upper

45 100

77 17.8 14.2 21.4

79 12.1 10.3 15.5



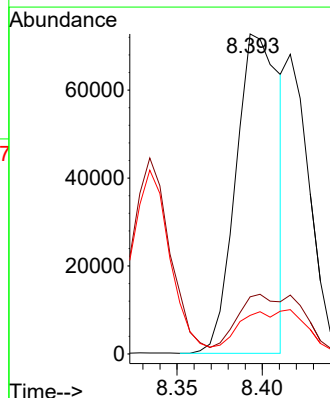
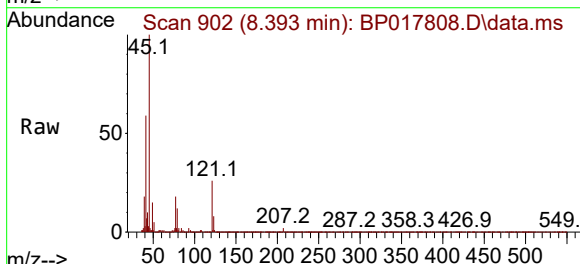




#16
Acetophenone
Concen: 21.640 ng/ul
RT: 8.740 min Scan# 961
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:105 Resp: 236532
Ion Ratio Lower Upper
105 100
77 83.5 64.4 96.6
51 27.9 21.2 31.8

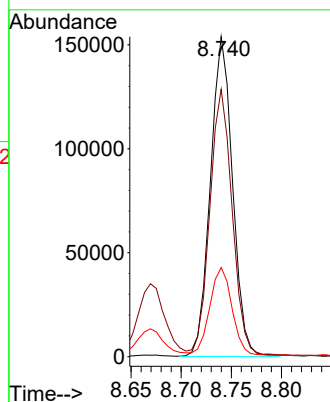

#17
N-Nitroso-di-n-propylamine
Concen: 21.503 ng/ul
RT: 8.705 min Scan# 955
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion: 70 Resp: 111484
Ion Ratio Lower Upper
70 100
42 56.4 44.6 66.8
101 10.1 7.5 11.3
130 19.5 17.3 25.9



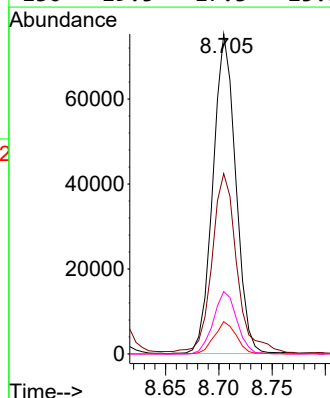





#18
4-Methylphenol
Concen: 21.353 ng/ul
RT: 8.669 min Scan# 949
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:108 Resp: 149389
Ion Ratio Lower Upper
108 100
107 111.8 87.5 131.3

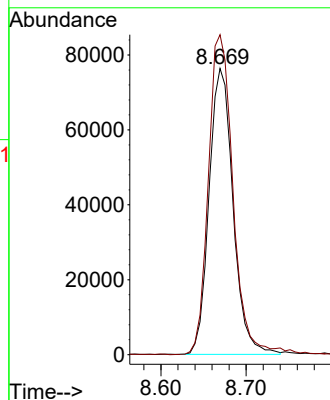

#19
Hexachloroethane
Concen: 22.800 ng/ul
RT: 8.940 min Scan# 995
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:117 Resp: 75977
Ion Ratio Lower Upper
117 100
201 103.8 96.3 144.5
199 63.0 57.7 86.5



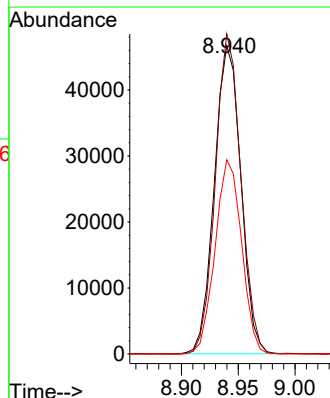





#22
Nitrobenzene
Concen: 22.802 ng/ul
RT: 9.134 min Scan# 1028
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion: 77 Resp: 193014
Ion Ratio Lower Upper
77 100
123 41.3 33.5 50.3
65 13.7 10.8 16.2



#23
Isophorone
Concen: 21.808 ng/ul
RT: 9.646 min Scan# 1115
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion: 82 Resp: 330099
Ion Ratio Lower Upper
82 100
95 7.7 6.2 9.2
138 17.4 14.4 21.6









#25
2-Nitrophenol
Concen: 21.538 ng/ul
RT: 9.840 min Scan# 1148
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:139 Resp: 86355
Ion Ratio Lower Upper
139 100
65 57.5 40.4 60.6
109 35.9 25.4 38.2



#26
2,4-Dimethylphenol
Concen: 21.893 ng/ul
RT: 9.881 min Scan# 1155
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:107 Resp: 172278
Ion Ratio Lower Upper
107 100
121 47.7 40.6 61.0
122 81.1 66.9 100.3









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.156 ng/ul
 RT: 10.134 min Scan# 1198
 Delta R.T. -0.012 min
 Lab File: BP017808.D
 Acq: 25 Oct 2023 18:07




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020795


Tgt Ion: 93 Resp: 198063
 Ion Ratio Lower Upper
 93 100
 95 33.4 24.7 37.1
 123 11.4 8.9 13.3

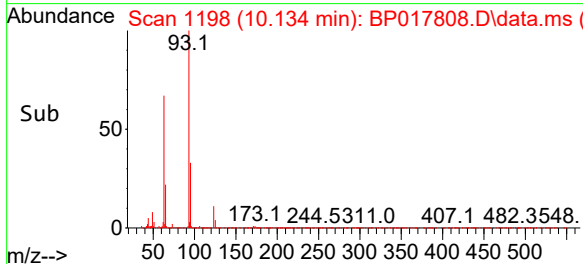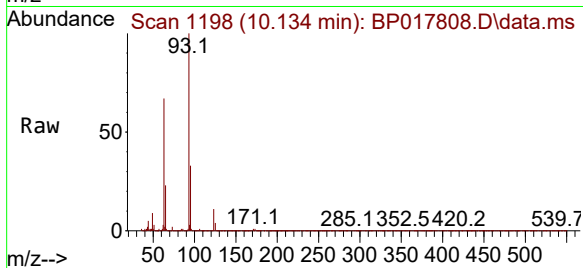

#29
 2,4-Dichlorophenol
 Concen: 20.277 ng/ul
 RT: 10.357 min Scan# 1236
 Delta R.T. -0.012 min
 Lab File: BP017808.D
 Acq: 25 Oct 2023 18:07

Tgt Ion:162 Resp: 142870
 Ion Ratio Lower Upper
 162 100
 164 64.8 53.8 80.8
 98 36.2 25.5 38.3


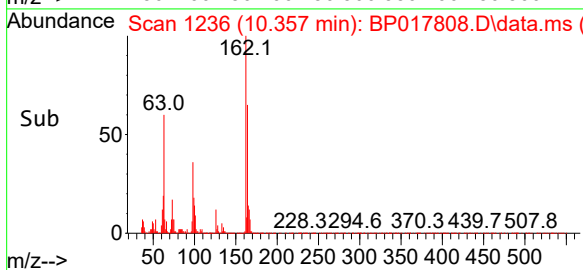

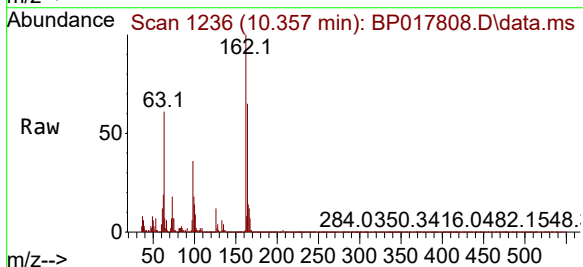




#30
Naphthalene
Concen: 20.313 ng/ul
RT: 10.763 min Scan# 1305
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:128 Resp: 490441
Ion Ratio Lower Upper
128 100
129 11.4 8.7 13.1
127 12.9 10.5 15.7

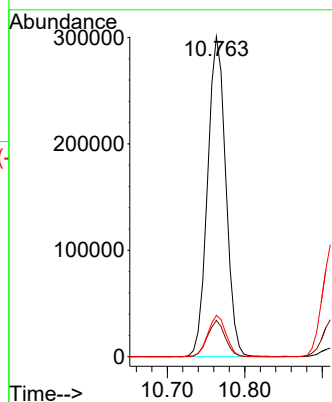

#32
4-Chloroaniline
Concen: 20.010 ng/ul
RT: 10.910 min Scan# 1330
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:127 Resp: 184763
Ion Ratio Lower Upper
127 100
129 33.0 25.1 37.7









#33
Hexachlorobutadiene
Concen: 18.535 ng/ul
RT: 10.987 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:225 Resp: 106033
Ion Ratio Lower Upper
225 100
223 63.6 50.6 75.8
227 62.3 50.1 75.1

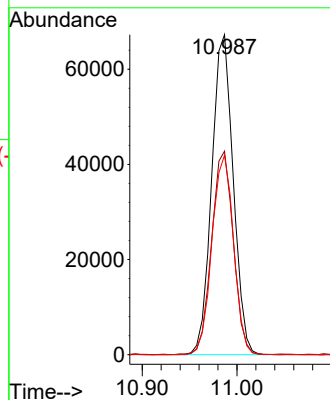

#34
Caprolactam
Concen: 19.013 ng/ul
RT: 11.751 min Scan# 1473
Delta R.T. -0.018 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:113 Resp: 34494
Ion Ratio Lower Upper
113 100
55 153.8 112.1 168.1
56 123.3 87.0 130.6



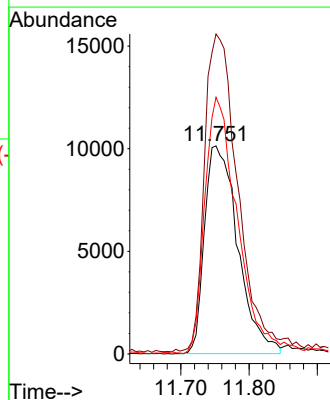





#35
4-Chloro-3-methylphenol
Concen: 21.887 ng/ul
RT: 12.022 min Scan# 1519
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:107 Resp: 145181
Ion Ratio Lower Upper
107 100
144 23.8 22.9 34.3
142 75.1 68.1 102.1

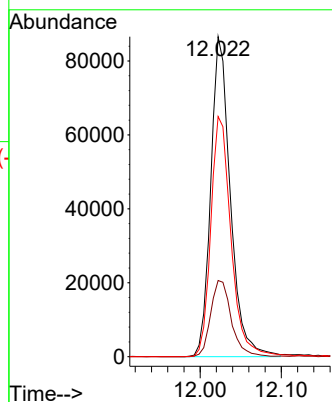

#36
2-Methylnaphthalene
Concen: 19.793 ng/ul
RT: 12.381 min Scan# 1580
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:142 Resp: 322805
Ion Ratio Lower Upper
142 100
141 89.7 71.5 107.3





#37

1-Methylnaphthalene

Concen: 19.351 ng/ul

RT: 12.604 min Scan# 1618

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:142 Resp: 322747

Ion Ratio Lower Upper

142 100

141 97.2 72.5 108.7

116 4.5 3.4 5.2



#39

1,2,4,5-Tetrachlorobenzene

Concen: 19.265 ng/ul

RT: 12.734 min Scan# 1640

Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Tgt Ion:216 Resp: 175527




Ion Ratio Lower Upper


216 100

214 77.5 62.2 93.2

179 22.9 15.8 23.8

108 18.9 12.6 18.8#

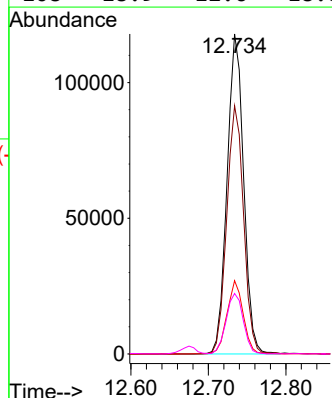



#40

Hexachlorocyclopentadiene

Concen: 17.248 ng/ul

RT: 12.675 min Scan# 1630

Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:237 Resp: 90290

Ion Ratio Lower Upper

237 100

235 62.1 50.3 75.5

272 13.2 11.1 16.7

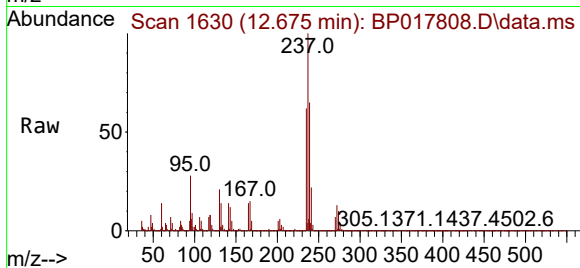

#41

2,4,6-Trichlorophenol

Concen: 20.201 ng/ul

RT: 12.998 min Scan# 1685

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:196 Resp: 110463


Ion Ratio Lower Upper

196 100

198 96.3 74.7 112.1

200 30.4 23.7 35.5



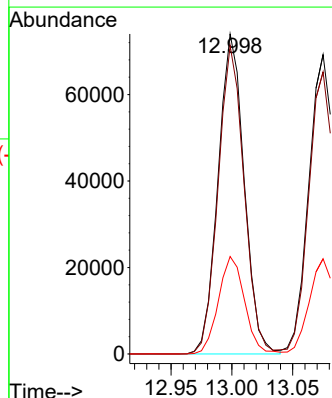
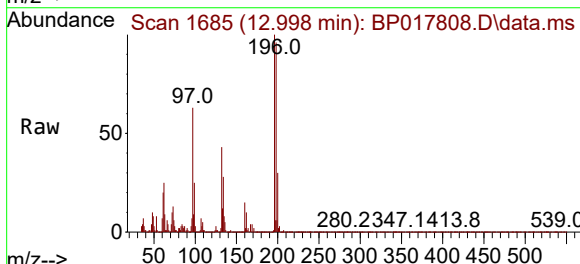




#42
2,4,5-Trichlorophenol
Concen: 20.230 ng/ul
RT: 13.075 min Scan# 1698
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:196 Resp: 114365
Ion Ratio Lower Upper
196 100
198 94.3 76.0 114.0
200 31.8 24.3 36.5



#43
1,1'-Biphenyl
Concen: 20.579 ng/ul
RT: 13.404 min Scan# 1754
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:154 Resp: 417467
Ion Ratio Lower Upper
154 100
153 39.7 32.6 49.0
76 12.6 9.8 14.8









#44
2-Chloronaphthalene
Concen: 20.325 ng/ul
RT: 13.451 min Scan# 1762
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:162 Resp: 333309
Ion Ratio Lower Upper
162 100
164 33.4 25.9 38.9
127 40.8 29.9 44.9

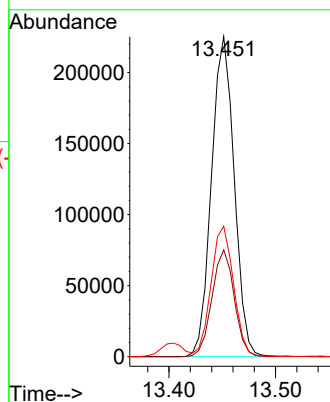

#45
2-Nitroaniline
Concen: 24.683 ng/ul
RT: 13.698 min Scan# 1804
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion: 65 Resp: 91982
Ion Ratio Lower Upper
65 100
92 70.6 56.2 84.4
138 96.4 85.9 128.9


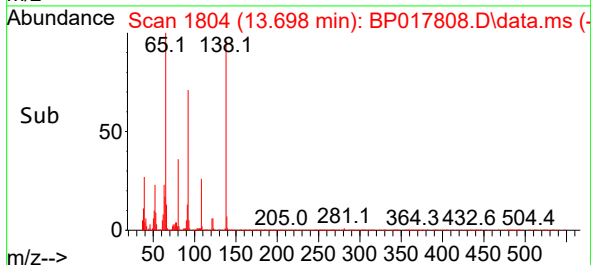
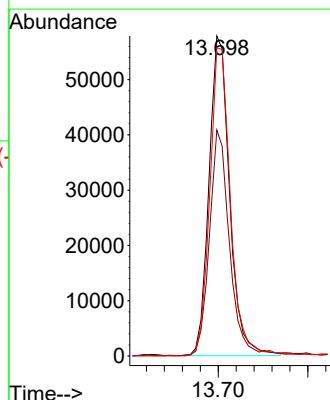
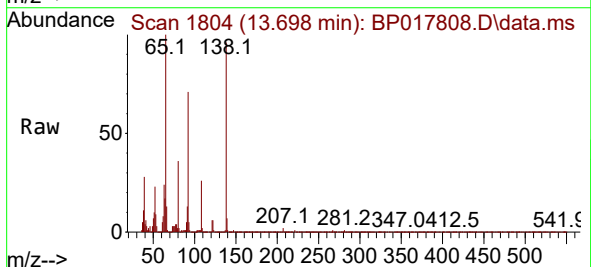


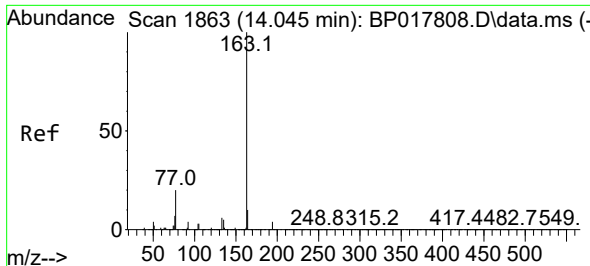

#47
Dimethylphthalate
Concen: 19.939 ng/ul
RT: 14.045 min Scan# 1863
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:163 Resp: 406190
Ion Ratio Lower Upper
163 100
194 4.1 3.4 5.0
164 10.0 8.2 12.4

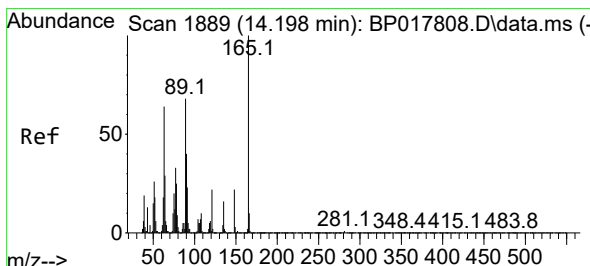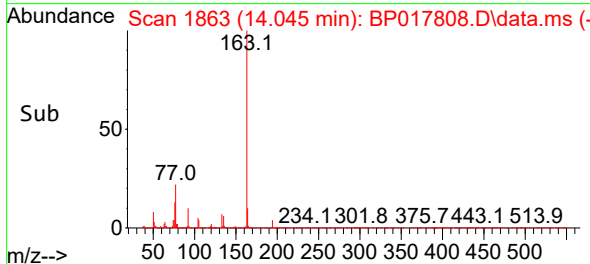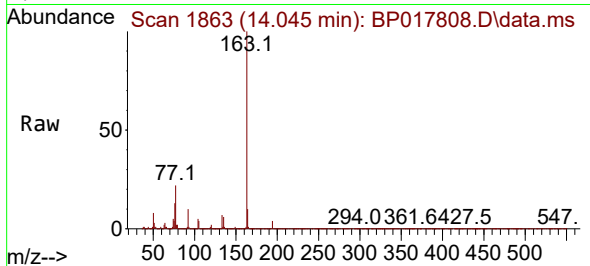

#48
2,6-Dinitrotoluene
Concen: 20.616 ng/ul
RT: 14.198 min Scan# 1889
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:165 Resp: 77305
Ion Ratio Lower Upper
165 100
89 68.0 48.0 72.0
121 22.4 16.6 24.8


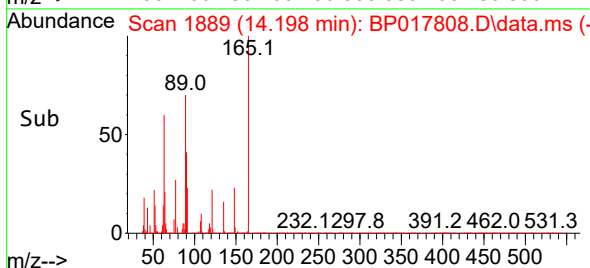
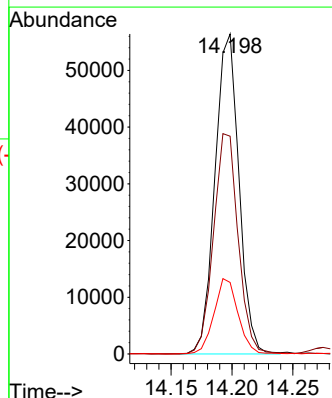
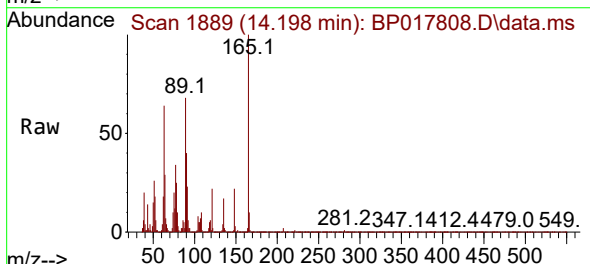




#50
Acenaphthylene
Concen: 20.642 ng/ul
RT: 14.304 min Scan# 1907
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:152 Resp: 533015
Ion Ratio Lower Upper
152 100
151 19.4 15.9 23.9
153 12.8 10.8 16.2

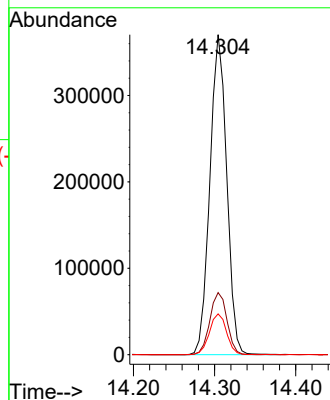

#51
3-Nitroaniline
Concen: 20.634 ng/ul
RT: 14.540 min Scan# 1947
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:138 Resp: 73586
Ion Ratio Lower Upper
138 100
108 11.3 9.3 13.9
92 125.0 95.2 142.8

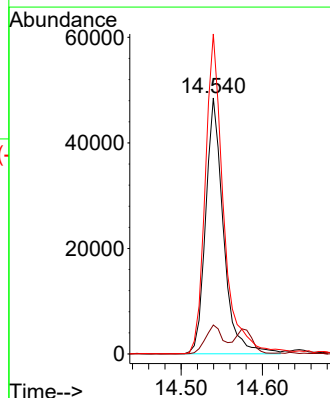



#52

Acenaphthene

Concen: 19.962 ng/ul

RT: 14.645 min Scan# 1965

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:153 Resp: 348446

Ion Ratio Lower Upper

153 100

152 49.1 37.6 56.4

154 88.2 70.0 105.0

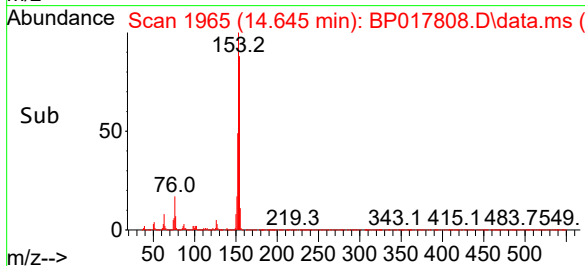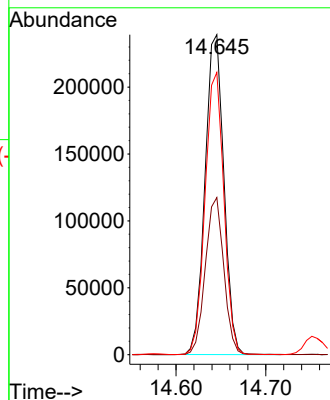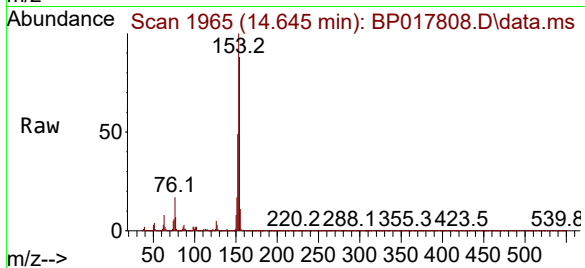

#53

2,4-Dinitrophenol

Concen: 15.785 ng/ul

RT: 14.751 min Scan# 1983

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:184 Resp: 33226


Ion Ratio Lower Upper

184 100

63 72.3 50.6 76.0

154 69.5 47.9 71.9



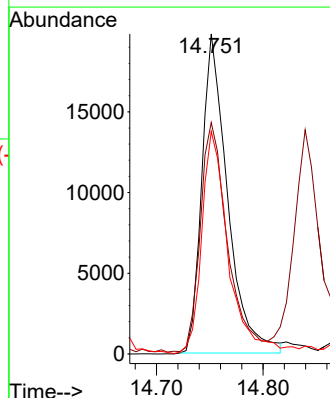
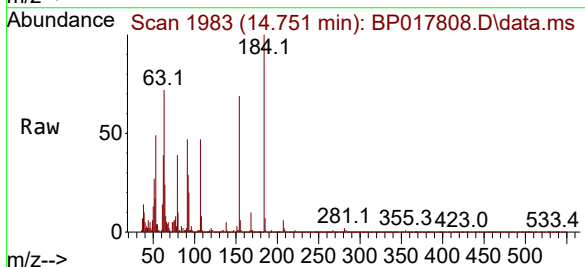




#55
4-Nitrophenol
Concen: 21.509 ng/ul
RT: 14.840 min Scan# 1998
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:109 Resp: 67061
Ion Ratio Lower Upper
109 100
139 104.4 92.9 139.3
65 118.5 94.5 141.7

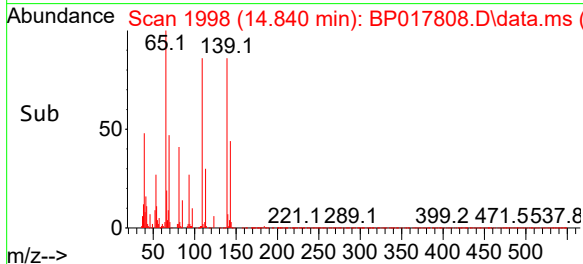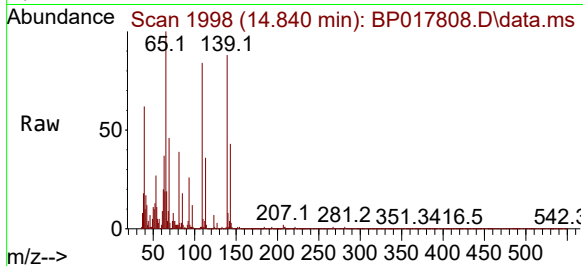

#56
Dibenzofuran
Concen: 19.613 ng/ul
RT: 14.981 min Scan# 2022
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:168 Resp: 480675
Ion Ratio Lower Upper
168 100
139 39.7 28.6 43.0


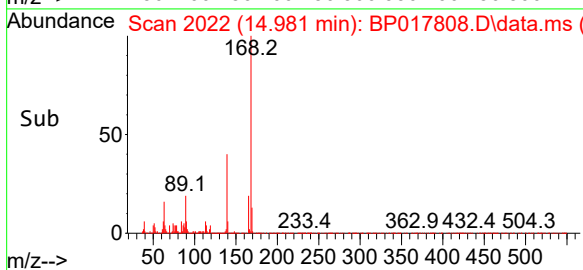

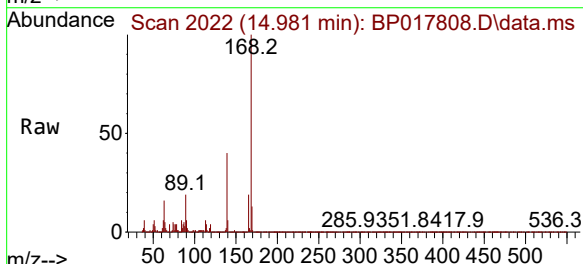




#57
2,4-Dinitrotoluene
Concen: 20.490 ng/ul
RT: 14.987 min Scan# 2023
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:165 Resp: 113396
Ion Ratio Lower Upper
165 100
63 70.7 51.1 76.7
182 2.9 2.7 4.1



#58
2,3,4,6-Tetrachlorophenol
Concen: 18.227 ng/ul
RT: 15.204 min Scan# 2060
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:232 Resp: 91442
Ion Ratio Lower Upper
232 100
131 52.7 32.9 49.3#
130 3.2 1.8 2.8#
166 38.3 23.3 34.9#









#59
Diethylphthalate
Concen: 20.726 ng/ul
RT: 15.404 min Scan# 2094
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:149 Resp: 407674
Ion Ratio Lower Upper
149 100
177 21.3 18.0 27.0
150 12.9 10.2 15.4



#61
Fluorene
Concen: 19.359 ng/ul
RT: 15.640 min Scan# 2134
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:166 Resp: 389726
Ion Ratio Lower Upper
166 100
165 98.9 77.4 116.0
167 13.1 10.9 16.3









#62
4-Chlorophenyl-phenylether
Concen: 18.394 ng/ul
RT: 15.634 min Scan# 2133
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:204 Resp: 196820
Ion Ratio Lower Upper
204 100
206 33.2 26.2 39.4
141 61.2 42.9 64.3



#63
4-Nitroaniline
Concen: 21.211 ng/ul
RT: 15.716 min Scan# 2147
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:138 Resp: 68226
Ion Ratio Lower Upper
138 100
92 59.4 43.0 64.6
108 109.5 82.7 124.1









#66
4,6-Dinitro-2-methylphenol
Concen: 18.703 ng/ul
RT: 15.745 min Scan# 2152
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:198 Resp: 66167
Ion Ratio Lower Upper
198 100
182 4.6 3.9 5.9
77 31.0 19.8 29.8#

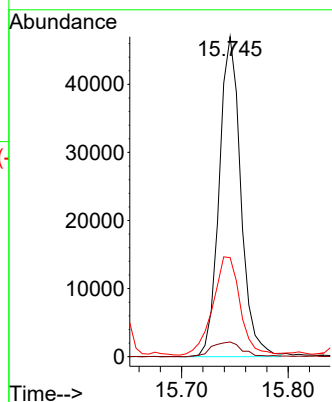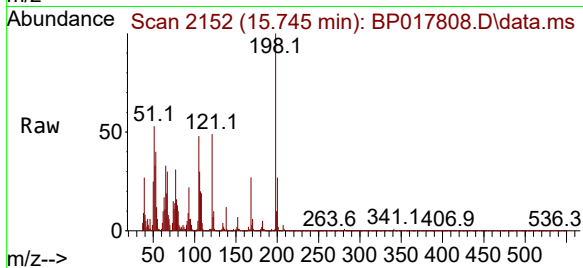

#67
N-Nitrosodiphenylamine
Concen: 21.311 ng/ul
RT: 15.863 min Scan# 2172
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:169 Resp: 323744
Ion Ratio Lower Upper
169 100
168 66.9 53.7 80.5
167 36.2 29.4 44.0




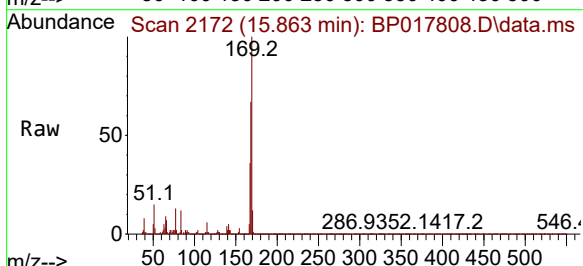




#68
4-Bromophenyl-phenylether
Concen: 18.981 ng/ul
RT: 16.539 min Scan# 2287
Delta R.T. -0.012 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:248 Resp: 111365
Ion Ratio Lower Upper
248 100
250 97.4 76.8 115.2
141 89.9 52.4 78.6#

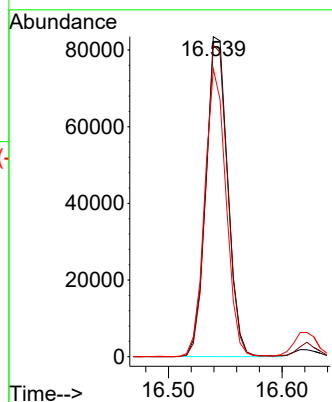

#69
Hexachlorobenzene
Concen: 17.876 ng/ul
RT: 16.622 min Scan# 2301
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:284 Resp: 120405
Ion Ratio Lower Upper
284 100
142 43.7 27.6 41.4#
249 35.4 24.5 36.7





#70

Atrazine

Concen: 19.833 ng/ul

RT: 16.828 min Scan# 2336

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:200 Resp: 110735

Ion Ratio Lower Upper

200 100

173 24.2 19.8 29.6

215 46.2 38.5 57.7



#71

Pentachlorophenol

Concen: 16.730 ng/ul

RT: 16.998 min Scan# 2365

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:266 Resp: 67748


Ion Ratio Lower Upper

266 100

264 71.2 49.4 74.2

268 64.7 50.3 75.5

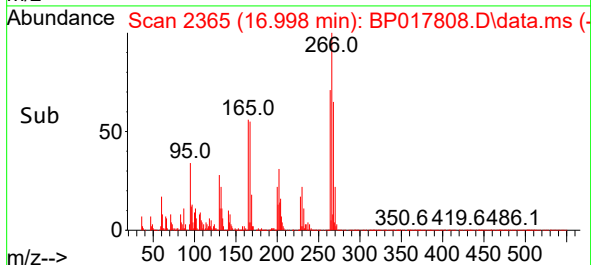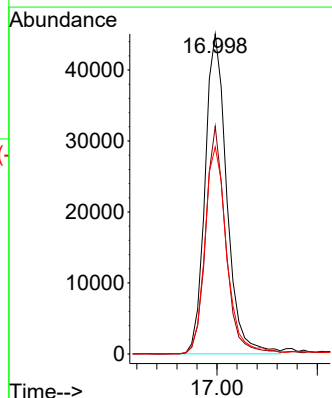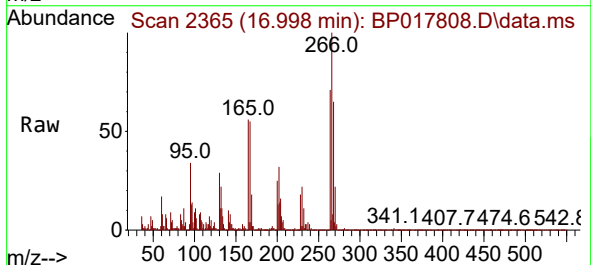



#72

Phenanthrene

Concen: 20.408 ng/ul

RT: 17.410 min Scan# 2435

Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:178 Resp: 599460

Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.2

176 19.2 15.3 22.9

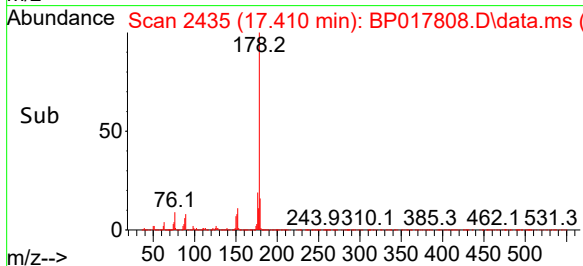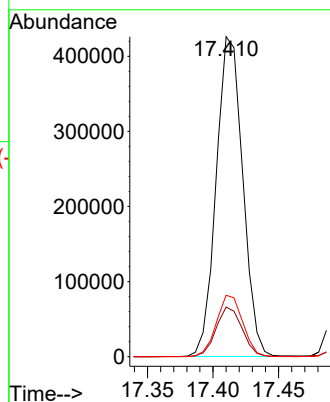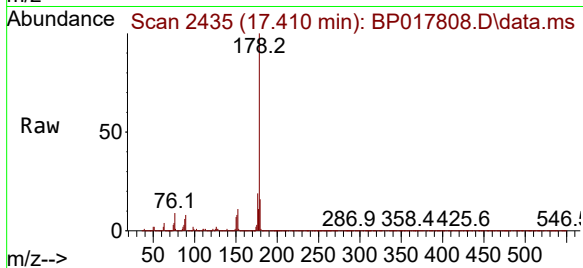

#74

Anthracene

Concen: 20.372 ng/ul

RT: 17.504 min Scan# 2451

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:178 Resp: 606104


Ion Ratio Lower Upper

178 100

179 15.6 12.0 18.0

176 19.3 14.8 22.2

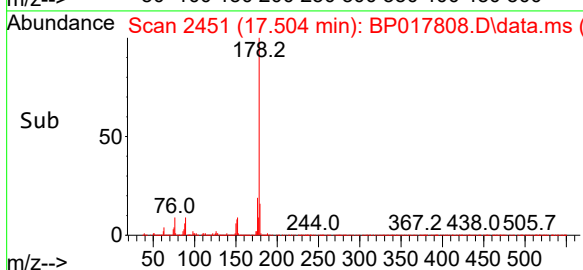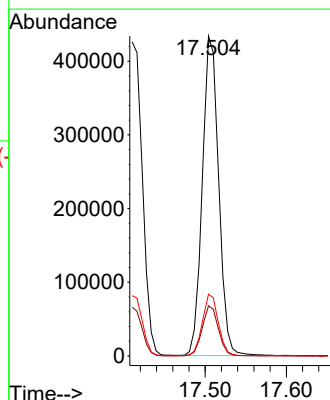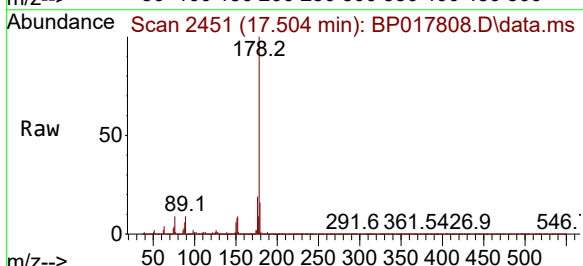



#75

1,2,3,4-Tetrachlorobenzene

Concen: 20.457 ng/uL

RT: 13.357 min Scan# 1746

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:216 Resp: 172119

Ion Ratio Lower Upper

216 100

214 81.5 60.7 91.1

218 46.8 38.2 57.4



#76

Pentachlorobenzene

Concen: 19.299 ng/uL

RT: 14.875 min Scan# 2004

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:250 Resp: 157370


Ion Ratio Lower Upper

250 100

248 63.0 50.2 75.4

252 64.9 49.6 74.4

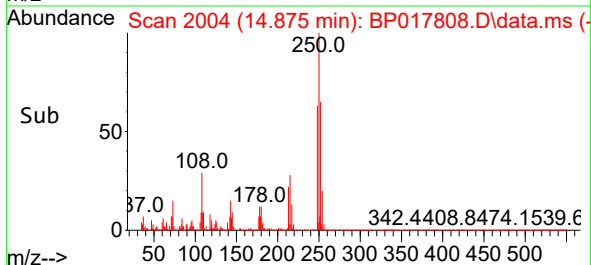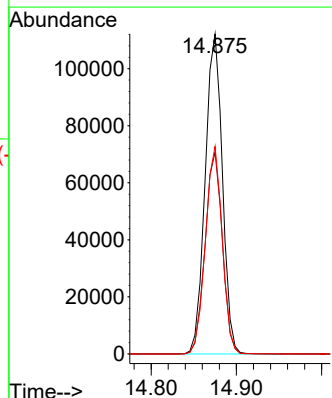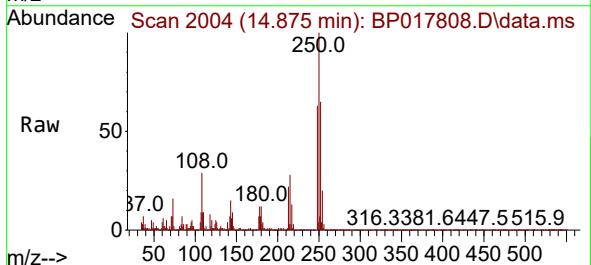



#77

Carbazole

Concen: 20.577 ng/ul

RT: 17.804 min Scan# 2502

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:167 Resp: 517393

Ion Ratio Lower Upper

167 100

166 21.1 16.7 25.1

139 13.1 9.8 14.6



#78

Di-n-butylphthalate

Concen: 22.756 ng/ul

RT: 18.310 min Scan# 2588

Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:149 Resp: 664311


Ion Ratio Lower Upper

149 100

150 9.3 7.2 10.8

104 5.9 4.3 6.5

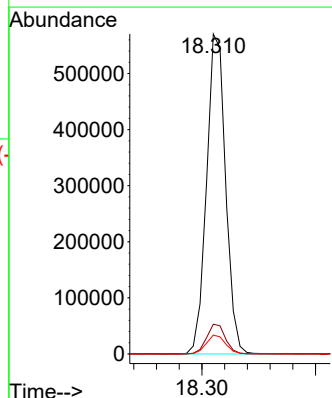



#80

Fluoranthene

Concen: 20.864 ng/ul

RT: 19.398 min Scan# 2773

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:202 Resp: 682914

Ion Ratio Lower Upper

202 100

101 9.6 7.1 10.7

100 7.5 5.7 8.5

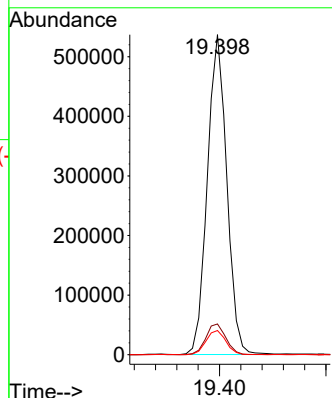

#82

Pyrene

Concen: 20.549 ng/ul

RT: 19.757 min Scan# 2834

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:202 Resp: 712581


Ion Ratio Lower Upper

202 100

101 12.0 8.3 12.5

100 9.7 7.4 11.0





#83

Butylbenzylphthalate

Concen: 24.626 ng/ul

RT: 20.627 min Scan# 2982

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:149 Resp: 293717

Ion Ratio Lower Upper

149 100

91 76.2 58.8 88.2

206 19.5 17.5 26.3

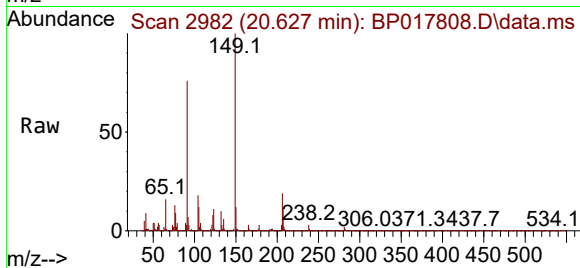

#84

3,3'-Dichlorobenzidine

Concen: 18.548 ng/ul

RT: 21.439 min Scan# 3120

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:252 Resp: 190420


Ion Ratio Lower Upper

252 100

254 63.4 51.8 77.8

126 11.9 7.8 11.6#

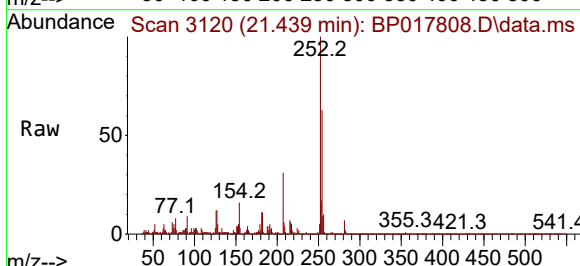



#85

Benzo(a)anthracene

Concen: 19.896 ng/ul

RT: 21.492 min Scan# 3129

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:228 Resp: 687298

Ion Ratio Lower Upper

228 100

229 19.7 15.6 23.4

226 28.0 21.1 31.7

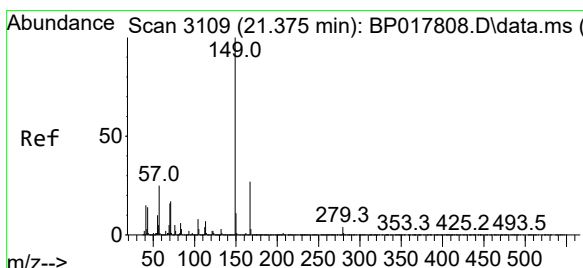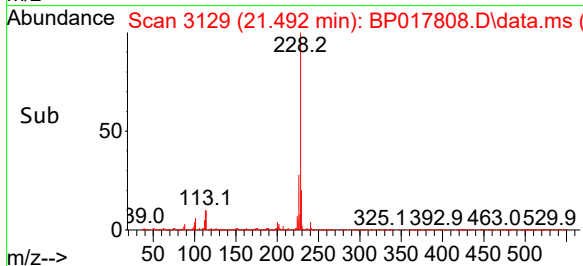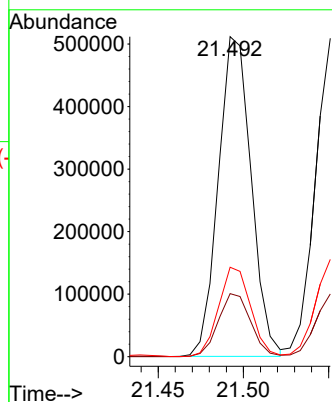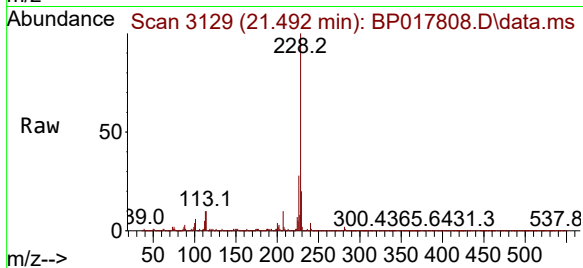

#86

Bis(2-ethylhexyl)phthalate

Concen: 24.701 ng/ul

RT: 21.375 min Scan# 3109

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:149 Resp: 411255


Ion Ratio Lower Upper

149 100

167 26.6 21.6 32.4

279 3.5 3.6 5.4#

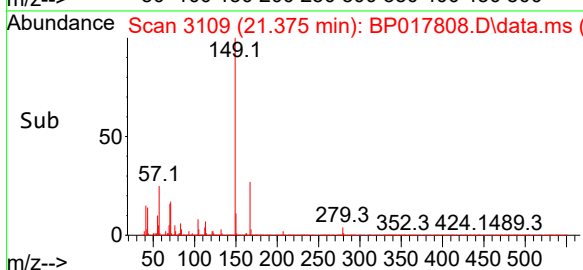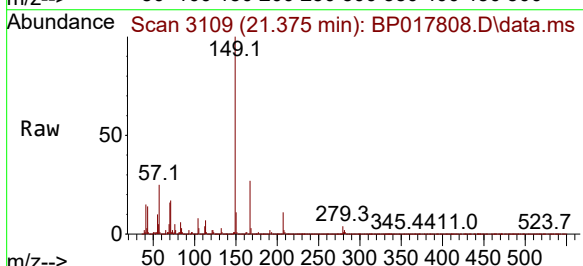



#87

Chrysene

Concen: 19.970 ng/ul

RT: 21.551 min Scan# 3139

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:228 Resp: 652352

Ion Ratio Lower Upper

228 100

226 30.5 24.0 36.0

229 19.7 15.5 23.3

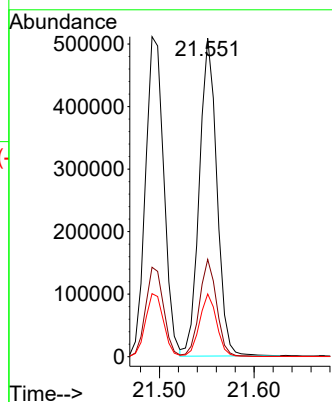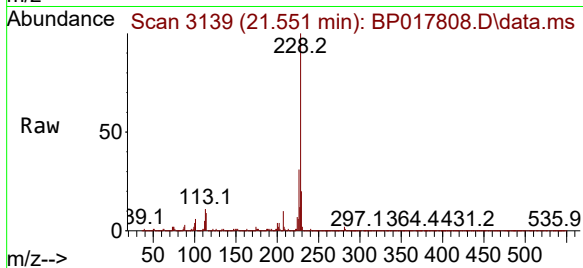

#89

Di-n-octyl phthalate

Concen: 24.331 ng/ul




RT: 22.351 min Scan# 3275


Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Tgt Ion:149 Resp: 694622


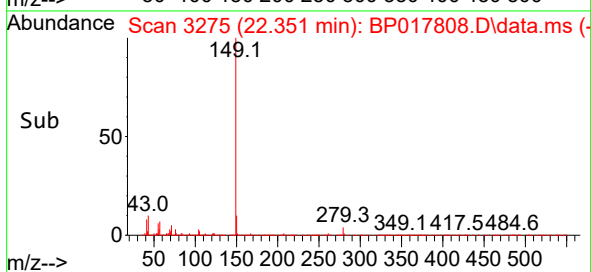
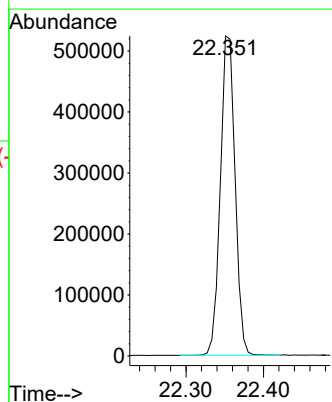
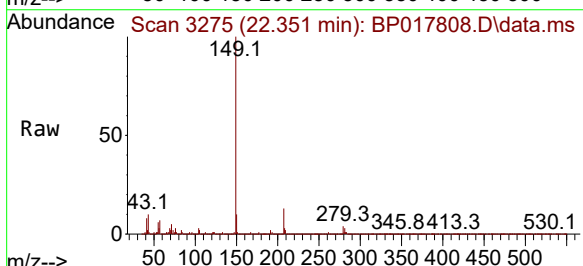




#90
Benzo(b)fluoranthene
Concen: 20.887 ng/ul
RT: 23.269 min Scan# 3431
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07




Instrument :
BNA_P
ClientSampleId :
SSTD020795


Tgt Ion:252 Resp: 640696
Ion Ratio Lower Upper
252 100
253 21.1 17.4 26.0
125 10.0 7.1 10.7



#91
Benzo(k)fluoranthene
Concen: 19.982 ng/ul
RT: 23.321 min Scan# 3440
Delta R.T. -0.006 min
Lab File: BP017808.D
Acq: 25 Oct 2023 18:07

Tgt Ion:252 Resp: 621195
Ion Ratio Lower Upper
252 100
253 22.0 17.5 26.3
125 10.4 7.0 10.6





#93

Benzo(a)pyrene

Concen: 20.173 ng/ul

RT: 23.945 min Scan# 3546

Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:252 Resp: 580918

Ion Ratio Lower Upper

252 100

253 22.2 17.4 26.2

125 11.3 7.8 11.6



#94

Indeno(1,2,3-cd)pyrene

Concen: 19.429 ng/ul

RT: 26.774 min Scan# 4027

Delta R.T. -0.006 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07




Tgt Ion:276 Resp: 666798


Ion Ratio Lower Upper

276 100

138 21.6 15.6 23.4

277 24.6 19.4 29.2





#95

Dibenzo(a,h)anthracene

Concen: 19.254 ng/ul

RT: 26.798 min Scan# 4031

Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Instrument :

BNA_P

ClientSampleId :

SSTD020795





Tgt Ion:278 Resp: 551345

Ion Ratio Lower Upper

278 100

139 15.9 11.4 17.2

279 23.6 18.8 28.2



#96

Benzo(g,h,i)perylene

Concen: 19.410 ng/ul

RT: 27.615 min Scan# 4170

Delta R.T. -0.012 min

Lab File: BP017808.D

Acq: 25 Oct 2023 18:07

Tgt Ion:276 Resp: 536732

Ion Ratio Lower Upper

276 100

138 21.8 15.0 22.6

277 23.6 18.5 27.7

