

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
 Data File : BP017809.D
 Acq On : 25 Oct 2023 18:42
 Operator : MA/JU
 Sample : PB156616BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK616

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017809.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	29	32	43	rVB3	13409	26473	0.71%	0.083%
2	3.711	102	106	126	rBV	125192	313124	8.42%	0.980%
3	4.005	153	156	166	rVB7	7660	15196	0.41%	0.048%
4	6.852	634	640	643	rBV6	3961	7977	0.21%	0.025%
5	7.046	667	673	687	rBV	198352	371154	9.98%	1.161%
6	7.234	697	705	714	rBV	168100	289712	7.79%	0.907%
7	7.405	728	734	748	rBV	226955	392118	10.54%	1.227%
8	7.881	809	815	824	rBV	547748	880329	23.67%	2.755%
9	8.604	930	938	955	rBV	341294	628153	16.89%	1.966%
10	9.093	1014	1021	1036	rBV	243449	421498	11.33%	1.319%
11	9.722	1127	1128	1134	rBV6	2159	4492	0.12%	0.014%
12	9.804	1134	1142	1154	rVV	234963	410569	11.04%	1.285%
13	10.334	1226	1232	1246	rBV	377094	690514	18.57%	2.161%
14	10.710	1289	1296	1312	rBV	668749	1128315	30.34%	3.531%
15	10.887	1319	1326	1346	rBV	511037	949923	25.54%	2.973%
16	11.740	1466	1471	1479	rVB10	4659	11309	0.30%	0.035%
17	12.316	1563	1569	1577	rVB7	5975	10621	0.29%	0.033%
18	12.763	1640	1645	1649	rBV7	4653	8661	0.23%	0.027%
19	13.416	1750	1756	1765	rBV3	12831	22755	0.61%	0.071%
20	13.687	1798	1802	1804	rBV5	3417	3983	0.11%	0.012%
21	13.998	1848	1855	1866	rBV	1532429	2105529	56.62%	6.589%
22	14.275	1895	1902	1914	rBV	1423355	2057806	55.34%	6.440%
23	14.422	1925	1927	1933	rVB7	3074	5992	0.16%	0.019%
24	14.581	1947	1954	1963	rBV	895958	1326166	35.66%	4.150%
25	14.822	1989	1995	2017	rBV	473044	949434	25.53%	2.971%
26	15.581	2117	2124	2135	rBV	1944246	2795696	75.18%	8.749%
27	15.728	2143	2149	2162	rBV	684305	1014266	27.28%	3.174%
28	15.828	2162	2166	2170	rVB6	10068	16999	0.46%	0.053%
29	17.028	2366	2370	2374	rBV7	4693	7032	0.19%	0.022%
30	17.163	2389	2393	2398	rBB7	3047	4733	0.13%	0.015%
31	17.369	2421	2428	2437	rBV	1096913	1487099	39.99%	4.654%
32	17.469	2437	2445	2459	rBV2	2338558	3282159	88.26%	10.271%
33	18.222	2569	2573	2581	rBV5	19176	40902	1.10%	0.128%
34	19.298	2752	2756	2762	rBV5	26627	36385	0.98%	0.114%
35	19.369	2765	2768	2772	rVB	22692	28887	0.78%	0.090%
36	19.474	2783	2786	2789	rBV3	12228	15227	0.41%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
Data File : BP017809.D
Acq On : 25 Oct 2023 18:42
Operator : MA/JU
Sample : PB156616BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK616

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	19.727	2823	2829	2839	rBV	2796655	3718661	100.00%	11.637%
38	21.510	3127	3132	3145	rBV	1074679	1569665	42.21%	4.912%
39	23.898	3530	3538	3546	rBV2	1712955	3484686	93.71%	10.905%
40	24.062	3559	3566	3576	rVB	678398	1421330	38.22%	4.448%




Sum of corrected areas: 31955530

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
Data File : BP017809.D
Acq On : 25 Oct 2023 18:42
Operator : MA/JU
Sample : PB156616BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

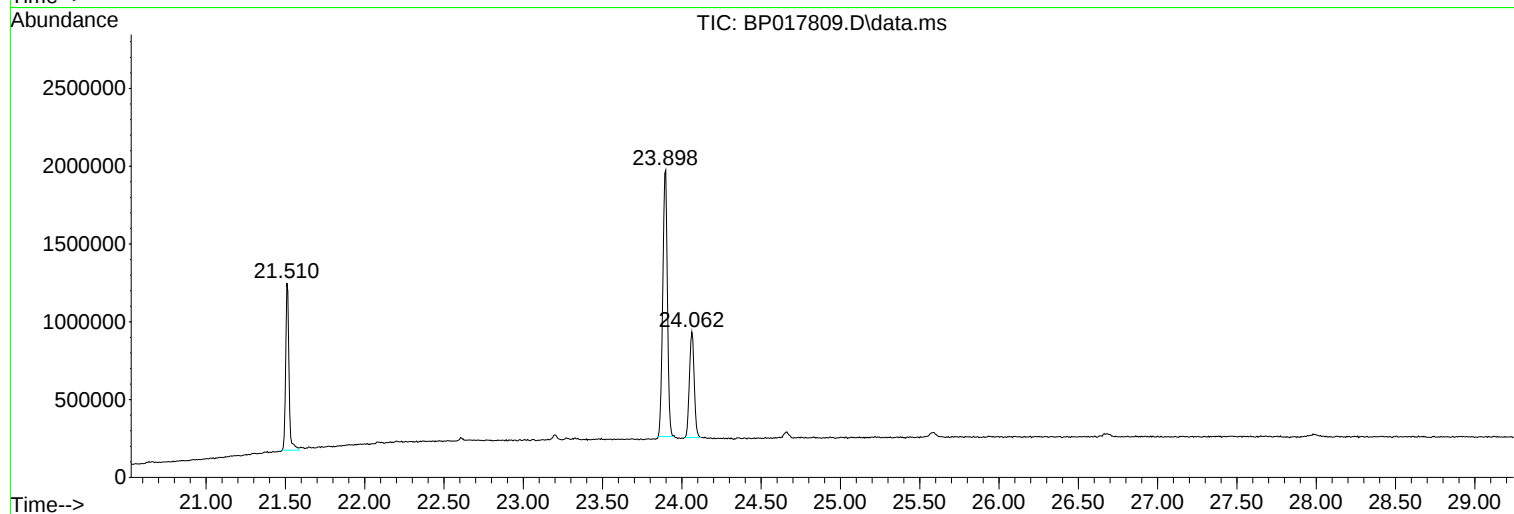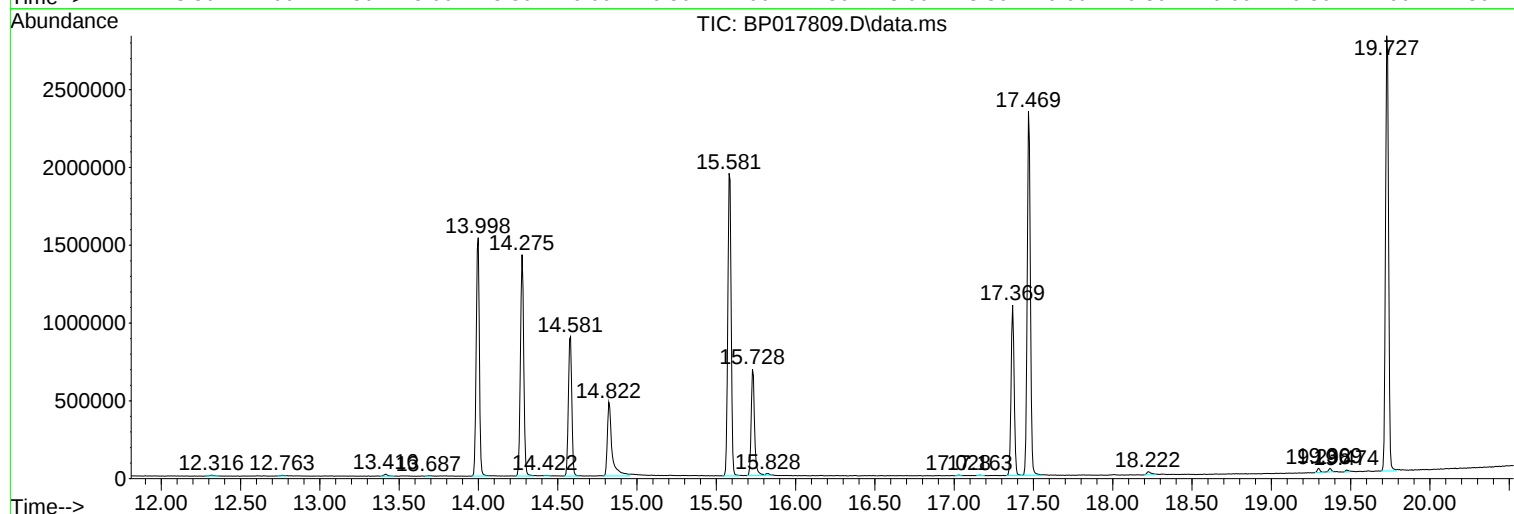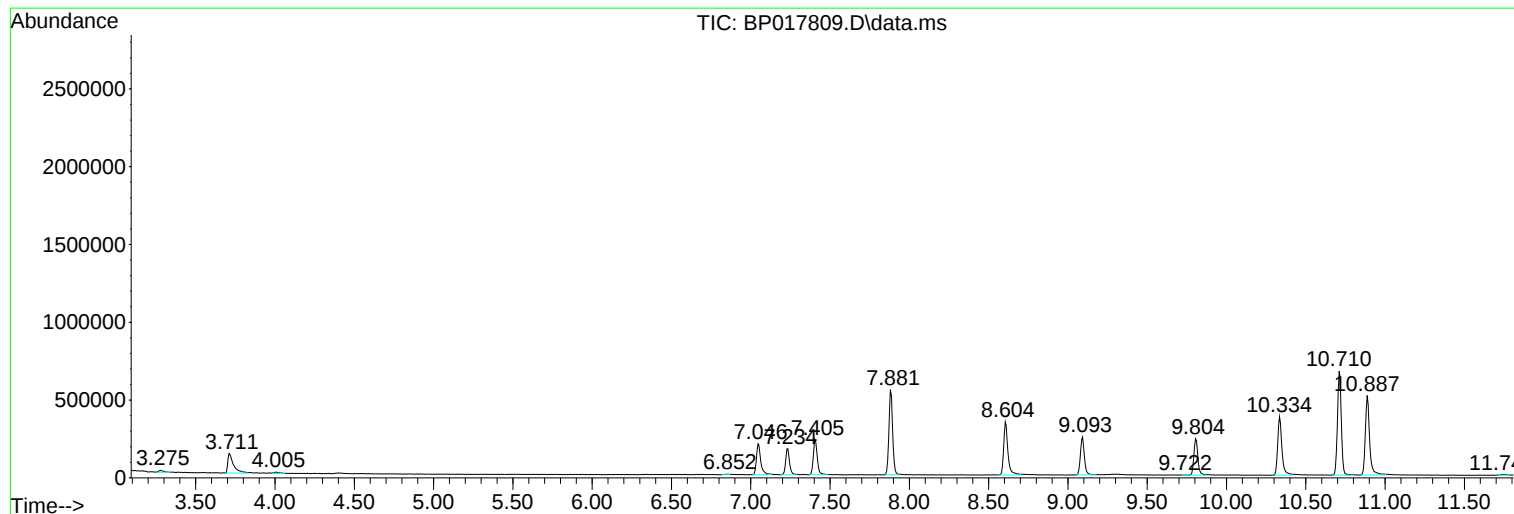

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
Data File : BP017809.D
Acq On : 25 Oct 2023 18:42
Operator : MA/JU
Sample : PB156616BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
Data File : BP017809.D
Acq On : 25 Oct 2023 18:42
Operator : MA/JU
Sample : PB156616BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
