

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
 Data File : BP017821.D
 Acq On : 26 Oct 2023 02:04
 Operator : MA/JU
 Sample : 04927-06DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.722	104	108	120	rBV	37144	92399	4.61%	0.582%
2	3.999	153	155	160	rVB6	6495	9310	0.46%	0.059%
3	4.399	220	223	227	rBV4	3150	4525	0.23%	0.029%
4	4.740	279	281	284	rVB4	3480	2481	0.12%	0.016%
5	4.934	309	314	324	rVV	14058	27928	1.39%	0.176%
6	5.004	324	326	330	rVB5	3619	3787	0.19%	0.024%
7	5.128	345	347	352	rVB6	3489	3920	0.20%	0.025%
8	5.163	352	353	358	rBV5	2635	3352	0.17%	0.021%
9	5.528	411	415	418	rBV6	3425	6325	0.32%	0.040%
10	5.787	458	459	464	rVB5	2664	2707	0.13%	0.017%
11	6.334	549	552	554	rBV4	2720	2786	0.14%	0.018%
12	6.475	574	576	580	rBV5	2767	3999	0.20%	0.025%
13	6.651	604	606	611	rVB6	2568	2602	0.13%	0.016%
14	6.840	636	638	642	rVB5	2282	3385	0.17%	0.021%
15	7.046	668	673	687	rBV	103135	206072	10.27%	1.299%
16	7.228	698	704	716	rBV	103723	178699	8.91%	1.126%
17	7.404	728	734	743	rBV	133117	225541	11.24%	1.422%
18	7.628	770	772	775	rVB3	2876	2740	0.14%	0.017%
19	7.881	808	815	829	rBV	564331	914388	45.58%	5.763%
20	8.016	835	838	839	rBV3	3127	2181	0.11%	0.014%
21	8.051	839	844	848	rBV8	3051	7492	0.37%	0.047%
22	8.610	932	939	953	rBV	102097	219409	10.94%	1.383%
23	8.875	981	984	985	rVB3	2504	2211	0.11%	0.014%
24	8.892	985	987	990	rVV4	1868	2590	0.13%	0.016%
25	8.928	991	993	999	rVV7	2369	3919	0.20%	0.025%
26	8.975	999	1001	1004	rVB4	1948	2401	0.12%	0.015%
27	9.092	1014	1021	1033	rBV	115470	212205	10.58%	1.338%
28	9.216	1040	1042	1044	rBV3	2522	2865	0.14%	0.018%
29	9.275	1048	1052	1053	rVV4	2195	2380	0.12%	0.015%
30	9.481	1086	1087	1096	rVV9	2131	4497	0.22%	0.028%
31	9.551	1096	1099	1102	rVB5	1816	2463	0.12%	0.016%
32	9.804	1136	1142	1153	rBV	94847	172412	8.60%	1.087%
33	10.339	1226	1233	1245	rBV	111600	244723	12.20%	1.542%
34	10.604	1277	1278	1283	rBV5	2519	3374	0.17%	0.021%
35	10.710	1288	1296	1309	rBV	700442	1172409	58.45%	7.390%
36	10.892	1319	1327	1341	rBV	71553	166246	8.29%	1.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
 Data File : BP017821.D
 Acq On : 26 Oct 2023 02:04
 Operator : MA/JU
 Sample : 04927-06DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	11.028	1347	1350	1352	rVB4	2373	2668	0.13%	0.017%
38	11.081	1357	1359	1363	rVB5	1753	2388	0.12%	0.015%
39	11.263	1385	1390	1392	rBV6	1715	2347	0.12%	0.015%
40	11.328	1399	1401	1404	rVB4	2667	2721	0.14%	0.017%
41	11.428	1412	1418	1419	rBV6	1994	2656	0.13%	0.017%
42	11.492	1427	1429	1433	rBV5	2586	4457	0.22%	0.028%
43	11.528	1433	1435	1439	rVV5	2527	3447	0.17%	0.022%
44	11.739	1466	1471	1475	rBV7	5322	11385	0.57%	0.072%
45	11.775	1475	1477	1483	rVB7	4486	5259	0.26%	0.033%
46	12.322	1562	1570	1573	rBV9	2687	5057	0.25%	0.032%
47	12.545	1605	1608	1609	rBV3	2107	2285	0.11%	0.014%
48	12.610	1615	1619	1620	rBV3	3022	3880	0.19%	0.024%
49	12.763	1638	1645	1653	rBV10	5451	14995	0.75%	0.095%
50	12.969	1678	1680	1682	rBV3	2129	2285	0.11%	0.014%
51	13.039	1686	1692	1694	rBV7	2348	4204	0.21%	0.026%
52	13.410	1751	1755	1763	rVB	28169	46848	2.34%	0.295%
53	13.692	1798	1803	1809	rVB8	5257	10480	0.52%	0.066%
54	13.739	1809	1811	1814	rBV4	2010	2773	0.14%	0.017%
55	13.792	1817	1820	1824	rVV5	3477	5742	0.29%	0.036%
56	13.839	1826	1828	1830	rVB3	2744	2470	0.12%	0.016%
57	13.992	1848	1854	1862	rBV	259337	356548	17.77%	2.247%
58	14.275	1896	1902	1910	rBV	270357	408998	20.39%	2.578%
59	14.427	1920	1928	1930	rBV9	3238	5520	0.28%	0.035%
60	14.575	1946	1953	1963	rBV	950315	1390016	69.30%	8.761%
61	14.716	1974	1977	1979	rBV4	1811	2213	0.11%	0.014%
62	14.863	1995	2002	2016	rBV7	13781	52930	2.64%	0.334%
63	14.980	2019	2022	2024	rVB4	3440	3976	0.20%	0.025%
64	15.198	2056	2059	2060	rBV3	2799	2696	0.13%	0.017%
65	15.327	2077	2081	2084	rVV6	2217	3345	0.17%	0.021%
66	15.375	2084	2089	2092	rVB6	3472	5524	0.28%	0.035%
67	15.486	2105	2108	2112	rBV4	2141	3510	0.17%	0.022%
68	15.539	2112	2117	2118	rBV5	2881	3839	0.19%	0.024%
69	15.580	2118	2124	2133	rVV	361919	525394	26.19%	3.312%
70	15.651	2133	2136	2143	rVB9	4007	8566	0.43%	0.054%
71	15.733	2145	2150	2161	rBV2	50444	90371	4.51%	0.570%
72	15.833	2164	2167	2172	rVB7	3936	5993	0.30%	0.038%
73	16.433	2264	2269	2272	rBV7	2468	3251	0.16%	0.020%
74	16.463	2272	2274	2278	rBV5	2948	4335	0.22%	0.027%
75	16.569	2289	2292	2295	rBV5	1991	3175	0.16%	0.020%
76	16.669	2307	2309	2314	rVB6	2303	3472	0.17%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
 Data File : BP017821.D
 Acq On : 26 Oct 2023 02:04
 Operator : MA/JU
 Sample : 04927-06DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCD10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

77	17.004	2363	2366	2367	rBV3	2759	2642	0.13%	0.017%
78	17.157	2388	2392	2394	rVB5	3668	4127	0.21%	0.026%
79	17.221	2401	2403	2407	rBV5	4947	5235	0.26%	0.033%
80	17.292	2411	2415	2419	rBV7	2881	4802	0.24%	0.030%
81	17.369	2421	2428	2439	rBV	1083603	1531431	76.35%	9.653%
82	17.469	2439	2445	2452	rBV2	344871	498323	24.84%	3.141%
83	17.710	2484	2486	2488	rBV3	3433	3700	0.18%	0.023%
84	17.998	2532	2535	2538	rVB5	3123	4374	0.22%	0.028%
85	18.080	2545	2549	2551	rBV5	3663	4189	0.21%	0.026%
86	18.110	2551	2554	2556	rVB4	3924	4389	0.22%	0.028%
87	18.163	2560	2563	2566	rBV4	9401	12766	0.64%	0.080%
88	18.216	2568	2572	2582	rVV2	91497	143670	7.16%	0.906%
89	18.310	2586	2588	2591	rVB2	6544	7015	0.35%	0.044%
90	18.768	2664	2666	2671	rVB6	7207	7371	0.37%	0.046%
91	18.927	2691	2693	2699	rBV7	6576	6596	0.33%	0.042%
92	19.368	2763	2768	2772	rBV2	32250	40414	2.01%	0.255%
93	19.463	2780	2784	2795	rBV2	67266	114590	5.71%	0.722%
94	19.604	2804	2808	2813	rBV	89429	99129	4.94%	0.625%
95	19.727	2824	2829	2836	rBV	473861	634199	31.62%	3.997%
96	20.639	2980	2984	2986	rBV2	67296	95847	4.78%	0.604%
97	21.368	3104	3108	3113	rBV	1868496	2005916	100.00%	12.643%
98	21.509	3127	3132	3137	rBV	1169535	1510292	75.29%	9.519%
99	23.886	3531	3536	3543	rVB	292260	582077	29.02%	3.669%
100	24.062	3559	3566	3578	rVB	730217	1599611	79.74%	10.082%




Sum of corrected areas: 15865447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
Data File : BP017821.D
Acq On : 26 Oct 2023 02:04
Operator : MA/JU
Sample : 04927-06DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD10DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

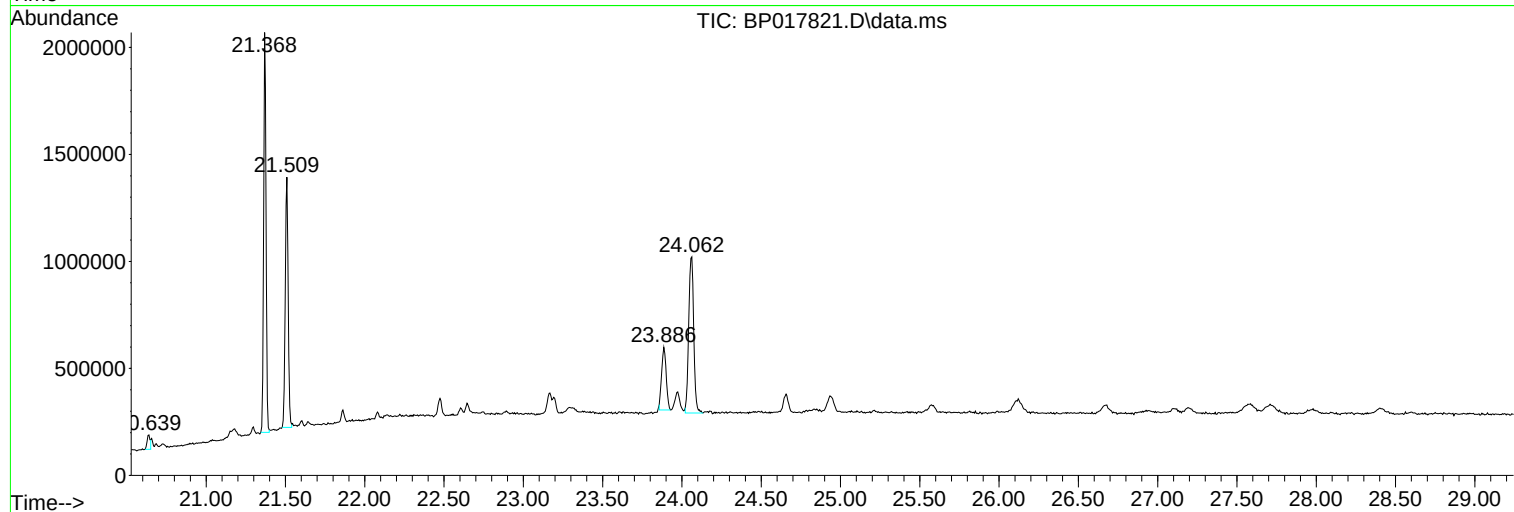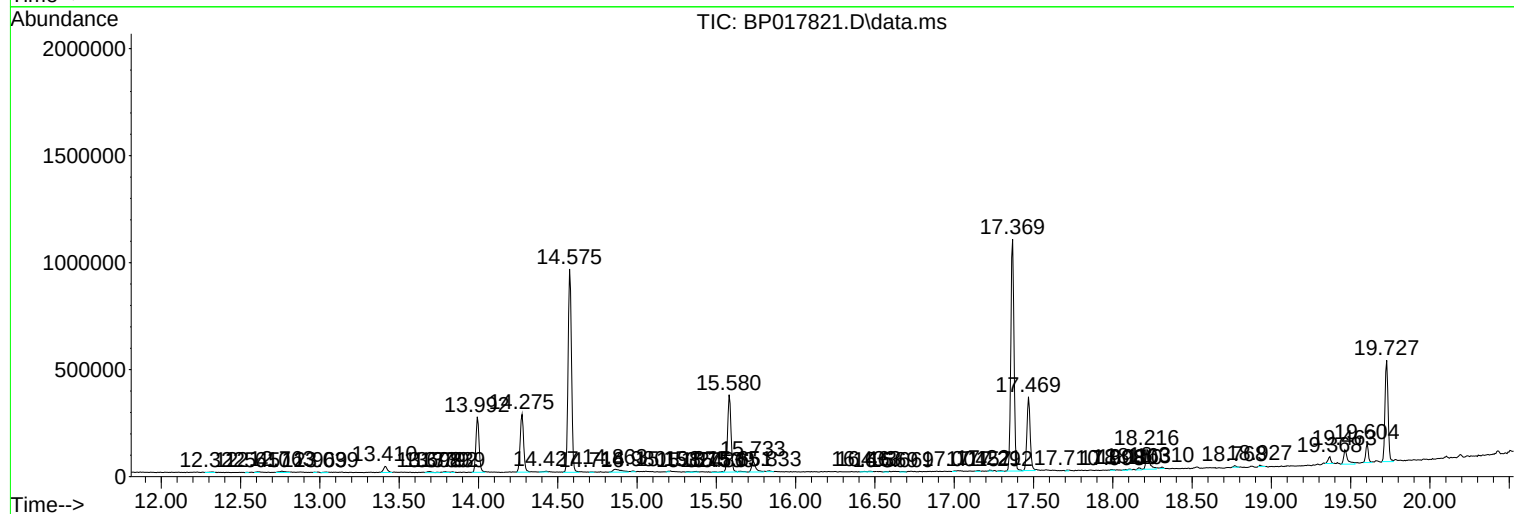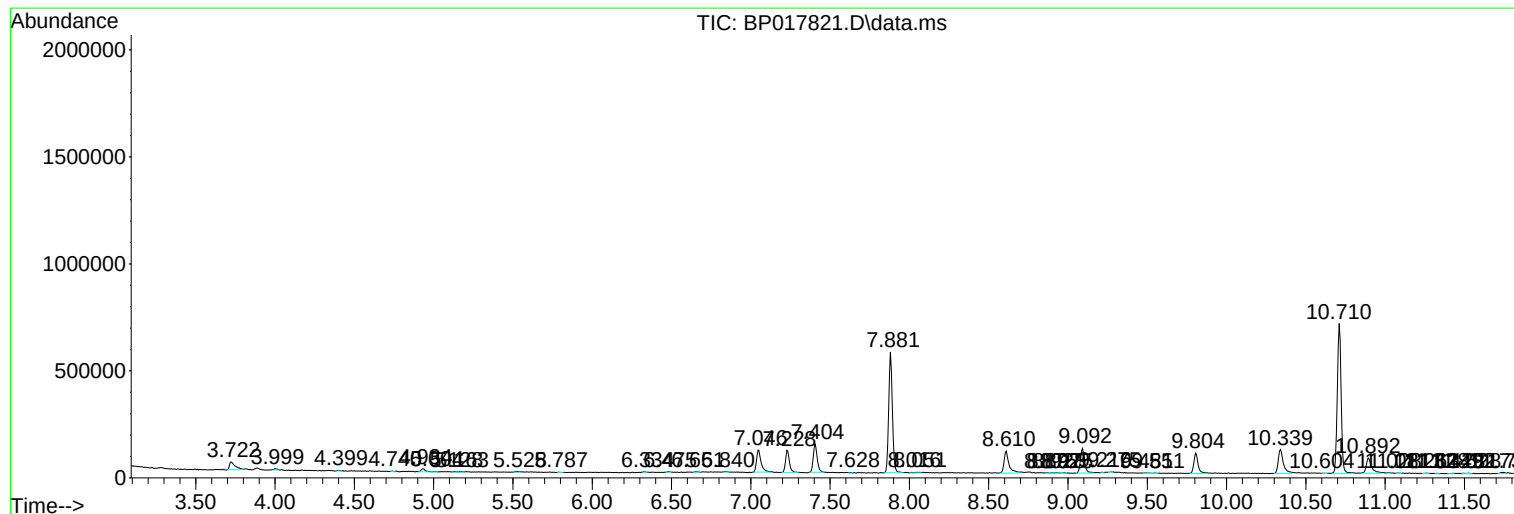

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
Data File : BP017821.D
Acq On : 26 Oct 2023 02:04
Operator : MA/JU
Sample : 04927-06DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD10DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102523\
Data File : BP017821.D
Acq On : 26 Oct 2023 02:04
Operator : MA/JU
Sample : 04927-06DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCD10DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc