

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007753.D
 Acq On : 28 Oct 2021 15:03
 Operator : CG/JU
 Sample : M4282-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY99

Quant Time: Oct 28 16:06:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	170447	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	716144	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	492961	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1081970	20.000	ng/ul	0.00
79) Chrysene-d12	21.410	240	1159633	20.000	ng/ul	-0.01
88) Perylene-d12	23.857	264	1216267	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	17002	4.531	ng/uL	0.00
4) Pyridine-d5	3.793	84	44274	3.902	ng/ul	0.01
7) Phenol-d5	7.093	99	144915	11.194	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	266558	37.085	ng/ul	0.00
11) 2-Chlorophenol-d4	7.464	132	314034	31.188	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	218854	21.589	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	195850	40.131	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	213299	40.016	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.352	165	370903	34.186	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	458220	31.941	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	1370818	41.052	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	1615441	39.471	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	64285	10.503	ng/ul	0.00
60) Fluorene-d10	15.563	176	1207400	42.891	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	196494	33.952	ng/ul	0.00
73) Anthracene-d10	17.422	188	2133692	47.986	ng/ul	0.00
81) Pyrene-d10	19.657	212	2560119	47.419	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	2684727	44.934	ng/ul	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.399	88	227080	54.132	ng/uL	89
59) Diethylphthalate	15.393	149	32808	1.014	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007753.D
Acq On : 28 Oct 2021 15:03
Operator : CG/JU
Sample : M4282-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY99

Quant Time: Oct 28 16:06:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 27 15:37:43 2021
Response via : Initial Calibration




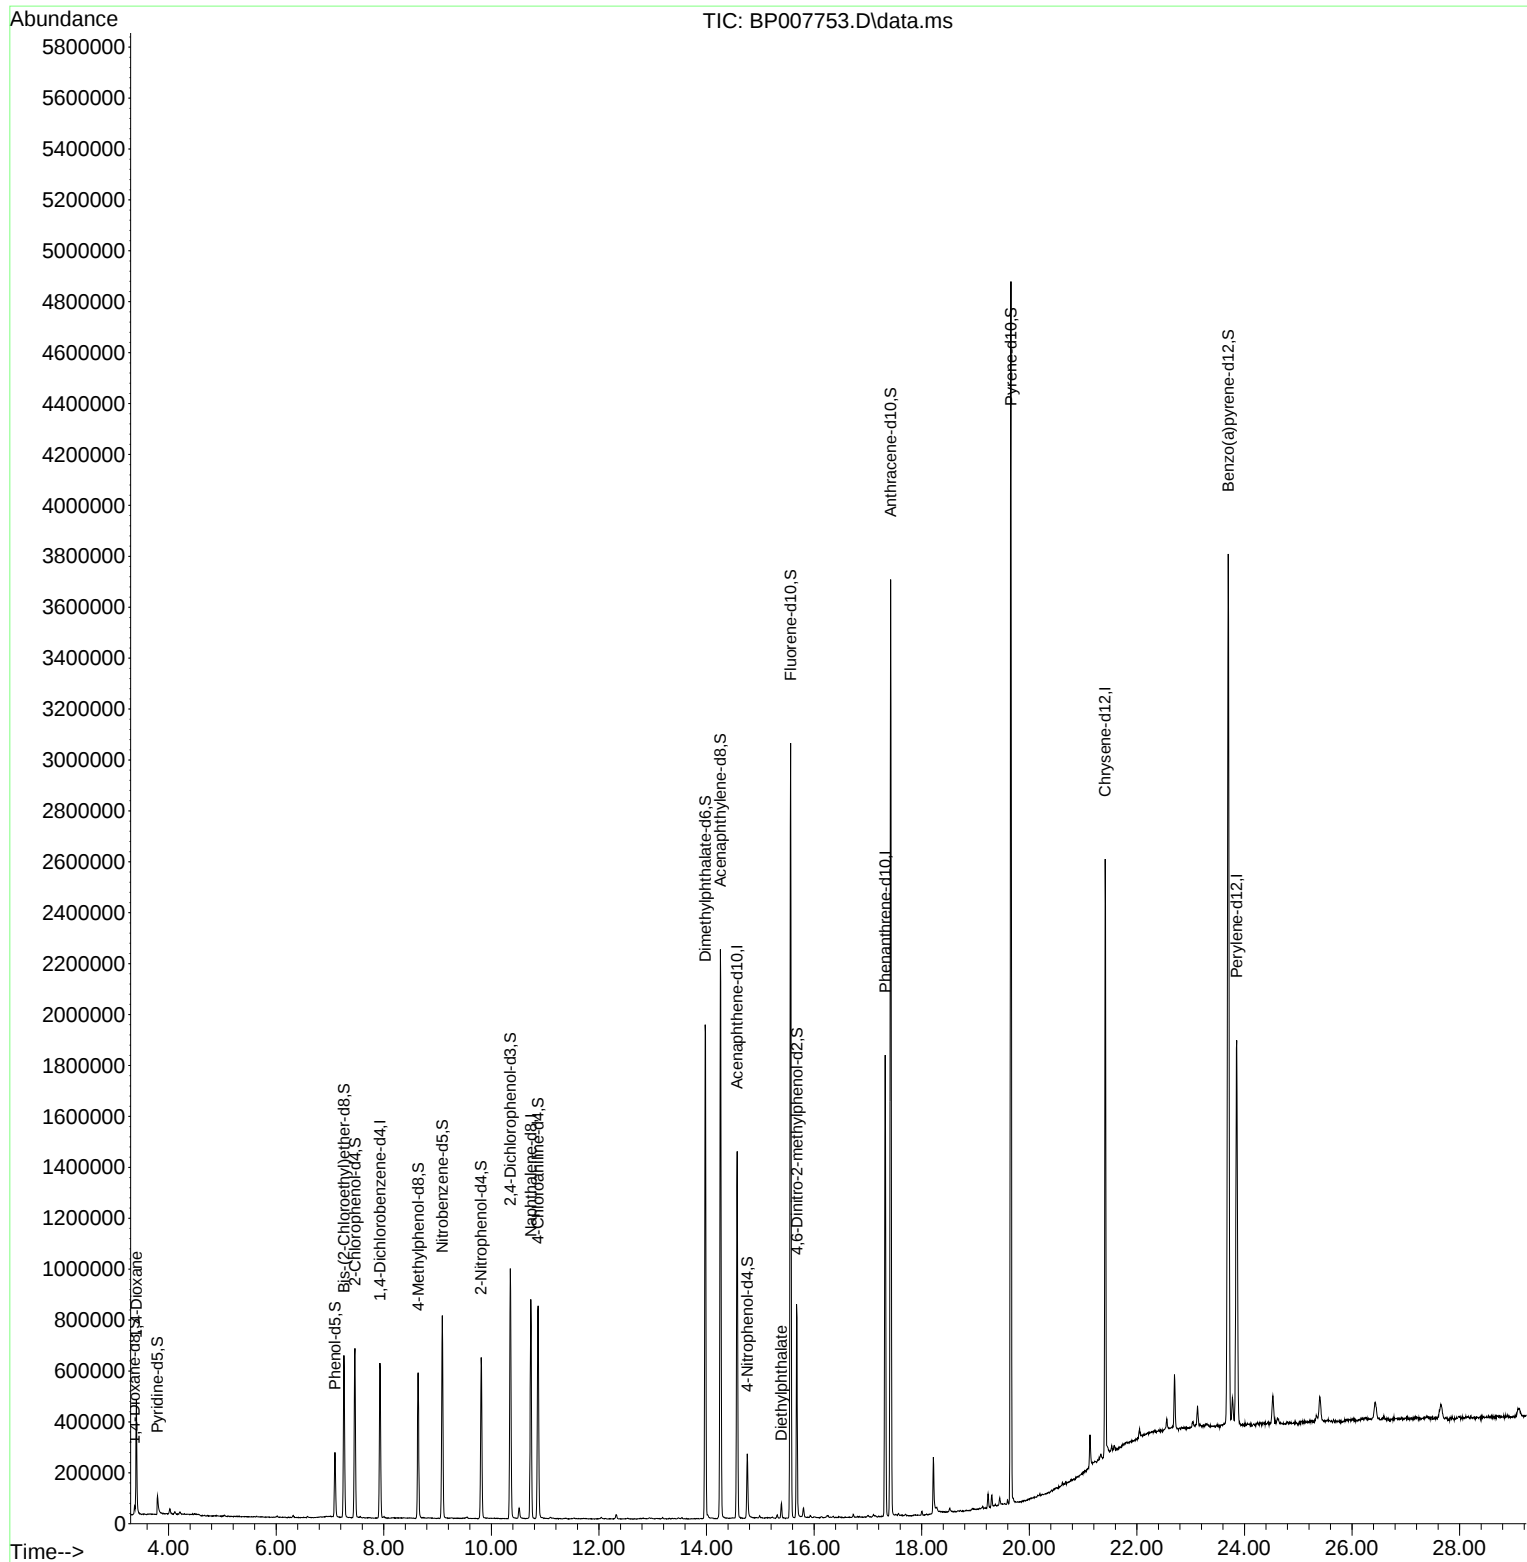


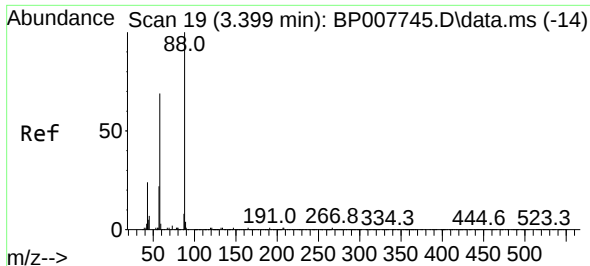

#2
1,4-Dioxane
Concen: 54.132 ng/uL
RT: 3.399 min Scan# 19
Delta R.T. 0.000 min
Lab File: BP007753.D
Acq: 28 Oct 2021 15:03

Instrument :
BNA_P
ClientSampleId :
BFY99

Tgt Ion: 88	Resp: 227080
Ion Ratio	Lower Upper
88	100
43	25.5 24.2 36.2
58	67.9 62.5 93.7

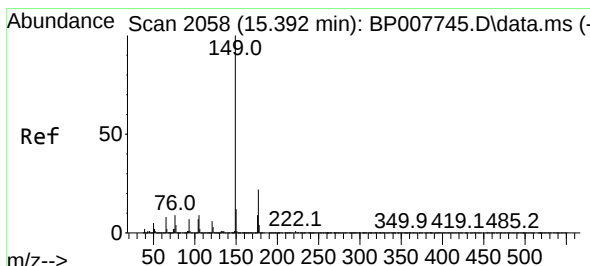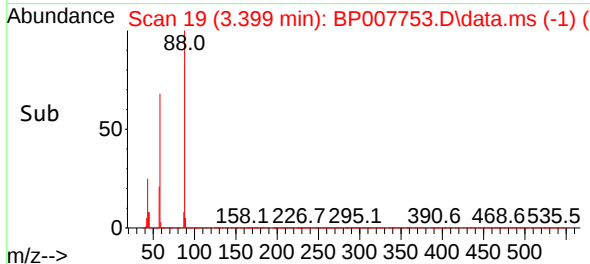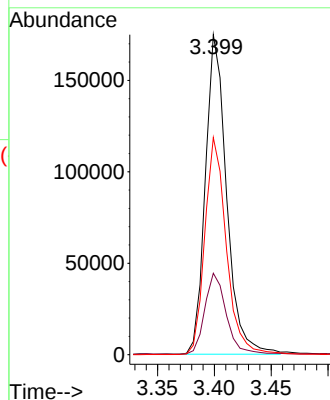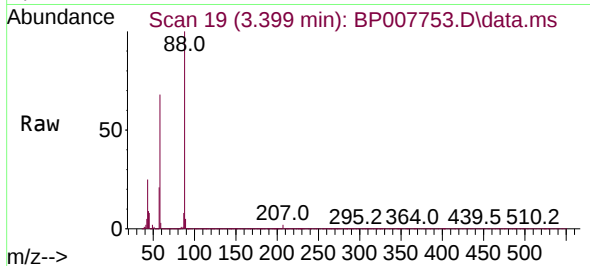

#59
Diethylphthalate
Concen: 1.014 ng/uL
RT: 15.393 min Scan# 2058
Delta R.T. -0.005 min
Lab File: BP007753.D
Acq: 28 Oct 2021 15:03

Tgt Ion: 149	Resp: 32808
Ion Ratio	Lower Upper
149	100
177	25.5 17.4 26.2
150	12.8 10.0 15.0

