

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007760.D
 Acq On : 28 Oct 2021 19:01
 Operator : CG/JU
 Sample : M4282-19
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFYA0

Quant Time: Oct 29 00:57:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	132183	20.000	ng/u1	0.00
20) Naphthalene-d8	10.734	136	550622	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.563	164	372449	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.322	188	817622	20.000	ng/u1	0.00
79) Chrysene-d12	21.410	240	936872	20.000	ng/u1	-0.01
88) Perylene-d12	23.851	264	999787	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	18695	6.425	ng/uL	0.00
4) Pyridine-d5	3.793	84	38578	4.384	ng/u1	0.01
7) Phenol-d5	7.093	99	151494	15.089	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	261856	46.976	ng/u1	0.00
11) 2-Chlorophenol-d4	7.464	132	317101	40.609	ng/u1	0.00
15) 4-Methylphenol-d8	8.634	113	225839	28.727	ng/u1	-0.01
21) Nitrobenzene-d5	9.087	128	185433	49.418	ng/u1	0.00
24) 2-Nitrophenol-d4	9.810	143	202850	49.496	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.352	165	358991	43.034	ng/u1	0.00
31) 4-Chloroaniline-d4	10.863	131	389038	35.271	ng/u1	0.00
46) Dimethylphthalate-d6	13.975	166	1290049	51.134	ng/u1	0.00
49) Acenaphthylene-d8	14.257	160	1497947	48.443	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	66013	14.274	ng/u1	0.00
60) Fluorene-d10	15.563	176	1117575	52.546	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	187160	42.794	ng/u1	0.00
73) Anthracene-d10	17.422	188	1987211	59.141	ng/u1	0.00
81) Pyrene-d10	19.657	212	2407209	55.189	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.692	264	2692758	54.827	ng/u1	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.399	88	302483	92.980	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007760.D
Acq On : 28 Oct 2021 19:01
Operator : CG/JU
Sample : M4282-19
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFYA0

Quant Time: Oct 29 00:57:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 27 15:37:43 2021
Response via : Initial Calibration

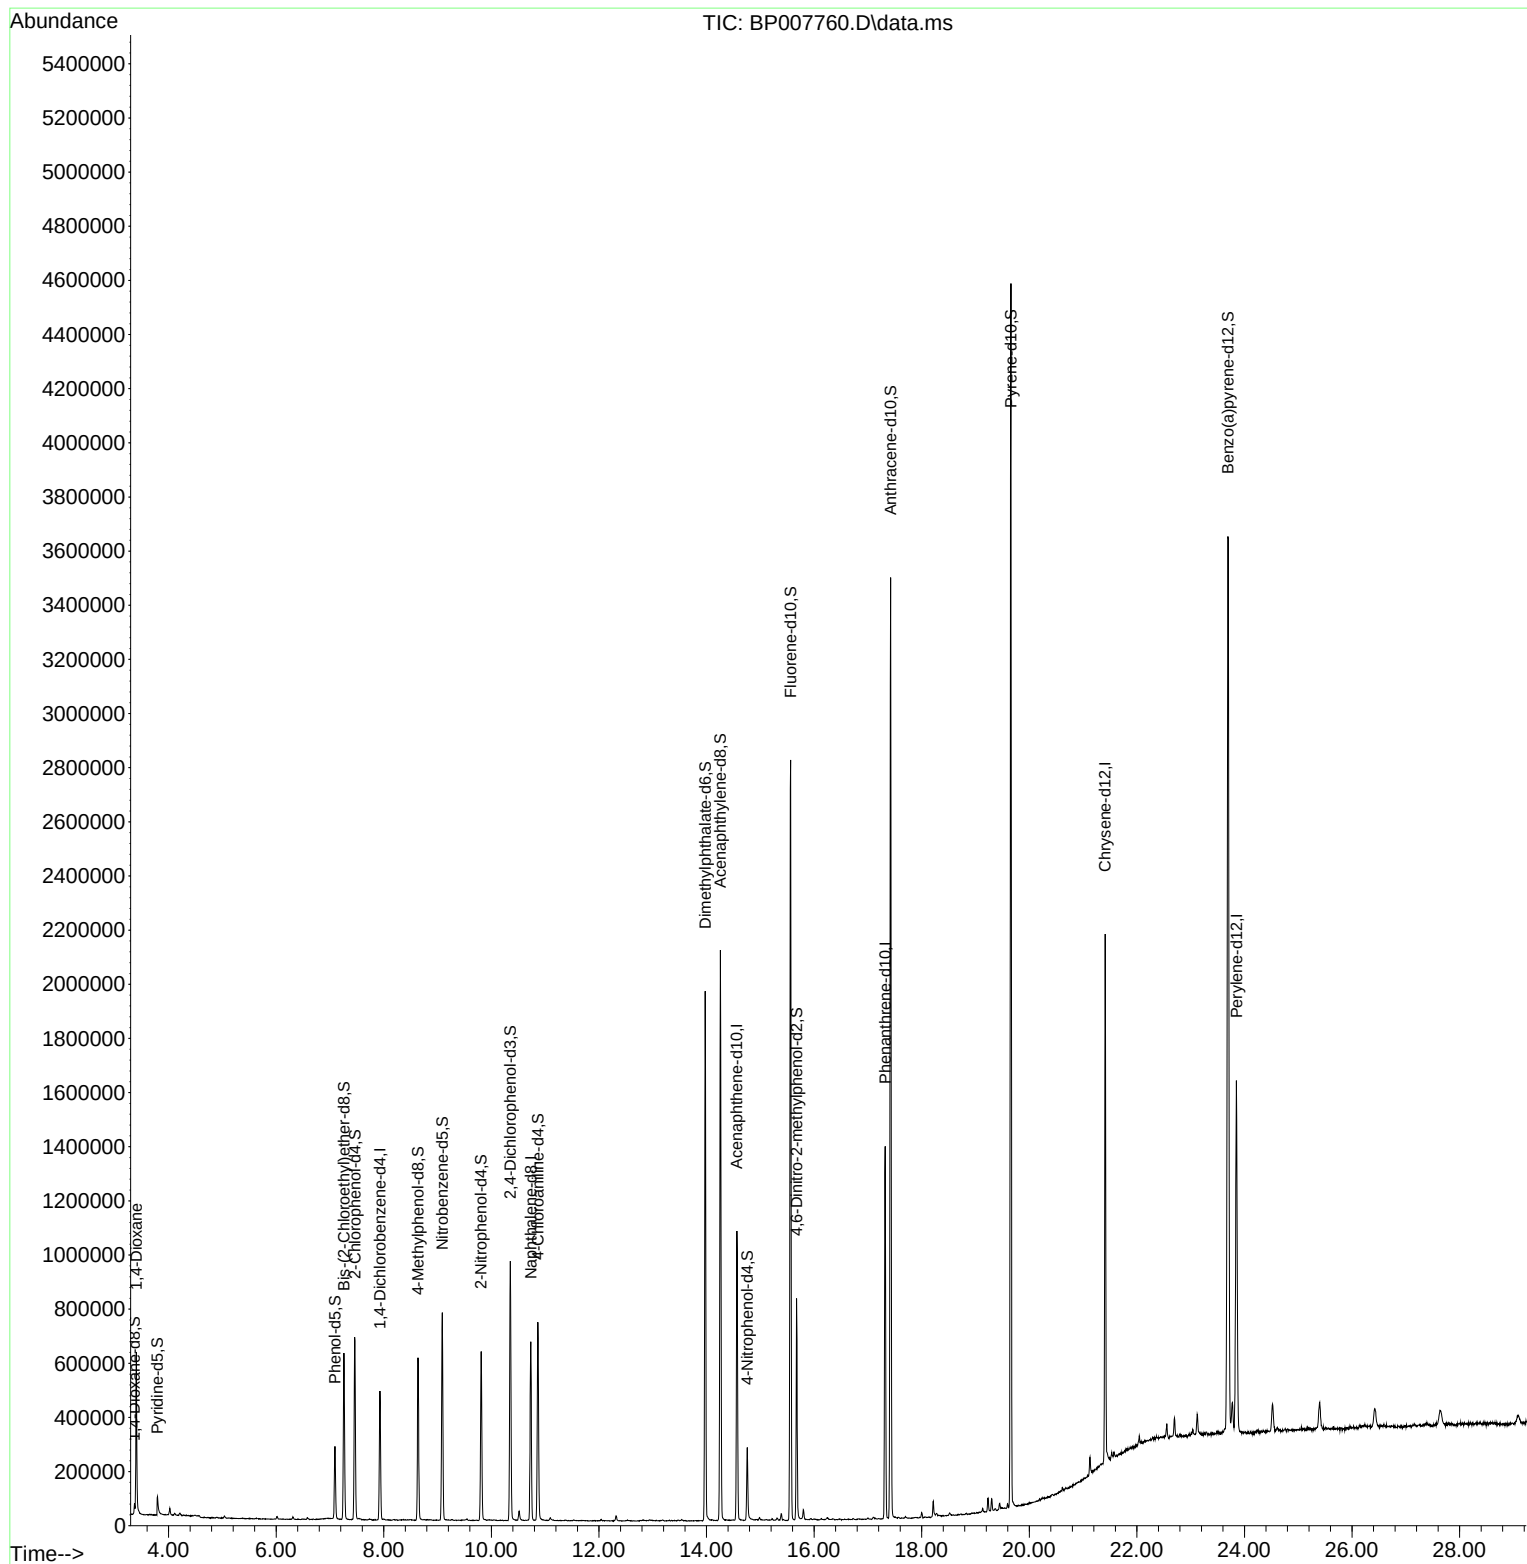

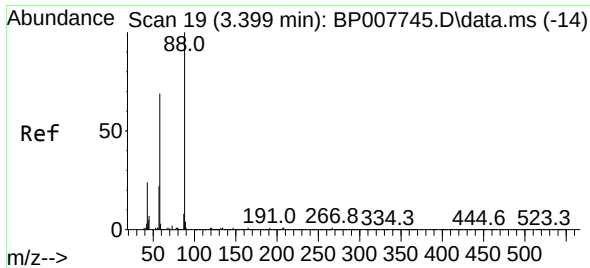

#2
 1,4-Dioxane
 Concen: 92.980 ng/uL
 RT: 3.399 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BP007760.D
 Acq: 28 Oct 2021 19:01

Instrument :
 BNA_P
 ClientSampleId :
 BFYA0

Tgt Ion: 88 Resp: 302483
 Ion Ratio Lower Upper
 88 100
 43 25.7 24.2 36.2
 58 70.2 62.5 93.7

