

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007746.D
 Acq On : 28 Oct 2021 10:59
 Operator : CG/JU
 Sample : PB140114BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	20	rVB	43822	56460	1.09%	0.107%
2	3.781	80	84	99	rBV	644505	978907	18.95%	1.853%
3	4.117	137	141	149	rVB	42364	60858	1.18%	0.115%
4	7.093	641	647	658	rVB	772224	1196564	23.16%	2.265%
5	7.258	669	675	685	rVB	576616	918170	17.77%	1.738%
6	7.464	703	710	718	rVB	755480	1227611	23.76%	2.324%
7	7.928	781	789	802	rBV	692039	1116907	21.62%	2.115%
8	8.634	902	909	920	rBV	944982	1544212	29.89%	2.924%
9	9.087	977	986	995	rBV	710709	1162918	22.51%	2.202%
10	9.811	1101	1109	1119	rBV	606125	996520	19.29%	1.887%
11	10.352	1189	1201	1212	rBV	943797	1609497	31.15%	3.047%
12	10.734	1258	1266	1275	rVB	996936	1676133	32.44%	3.173%
13	10.869	1281	1289	1298	rBV	904816	1593505	30.85%	3.017%
14	12.322	1532	1536	1544	rVB2	18241	30930	0.60%	0.059%
15	13.304	1701	1703	1709	rVB7	4107	5941	0.11%	0.011%
16	13.540	1734	1743	1749	rBV10	6276	16785	0.32%	0.032%
17	13.975	1811	1817	1830	rBV	1726192	2451905	47.46%	4.642%
18	14.257	1857	1865	1875	rBV	1933143	2924431	56.61%	5.537%
19	14.569	1911	1918	1926	rBV	1634124	2432313	47.08%	4.605%
20	14.757	1943	1950	1962	rBV	813978	1190144	23.04%	2.253%
21	14.987	1986	1989	1995	rVB8	3621	5362	0.10%	0.010%
22	15.563	2080	2087	2100	rBV	2621853	3709078	71.80%	7.022%
23	15.675	2100	2106	2121	rVV	665749	993609	19.23%	1.881%
24	15.804	2122	2128	2136	rVB2	33019	57659	1.12%	0.109%
25	16.134	2177	2184	2186	rBV8	3725	7581	0.15%	0.014%
26	16.240	2198	2202	2210	rBV8	6871	15463	0.30%	0.029%
27	16.345	2215	2220	2221	rBV5	4299	5917	0.11%	0.011%
28	16.998	2326	2331	2338	rBV10	6099	13748	0.27%	0.026%
29	17.110	2345	2350	2354	rVB3	11266	17457	0.34%	0.033%
30	17.322	2379	2386	2396	rBV	2078802	2978967	57.66%	5.640%
31	17.422	2396	2403	2415	rBV2	2922830	4191718	81.14%	7.936%
32	17.704	2447	2451	2452	rBV3	5127	6018	0.12%	0.011%
33	18.063	2509	2512	2517	rVB7	4944	6579	0.13%	0.012%
34	18.234	2536	2541	2546	rBV9	5846	16702	0.32%	0.032%
35	19.234	2707	2711	2717	rBV2	42849	64226	1.24%	0.122%
36	19.304	2719	2723	2728	rVB	43924	55301	1.07%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007746.D
Acq On : 28 Oct 2021 10:59
Operator : CG/JU
Sample : PB140114BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK114

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Title : SVOA CALIBRATION

37	19.657	2777	2783	2789	rBV	3830898	5010269	96.98%	9.486%
38	21.416	3077	3082	3096	rVB	2651879	3607746	69.83%	6.831%
39	23.704	3463	3471	3479	rBV2	2543519	5166102	100.00%	9.781%
40	23.857	3491	3497	3508	rVB2	1740007	3697225	71.57%	7.000%




Sum of corrected areas: 52817438

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007746.D
Acq On : 28 Oct 2021 10:59
Operator : CG/JU
Sample : PB140114BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK114

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

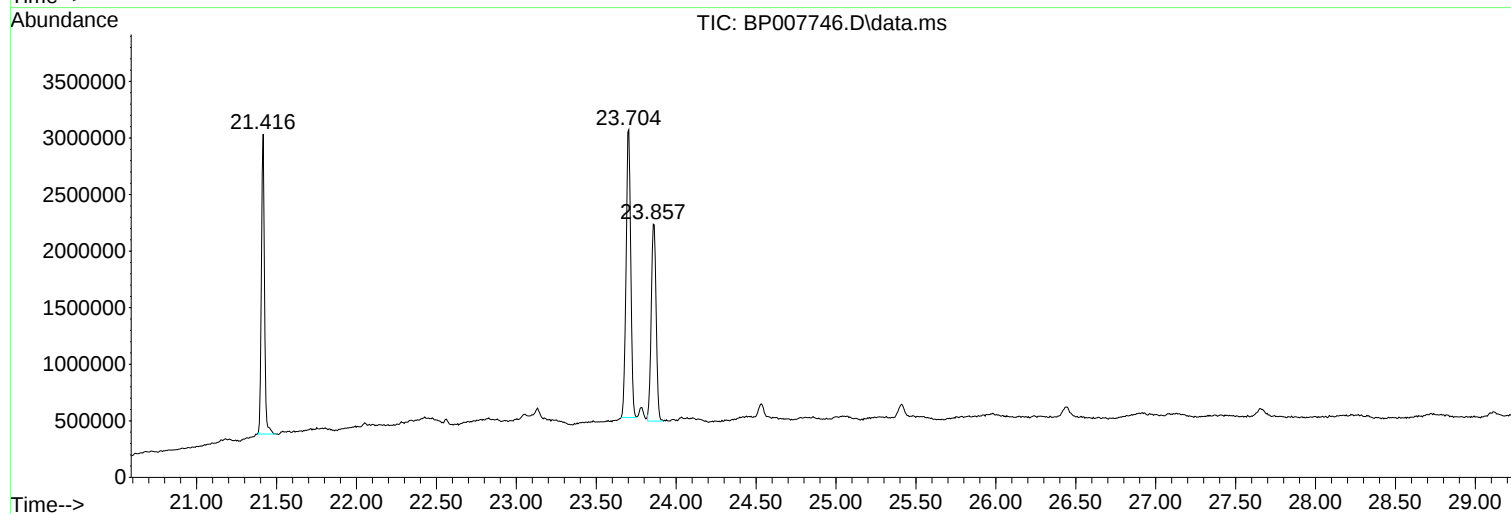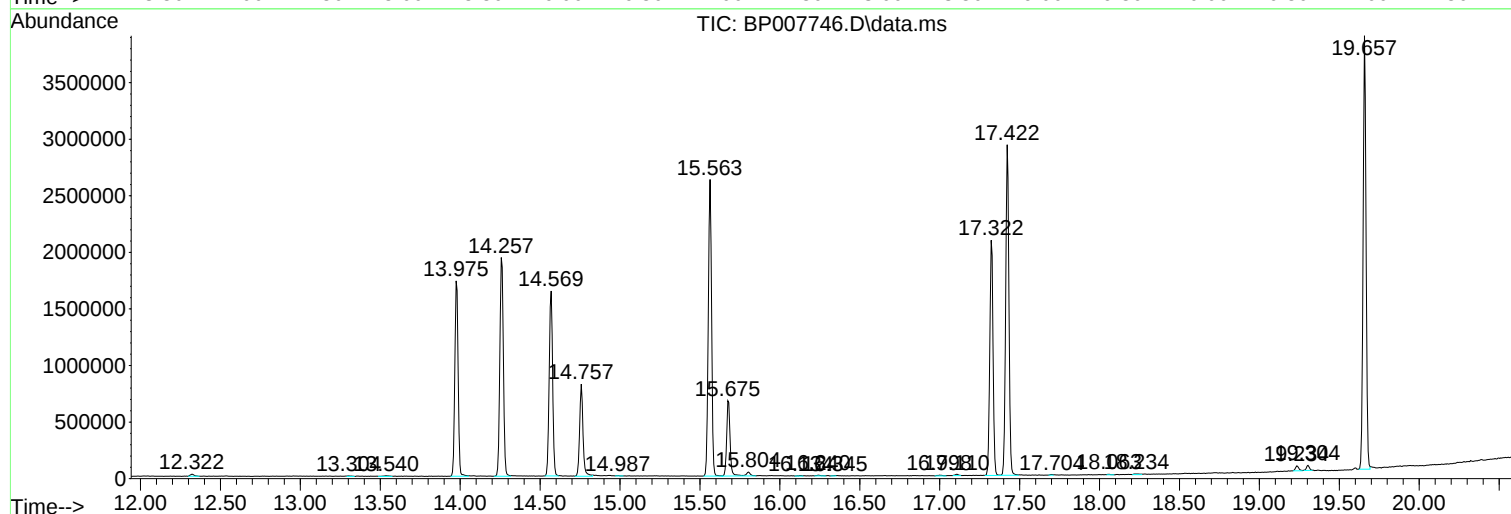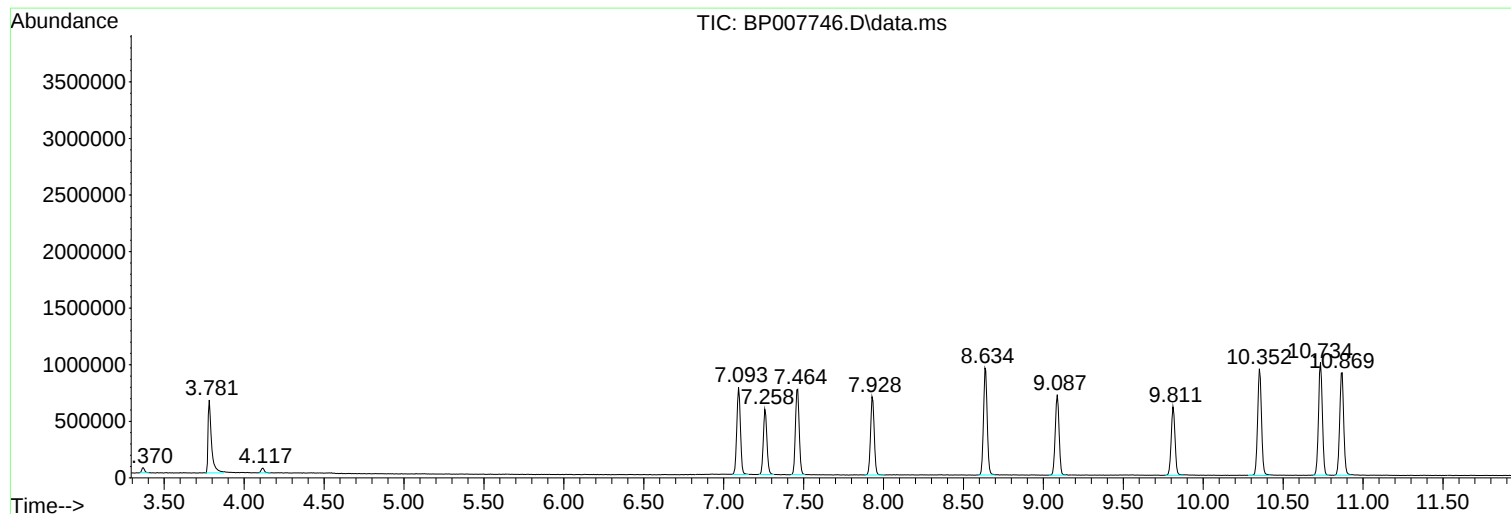

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007746.D
Acq On : 28 Oct 2021 10:59
Operator : CG/JU
Sample : PB140114BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK114

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007746.D
Acq On : 28 Oct 2021 10:59
Operator : CG/JU
Sample : PB140114BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK114

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------