

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007757.D
 Acq On : 28 Oct 2021 17:19
 Operator : CG/JU
 Sample : M4282-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	18	rBV	43528	52814	0.82%	0.098%
2	3.640	58	60	67	rBV5	5705	10447	0.16%	0.019%
3	3.781	82	84	98	rBV	156905	240835	3.74%	0.446%
4	4.022	120	125	130	rVB	27327	43194	0.67%	0.080%
5	4.111	136	140	147	rVB3	12607	19379	0.30%	0.036%
6	4.211	153	157	161	rVB5	12360	17191	0.27%	0.032%
7	5.040	291	298	303	rBV4	9347	15550	0.24%	0.029%
8	6.311	507	514	520	rBV5	9537	17627	0.27%	0.033%
9	6.928	615	619	623	rBV7	4539	9429	0.15%	0.017%
10	7.093	639	647	656	rVB	347439	538579	8.36%	0.997%
11	7.258	668	675	689	rVB	689697	1081585	16.80%	2.003%
12	7.463	702	710	721	rBV	765438	1240052	19.26%	2.296%
13	7.928	782	789	797	rBV	630146	991433	15.40%	1.836%
14	8.005	799	802	805	rVB5	6049	7246	0.11%	0.013%
15	8.175	825	831	833	rBV7	3890	6931	0.11%	0.013%
16	8.640	902	910	918	rBV	713894	1166857	18.12%	2.160%
17	9.087	978	986	998	rBV	838516	1379216	21.42%	2.554%
18	9.552	1059	1065	1068	rVB7	6748	10965	0.17%	0.020%
19	9.810	1099	1109	1124	rBV	692839	1146121	17.80%	2.122%
20	10.351	1194	1201	1213	rBV	1065256	1777015	27.59%	3.290%
21	10.516	1224	1229	1238	rBV	75277	125412	1.95%	0.232%
22	10.734	1256	1266	1274	rBV	867415	1467936	22.80%	2.718%
23	10.869	1280	1289	1304	rBV	902365	1597490	24.81%	2.958%
24	12.040	1483	1488	1493	rBV8	3896	7971	0.12%	0.015%
25	12.322	1530	1536	1545	rVB2	18228	32423	0.50%	0.060%
26	12.934	1635	1640	1645	rBV8	3403	6901	0.11%	0.013%
27	13.187	1677	1683	1687	rBV7	6307	9909	0.15%	0.018%
28	13.540	1737	1743	1748	rBV9	4858	8561	0.13%	0.016%
29	13.975	1810	1817	1833	rBV	1978386	2792147	43.36%	5.170%
30	14.257	1854	1865	1878	rBV	2224145	3342991	51.91%	6.189%
31	14.569	1907	1918	1930	rBV	1357883	2067928	32.11%	3.829%
32	14.757	1941	1950	1962	rBV	320025	501607	7.79%	0.929%
33	14.987	1984	1989	1992	rBV7	6253	8665	0.13%	0.016%
34	15.381	2053	2056	2063	rBV7	6583	13173	0.20%	0.024%
35	15.563	2079	2087	2099	rBV	2887855	4231870	65.72%	7.835%
36	15.675	2100	2106	2118	rVV	863580	1171285	18.19%	2.169%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007757.D
 Acq On : 28 Oct 2021 17:19
 Operator : CG/JU
 Sample : M4282-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.804	2121	2128	2135	rVB	36588	61786	0.96%	0.114%
38	16.239	2198	2202	2208	rBV9	7967	17917	0.28%	0.033%
39	16.575	2254	2259	2264	rBV9	5003	9908	0.15%	0.018%
40	17.098	2343	2348	2353	rBV5	11556	25148	0.39%	0.047%
41	17.322	2379	2386	2396	rVV	1825227	2554877	39.67%	4.730%
42	17.422	2396	2403	2414	rBV2	3307850	4833869	75.06%	8.950%
43	17.698	2447	2450	2455	rBV6	6360	8294	0.13%	0.015%
44	18.004	2497	2502	2506	rVB3	21196	27731	0.43%	0.051%
45	18.216	2534	2538	2543	rBV4	50833	71302	1.11%	0.132%
46	18.280	2547	2549	2555	rVB2	11305	15208	0.24%	0.028%
47	19.233	2707	2711	2716	rBV3	49120	62866	0.98%	0.116%
48	19.304	2719	2723	2726	rBV	39062	49840	0.77%	0.092%
49	19.451	2745	2748	2753	rBV7	13721	16860	0.26%	0.031%
50	19.592	2770	2772	2776	rBV3	17293	20688	0.32%	0.038%
51	19.657	2777	2783	2789	rBV	4539013	5934110	92.15%	10.987%
52	21.127	3030	3033	3039	rBV	96423	137844	2.14%	0.255%
53	21.416	3076	3082	3092	rBV	2324785	3227664	50.12%	5.976%
54	23.698	3462	3470	3479	rBV2	3286458	6439672	100.00%	11.923%
55	23.857	3490	3497	3507	rVB2	1624312	3337346	51.82%	6.179%




Sum of corrected areas: 54011665

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007757.D
Acq On : 28 Oct 2021 17:19
Operator : CG/JU
Sample : M4282-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY82

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

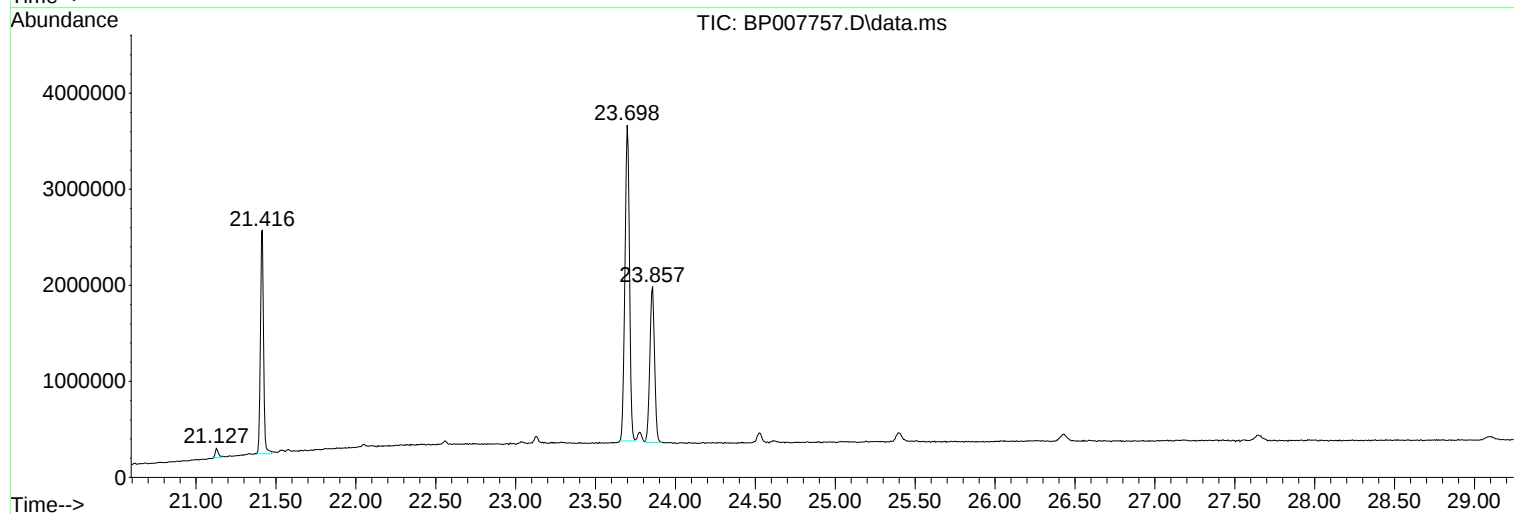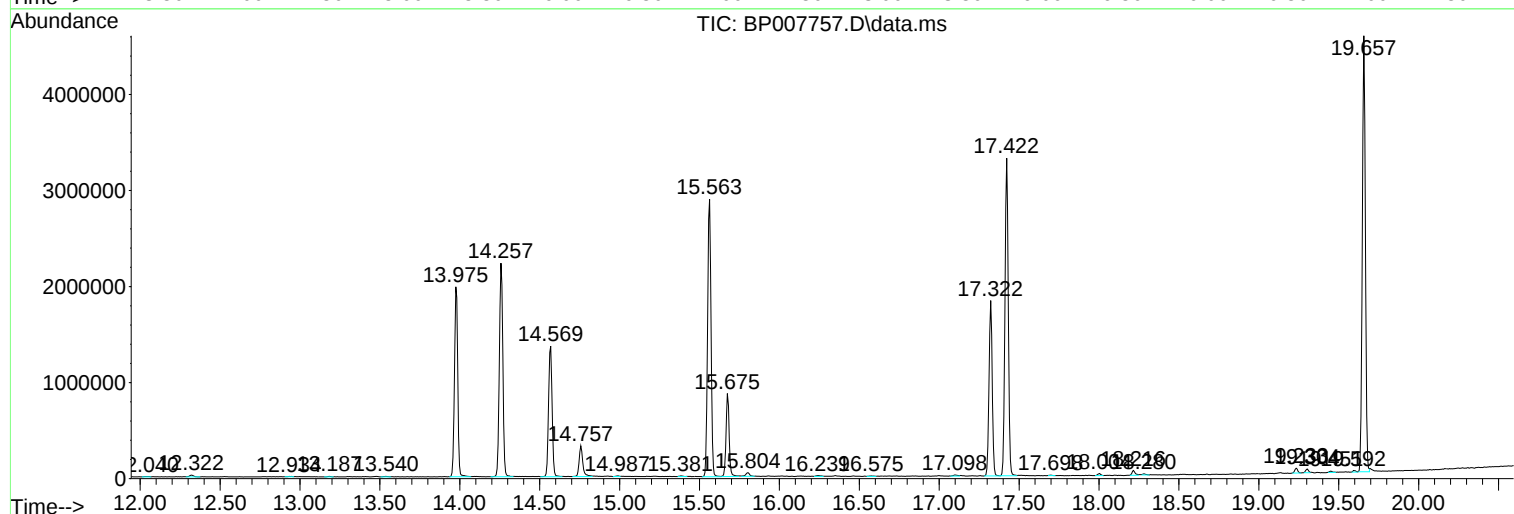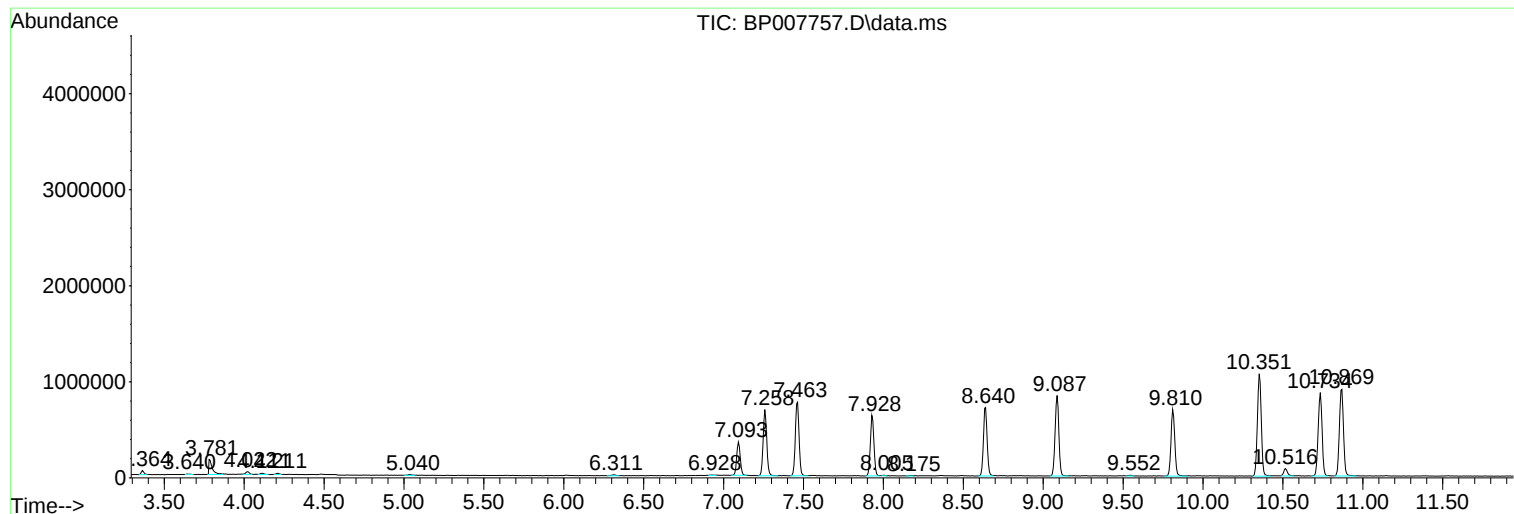

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007757.D
Acq On : 28 Oct 2021 17:19
Operator : CG/JU
Sample : M4282-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY82

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007757.D
Acq On : 28 Oct 2021 17:19
Operator : CG/JU
Sample : M4282-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY82

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
