

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007758.D
 Acq On : 28 Oct 2021 17:53
 Operator : CG/JU
 Sample : M4282-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	17	rBV	33372	42640	0.67%	0.083%
2	3.787	82	85	97	rBV	85823	137340	2.17%	0.268%
3	4.022	121	125	129	rVB2	21385	28806	0.45%	0.056%
4	4.111	137	140	145	rVB	10522	14567	0.23%	0.028%
5	4.211	153	157	162	rBV6	8429	11944	0.19%	0.023%
6	5.040	294	298	302	rVB7	7498	9514	0.15%	0.019%
7	6.311	511	514	519	rVB5	8818	12362	0.20%	0.024%
8	7.093	641	647	657	rVB	253422	396472	6.26%	0.774%
9	7.258	667	675	688	rBV	612265	958660	15.14%	1.873%
10	7.458	703	709	717	rBV	646121	1032396	16.31%	2.017%
11	7.928	782	789	797	rBV	633895	1019451	16.10%	1.991%
12	7.999	799	801	806	rVB6	4857	7155	0.11%	0.014%
13	8.640	902	910	919	rBV	547766	886548	14.00%	1.732%
14	9.087	978	986	997	rBV	748893	1212043	19.14%	2.368%
15	9.534	1059	1062	1068	rVB7	6181	12023	0.19%	0.023%
16	9.810	1100	1109	1117	rBV	601790	991852	15.66%	1.937%
17	10.352	1193	1201	1212	rBV	943749	1548057	24.45%	3.024%
18	10.516	1223	1229	1241	rBV	58012	101338	1.60%	0.198%
19	10.734	1257	1266	1277	rVB	879408	1480489	23.38%	2.892%
20	10.863	1279	1288	1306	rBV	780780	1373604	21.69%	2.683%
21	11.540	1398	1403	1406	rBV6	2862	6572	0.10%	0.013%
22	12.040	1484	1488	1495	rVB2	14190	21355	0.34%	0.042%
23	12.257	1519	1525	1531	rBV2	36819	61272	0.97%	0.120%
24	12.322	1531	1536	1540	rVV2	13660	22929	0.36%	0.045%
25	13.534	1737	1742	1748	rBV10	6297	11694	0.18%	0.023%
26	13.975	1809	1817	1823	rBV	1843764	2511232	39.66%	4.905%
27	14.257	1855	1865	1882	rBV	2064772	3020504	47.70%	5.900%
28	14.569	1907	1918	1930	rBV	1361975	2078352	32.82%	4.060%
29	14.757	1941	1950	1963	rBV	211178	352455	5.57%	0.688%
30	14.987	1985	1989	1993	rBV5	8882	12633	0.20%	0.025%
31	15.222	2023	2029	2033	rBV8	4499	8988	0.14%	0.018%
32	15.387	2053	2057	2062	rBV5	4945	9543	0.15%	0.019%
33	15.563	2079	2087	2096	rBV	2703063	3881455	61.30%	7.582%
34	15.675	2100	2106	2115	rBV	736305	1054529	16.65%	2.060%
35	15.804	2124	2128	2132	rVB	32822	44264	0.70%	0.086%
36	15.934	2144	2150	2155	rBV10	4565	7689	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007758.D
 Acq On : 28 Oct 2021 17:53
 Operator : CG/JU
 Sample : M4282-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.134	2179	2184	2189	rBV8	4582	8049	0.13%	0.016%
38	16.257	2198	2205	2209	rBV4	13950	27371	0.43%	0.053%
39	16.322	2213	2216	2219	rBV3	7233	8948	0.14%	0.017%
40	16.998	2329	2331	2338	rVB8	6976	7536	0.12%	0.015%
41	17.110	2345	2350	2352	rBV2	7788	12498	0.20%	0.024%
42	17.145	2352	2356	2362	rVB7	9682	17334	0.27%	0.034%
43	17.322	2379	2386	2395	rBV	1843780	2564891	40.51%	5.010%
44	17.422	2396	2403	2414	rBV	3275554	4602462	72.69%	8.990%
45	17.698	2446	2450	2455	rBV6	9775	13632	0.22%	0.027%
46	17.998	2498	2501	2506	rVB4	14064	17653	0.28%	0.034%
47	18.216	2533	2538	2546	rBV3	89581	135561	2.14%	0.265%
48	18.528	2587	2591	2596	rBV6	6152	13885	0.22%	0.027%
49	19.233	2707	2711	2717	rBV3	48269	67590	1.07%	0.132%
50	19.304	2719	2723	2728	rVV	40879	57387	0.91%	0.112%
51	19.451	2744	2748	2753	rBV4	32251	45912	0.73%	0.090%
52	19.657	2777	2783	2789	rBV	4363440	5683821	89.77%	11.102%
53	21.127	3030	3033	3038	rBV2	111231	153733	2.43%	0.300%
54	21.416	3076	3082	3092	rBV	2467279	3372202	53.26%	6.587%
55	22.704	3298	3301	3307	rVB	124915	169538	2.68%	0.331%
56	23.704	3463	3471	3479	rVB	3160242	6331728	100.00%	12.368%
57	23.857	3490	3497	3506	rVB	1651096	3500370	55.28%	6.837%




Sum of corrected areas: 51194828

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007758.D
Acq On : 28 Oct 2021 17:53
Operator : CG/JU
Sample : M4282-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

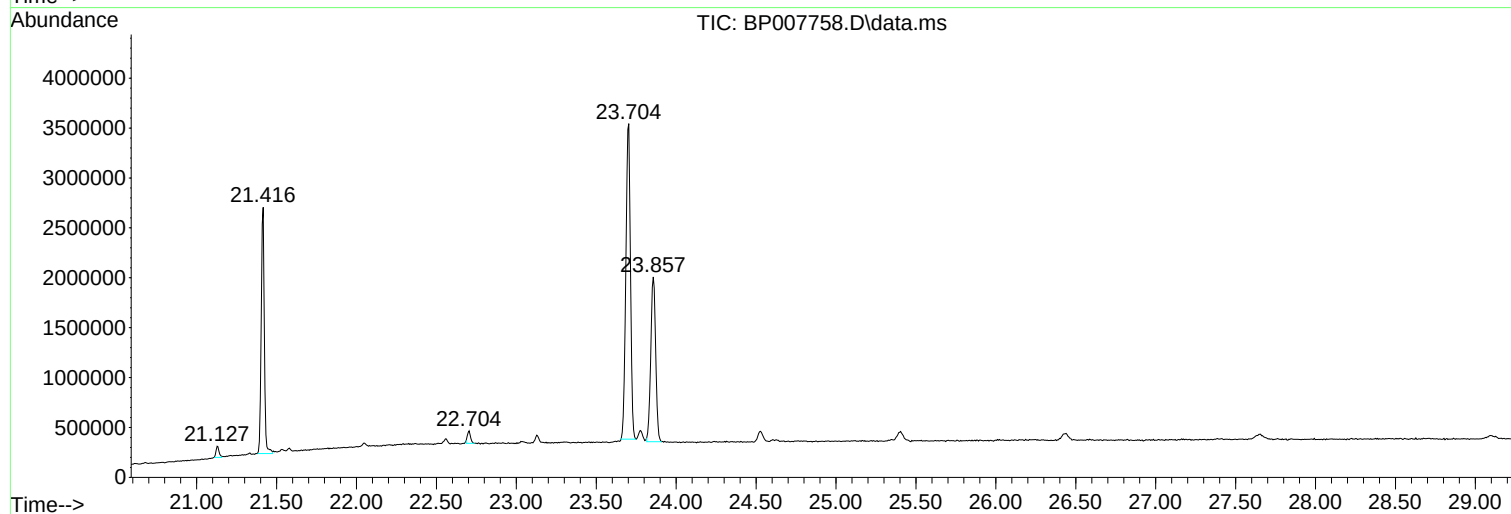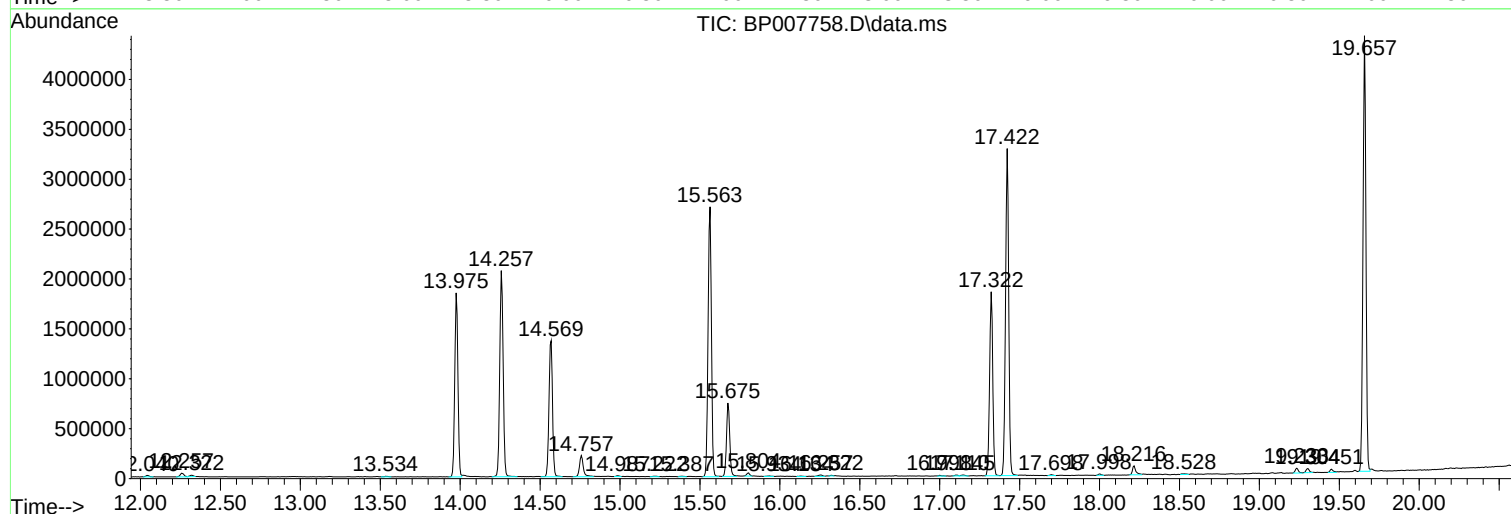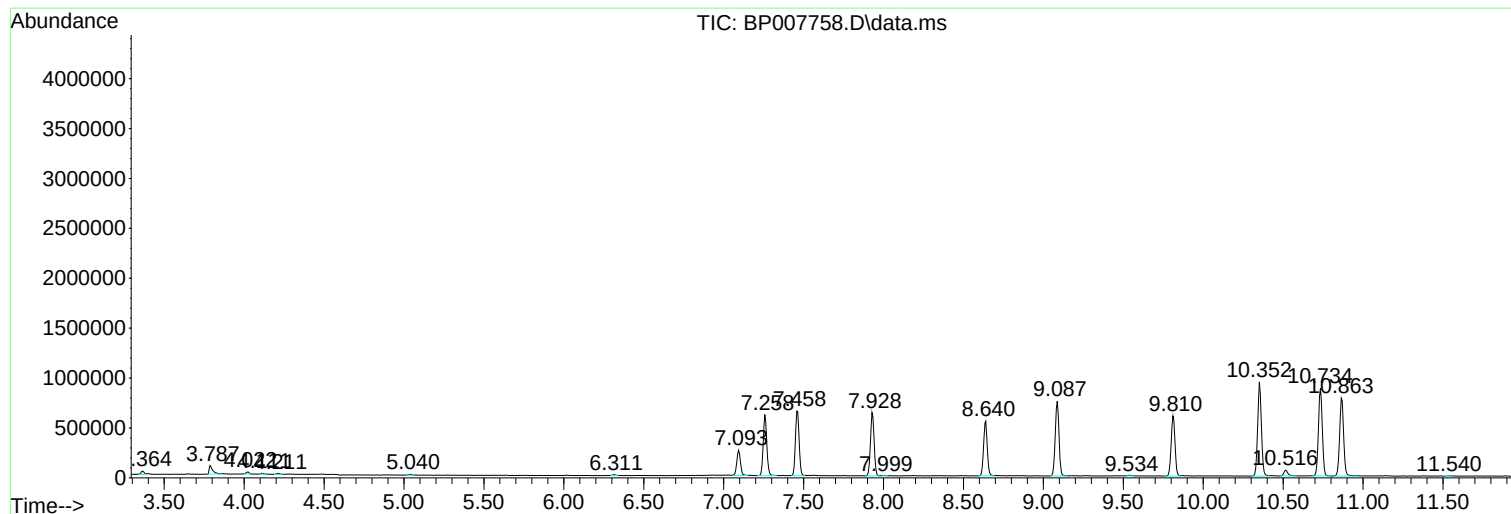

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007758.D
Acq On : 28 Oct 2021 17:53
Operator : CG/JU
Sample : M4282-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007758.D
Acq On : 28 Oct 2021 17:53
Operator : CG/JU
Sample : M4282-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
