

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007763.D
 Acq On : 28 Oct 2021 21:17
 Operator : CG/JU
 Sample : PB140115BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK115

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	20	rBV	46649	62933	1.22%	0.131%
2	3.781	80	84	103	rBV	604584	969353	18.74%	2.016%
3	4.111	137	140	148	rVB	31676	43863	0.85%	0.091%
4	7.093	640	647	658	rVB	744529	1170853	22.63%	2.435%
5	7.258	668	675	687	rVB	580438	897746	17.35%	1.867%
6	7.458	702	709	719	rBV	762568	1210471	23.40%	2.518%
7	7.928	781	789	802	rBV	610933	957574	18.51%	1.992%
8	8.634	899	909	920	rBV	915934	1484142	28.69%	3.087%
9	9.087	977	986	999	rBV	693449	1127422	21.79%	2.345%
10	9.810	1102	1109	1118	rBV	580952	949917	18.36%	1.976%
11	10.352	1191	1201	1214	rBV	912958	1546887	29.90%	3.218%
12	10.734	1259	1266	1275	rVB	819642	1373946	26.56%	2.858%
13	10.863	1280	1288	1303	rBV	885256	1509793	29.19%	3.141%
14	12.322	1529	1536	1543	rBV2	18363	32785	0.63%	0.068%
15	13.534	1738	1742	1746	rVB5	3356	5406	0.10%	0.011%
16	13.975	1809	1817	1827	rBV	1664170	2278328	44.04%	4.739%
17	14.257	1858	1865	1876	rBV	1836820	2654284	51.31%	5.521%
18	14.563	1908	1917	1930	rVB	1279705	1941122	37.52%	4.038%
19	14.757	1943	1950	1969	rBV	762361	1147446	22.18%	2.387%
20	14.922	1975	1978	1982	rVB6	3401	5579	0.11%	0.012%
21	15.228	2025	2030	2036	rVB9	4937	10513	0.20%	0.022%
22	15.557	2079	2086	2100	rBV	2319076	3403693	65.80%	7.080%
23	15.675	2100	2106	2120	rVV	602031	838739	16.21%	1.745%
24	15.798	2123	2127	2133	rVB	31442	43682	0.84%	0.091%
25	16.845	2300	2305	2308	rBV6	3633	6077	0.12%	0.013%
26	16.998	2328	2331	2335	rVB6	4837	7073	0.14%	0.015%
27	17.104	2344	2349	2353	rBV3	7950	12428	0.24%	0.026%
28	17.322	2379	2386	2395	rBV	1664067	2411264	46.61%	5.016%
29	17.422	2396	2403	2416	rVV	2683525	3836524	74.17%	7.980%
30	17.698	2445	2450	2454	rBV6	4451	7577	0.15%	0.016%
31	17.998	2498	2501	2506	rVB7	3825	6462	0.12%	0.013%
32	19.233	2707	2711	2718	rVB2	36237	47295	0.91%	0.098%
33	19.298	2718	2722	2726	rBV	40588	54448	1.05%	0.113%
34	19.592	2770	2772	2776	rBV5	9478	8981	0.17%	0.019%
35	19.657	2777	2783	2793	rVV	3294239	4664442	90.17%	9.703%
36	21.410	3076	3081	3089	rBV	2288593	3006635	58.12%	6.254%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007763.D
Acq On : 28 Oct 2021 21:17
Operator : CG/JU
Sample : PB140115BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK115

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Title : SVOA CALIBRATION

37	23.692	3461	3469	3477	rBV2	2558671	5172883	100.00%	10.760%
38	23.851	3489	3496	3505	rVB	1521650	3165921	61.20%	6.585%




Sum of corrected areas: 48074487

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007763.D
Acq On : 28 Oct 2021 21:17
Operator : CG/JU
Sample : PB140115BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK115

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

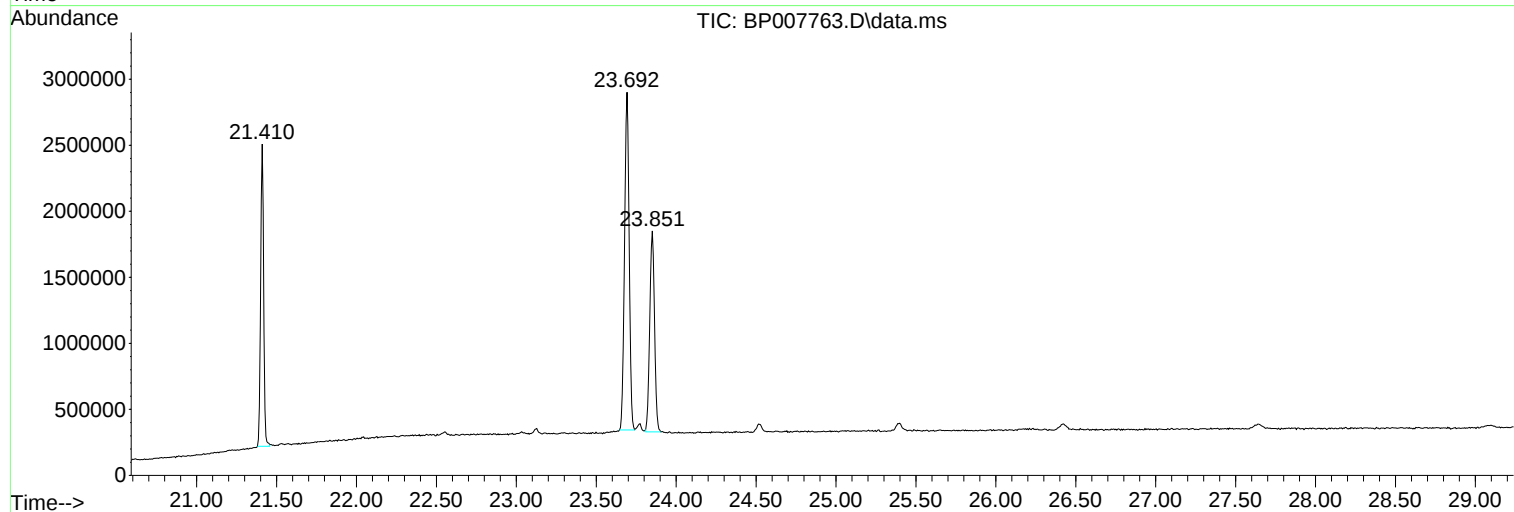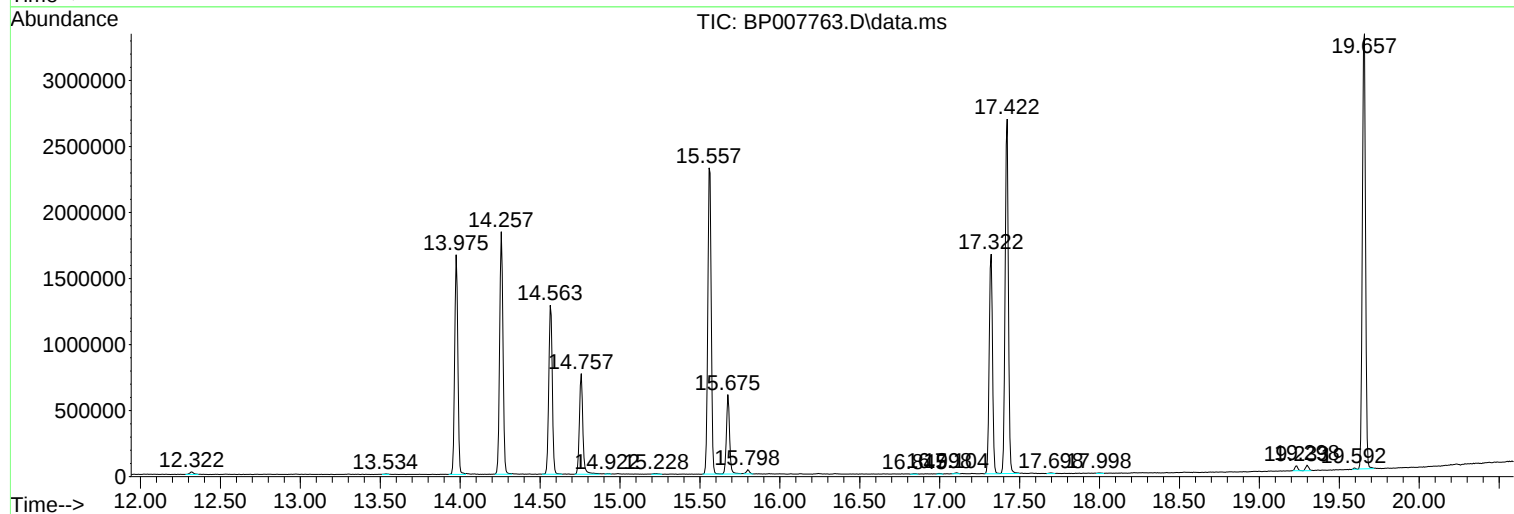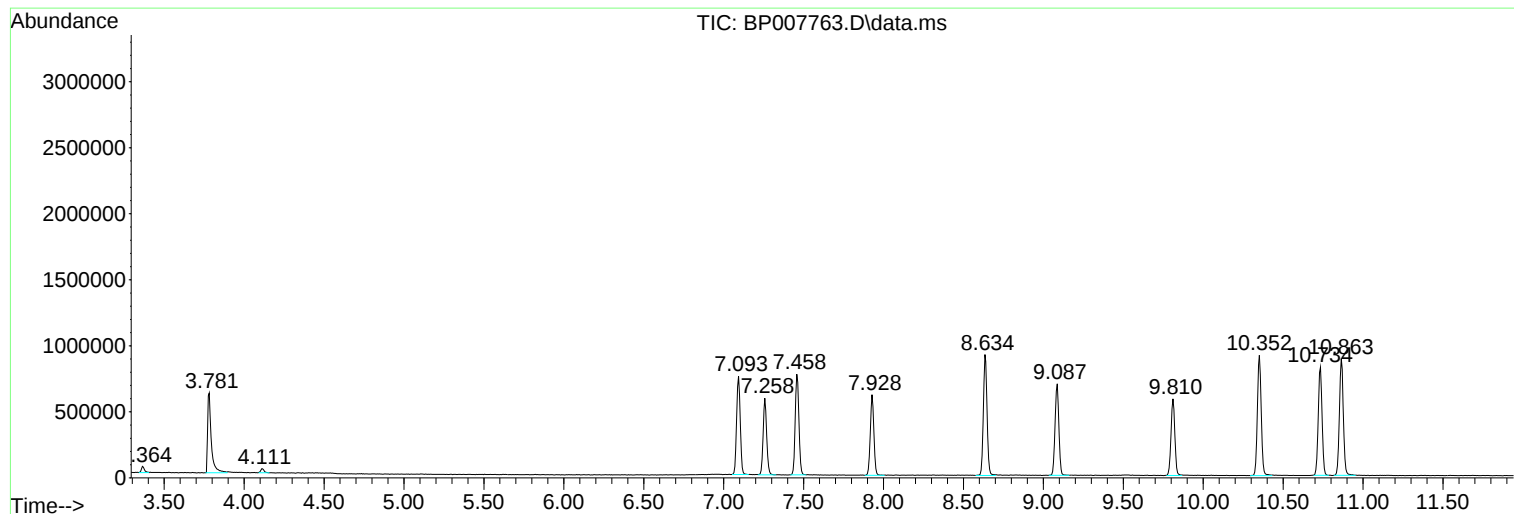

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007763.D
Acq On : 28 Oct 2021 21:17
Operator : CG/JU
Sample : PB140115BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK115

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007763.D
Acq On : 28 Oct 2021 21:17
Operator : CG/JU
Sample : PB140115BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK115

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
