

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007765.D
 Acq On : 28 Oct 2021 22:24
 Operator : CG/JU
 Sample : M4262-07DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY91DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	15	19	28	rVB	86709	109964	2.92%	0.490%
2	3.799	85	87	94	rBV	28033	42781	1.14%	0.191%
3	4.117	137	141	146	rVB2	10427	16571	0.44%	0.074%
4	7.093	641	647	658	rVB	36030	68965	1.83%	0.308%
5	7.175	659	661	668	rVV8	2826	4264	0.11%	0.019%
6	7.258	669	675	685	rVV	118825	193211	5.14%	0.862%
7	7.458	703	709	718	rBV	122174	194720	5.18%	0.868%
8	7.569	726	728	736	rVB8	2341	3960	0.11%	0.018%
9	7.928	781	789	796	rBV	687657	1088611	28.94%	4.855%
10	8.181	827	832	837	rVB8	2592	5383	0.14%	0.024%
11	8.634	902	909	916	rBV	89545	153016	4.07%	0.682%
12	8.834	937	943	946	rVB6	3508	5861	0.16%	0.026%
13	9.087	979	986	993	rBV	128199	214586	5.71%	0.957%
14	9.528	1060	1061	1068	rVB7	3660	6590	0.18%	0.029%
15	9.810	1102	1109	1117	rBV	96890	164647	4.38%	0.734%
16	10.352	1194	1201	1210	rBV	163021	278885	7.41%	1.244%
17	10.516	1222	1229	1240	rBV	66033	129231	3.44%	0.576%
18	10.728	1257	1265	1276	rBV	916996	1581730	42.05%	7.054%
19	10.863	1281	1288	1297	rBV	139094	243333	6.47%	1.085%
20	11.381	1372	1376	1382	rVB9	2184	4079	0.11%	0.018%
21	12.034	1485	1487	1494	rVB7	3637	6660	0.18%	0.030%
22	12.322	1531	1536	1542	rVB8	4291	8309	0.22%	0.037%
23	13.887	1797	1802	1807	rBV8	2087	4565	0.12%	0.020%
24	13.975	1810	1817	1829	rBV	373572	519051	13.80%	2.315%
25	14.257	1855	1865	1873	rBV	366773	540198	14.36%	2.409%
26	14.563	1910	1917	1926	rBV	1513355	2242593	59.63%	10.002%
27	14.763	1946	1951	1960	rBV3	21403	36927	0.98%	0.165%
28	15.557	2079	2086	2095	rVV	556586	806983	21.46%	3.599%
29	15.675	2100	2106	2113	rBV	81406	127750	3.40%	0.570%
30	15.798	2119	2127	2130	rBV8	6438	11109	0.30%	0.050%
31	15.998	2153	2161	2170	rBV8	3413	11736	0.31%	0.052%
32	16.122	2179	2182	2187	rBV7	2074	3836	0.10%	0.017%
33	16.251	2202	2204	2209	rVB6	2797	3906	0.10%	0.017%
34	16.775	2290	2293	2296	rBV5	2254	4003	0.11%	0.018%
35	16.987	2324	2329	2331	rBV6	3290	4948	0.13%	0.022%
36	17.104	2342	2349	2352	rBV2	8278	12193	0.32%	0.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007765.D
 Acq On : 28 Oct 2021 22:24
 Operator : CG/JU
 Sample : M4262-07DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY91DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.316	2379	2385	2396	rBV	1906762	2759526	73.37%	12.307%
38	17.416	2396	2402	2414	rVV	652666	955075	25.39%	4.259%
39	17.998	2498	2501	2505	rVB3	18397	20439	0.54%	0.091%
40	18.210	2533	2537	2543	rBV7	10845	18965	0.50%	0.085%
41	18.516	2587	2589	2591	rBV3	4722	5147	0.14%	0.023%
42	19.134	2691	2694	2698	rVB5	12630	14429	0.38%	0.064%
43	19.592	2769	2772	2776	rBV5	14195	17680	0.47%	0.079%
44	19.651	2777	2782	2788	rBV	935934	1189315	31.62%	5.304%
45	21.410	3075	3081	3095	rBV	2676685	3557270	94.58%	15.865%
46	23.686	3462	3468	3475	rVB2	625019	1268439	33.72%	5.657%
47	23.851	3488	3496	3507	rVB2	1765556	3761125	100.00%	16.774%




Sum of corrected areas: 22422565

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007765.D
Acq On : 28 Oct 2021 22:24
Operator : CG/JU
Sample : M4262-07DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY91DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

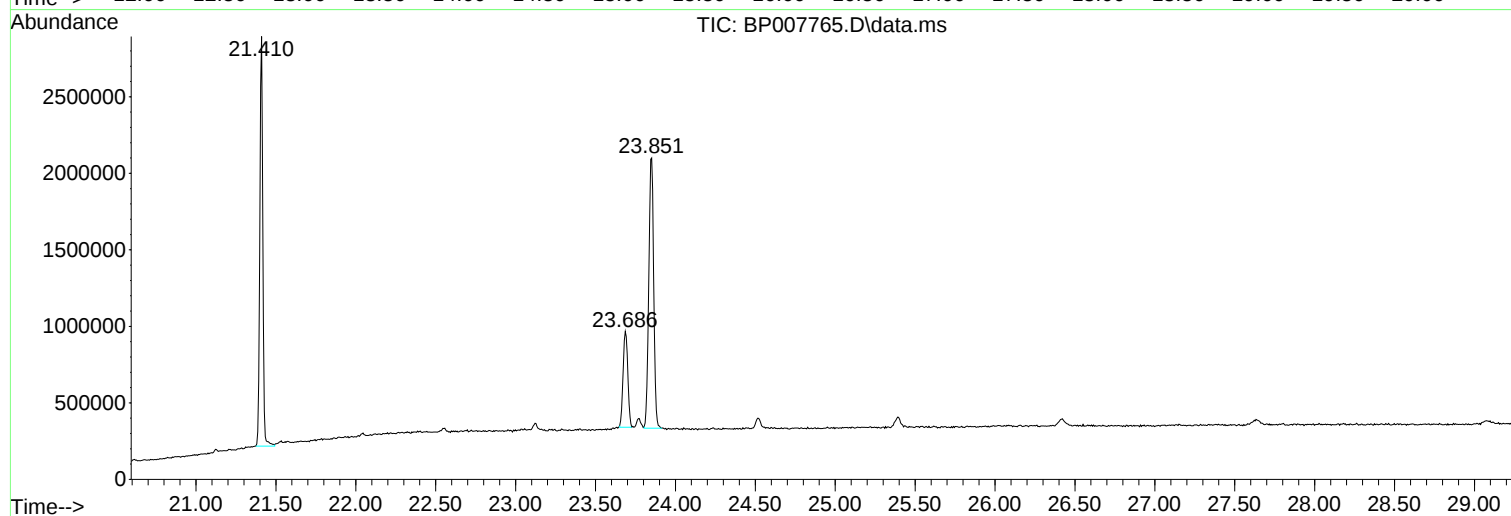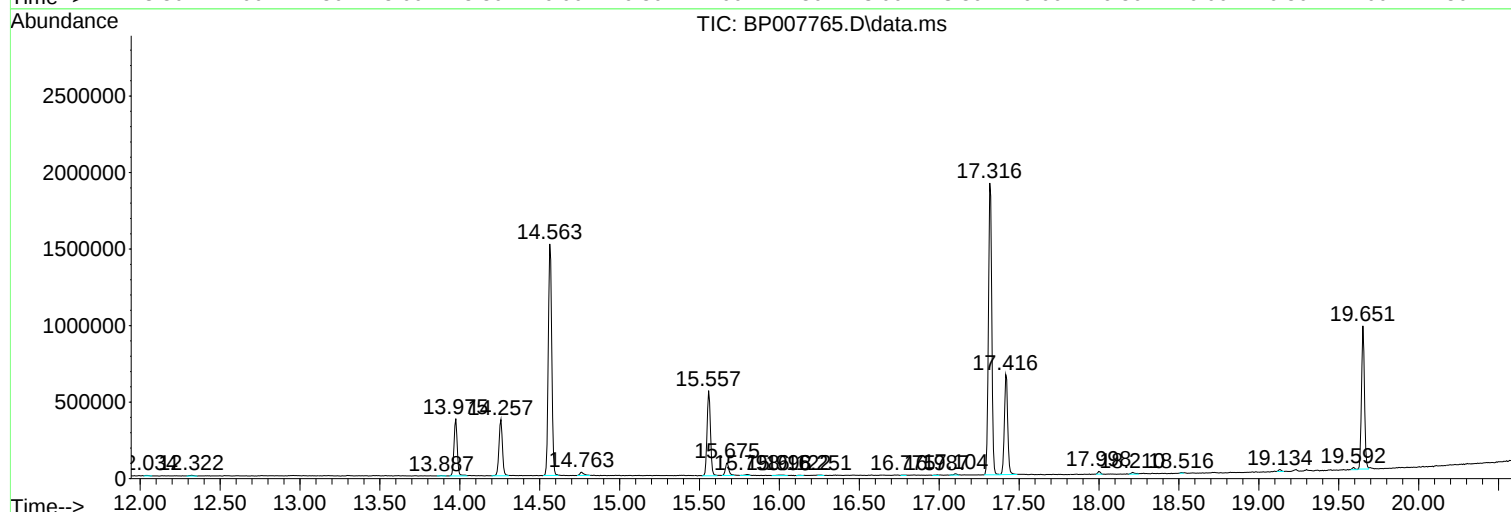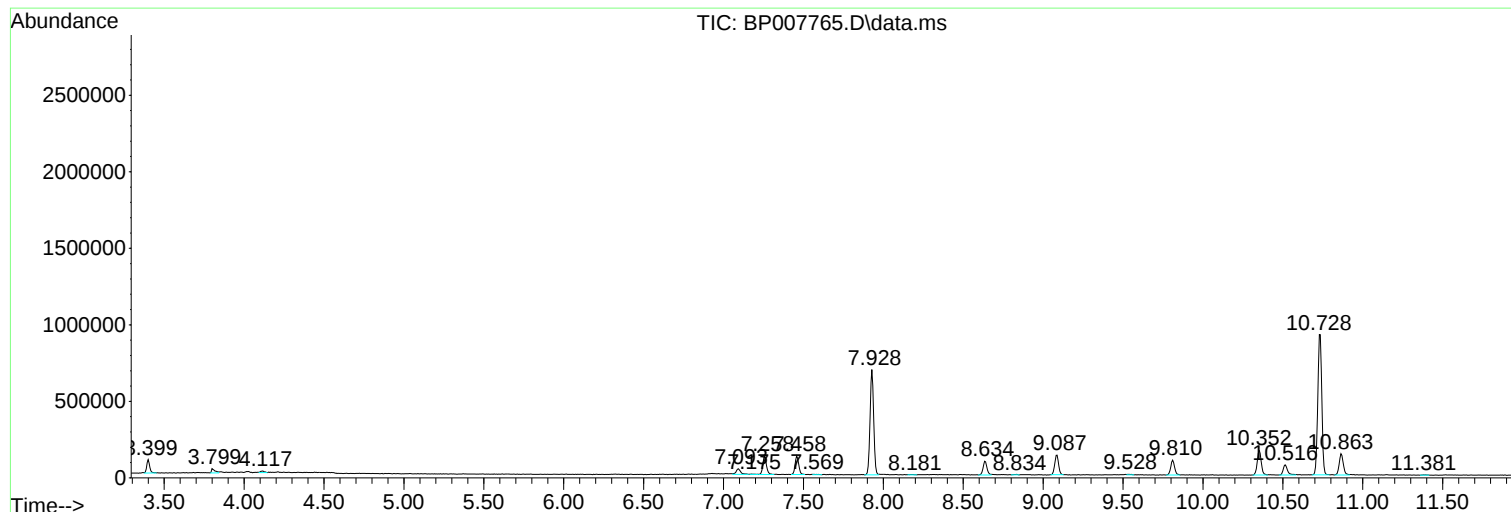

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007765.D
Acq On : 28 Oct 2021 22:24
Operator : CG/JU
Sample : M4262-07DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY91DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007765.D
Acq On : 28 Oct 2021 22:24
Operator : CG/JU
Sample : M4262-07DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY91DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
